

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018894.D
 Acq On : 15 Dec 2023 23:27
 Operator : MA/JU
 Sample : 05627-17DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	27	29	35	rVB2	11405	15526	0.39%	0.052%
2	3.687	99	102	110	rBV	35456	60447	1.52%	0.201%
3	4.005	153	156	163	rVB	18621	25364	0.64%	0.084%
4	4.864	300	302	307	rBV6	2286	4388	0.11%	0.015%
5	5.334	378	382	389	rVB2	15883	23173	0.58%	0.077%
6	5.464	399	404	413	rBV	31572	72631	1.82%	0.242%
7	5.528	413	415	418	rVB3	3868	4099	0.10%	0.014%
8	5.834	462	467	473	rBV	24210	39489	0.99%	0.131%
9	6.911	648	650	655	rVB5	6706	9104	0.23%	0.030%
10	6.999	661	665	677	rVB	58535	104532	2.62%	0.348%
11	7.163	687	693	701	rBV	228980	357805	8.98%	1.191%
12	7.358	718	726	734	rBV	212911	342698	8.61%	1.141%
13	7.828	799	806	814	rBV	949192	1490830	37.44%	4.964%
14	7.905	817	819	824	rVB5	8516	11553	0.29%	0.038%
15	8.234	872	875	877	rBV4	3256	4115	0.10%	0.014%
16	8.540	920	927	936	rBV	155071	258299	6.49%	0.860%
17	8.657	944	947	950	rVB5	4314	5838	0.15%	0.019%
18	8.693	950	953	955	rBV3	3594	4511	0.11%	0.015%
19	8.987	996	1003	1013	rBV	218502	357433	8.98%	1.190%
20	9.369	1063	1068	1069	rBV3	6390	7124	0.18%	0.024%
21	9.546	1094	1098	1103	rVB7	3099	5359	0.13%	0.018%
22	9.710	1119	1126	1135	rBV	120113	212611	5.34%	0.708%
23	9.887	1151	1156	1160	rBV8	2679	4741	0.12%	0.016%
24	10.246	1207	1217	1226	rBV	238136	424850	10.67%	1.415%
25	10.622	1274	1281	1291	rVB	1136520	1872774	47.03%	6.236%
26	10.763	1298	1305	1320	rBV	167671	325095	8.16%	1.082%
27	11.240	1382	1386	1387	rBV4	3823	4603	0.12%	0.015%
28	11.275	1387	1392	1393	rBV5	6347	8222	0.21%	0.027%
29	11.893	1494	1497	1502	rVB7	5012	7641	0.19%	0.025%
30	12.210	1548	1551	1557	rVB6	5142	9326	0.23%	0.031%
31	12.404	1578	1584	1589	rBV	24587	44127	1.11%	0.147%
32	12.822	1653	1655	1661	rVB7	3637	6173	0.16%	0.021%
33	13.045	1687	1693	1695	rBV7	2232	4979	0.13%	0.017%
34	13.293	1731	1735	1738	rVB5	3612	4676	0.12%	0.016%
35	13.351	1742	1745	1751	rBV8	9282	16943	0.43%	0.056%
36	13.645	1792	1795	1799	rBV6	3644	4352	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018894.D
 Acq On : 15 Dec 2023 23:27
 Operator : MA/JU
 Sample : 05627-17DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	13.875	1824	1834	1841	rBV	493938	682018	17.13%	2.271%
38	13.992	1849	1854	1858	rVB7	8546	13121	0.33%	0.044%
39	14.151	1873	1881	1889	rBV	532565	771944	19.38%	2.570%
40	14.457	1926	1933	1943	rBV	1562441	2256161	56.65%	7.512%
41	14.528	1943	1945	1948	rVB4	3984	4452	0.11%	0.015%
42	14.681	1966	1971	1982	rBV5	19487	44655	1.12%	0.149%
43	15.451	2095	2102	2117	rBV	741982	1137819	28.57%	3.788%
44	15.569	2117	2122	2129	rBV2	98862	148238	3.72%	0.494%
45	15.916	2179	2181	2186	rVB6	3403	4359	0.11%	0.015%
46	16.610	2295	2299	2303	rBV7	7604	13042	0.33%	0.043%
47	17.016	2365	2368	2372	rVB2	13507	16984	0.43%	0.057%
48	17.204	2394	2400	2410	rBV	1958268	2775980	69.71%	9.243%
49	17.304	2411	2417	2428	rVV	874165	1243509	31.23%	4.140%
50	17.751	2492	2493	2497	rBV4	6333	6014	0.15%	0.020%
51	17.875	2511	2514	2517	rBV5	6398	7707	0.19%	0.026%
52	18.098	2547	2552	2557	rBV2	87753	121861	3.06%	0.406%
53	18.169	2559	2564	2574	rVV	2791429	3295205	82.75%	10.972%
54	19.116	2723	2725	2731	rVB4	13374	19319	0.49%	0.064%
55	19.192	2735	2738	2739	rBV2	13892	14955	0.38%	0.050%
56	19.333	2759	2762	2766	rVB5	32650	38281	0.96%	0.127%
57	19.480	2784	2787	2791	rVB3	23855	27927	0.70%	0.093%
58	19.539	2792	2797	2804	rBV	1299828	1704804	42.81%	5.676%
59	21.292	3090	3095	3101	rBV	2848534	3664034	92.01%	12.200%
60	23.498	3464	3470	3484	rVB	961504	1883439	47.29%	6.271%
61	23.651	3489	3496	3505	rVB	2065961	3982338	100.00%	13.260%




Sum of corrected areas: 30033597

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018894.D
Acq On : 15 Dec 2023 23:27
Operator : MA/JU
Sample : 05627-17DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

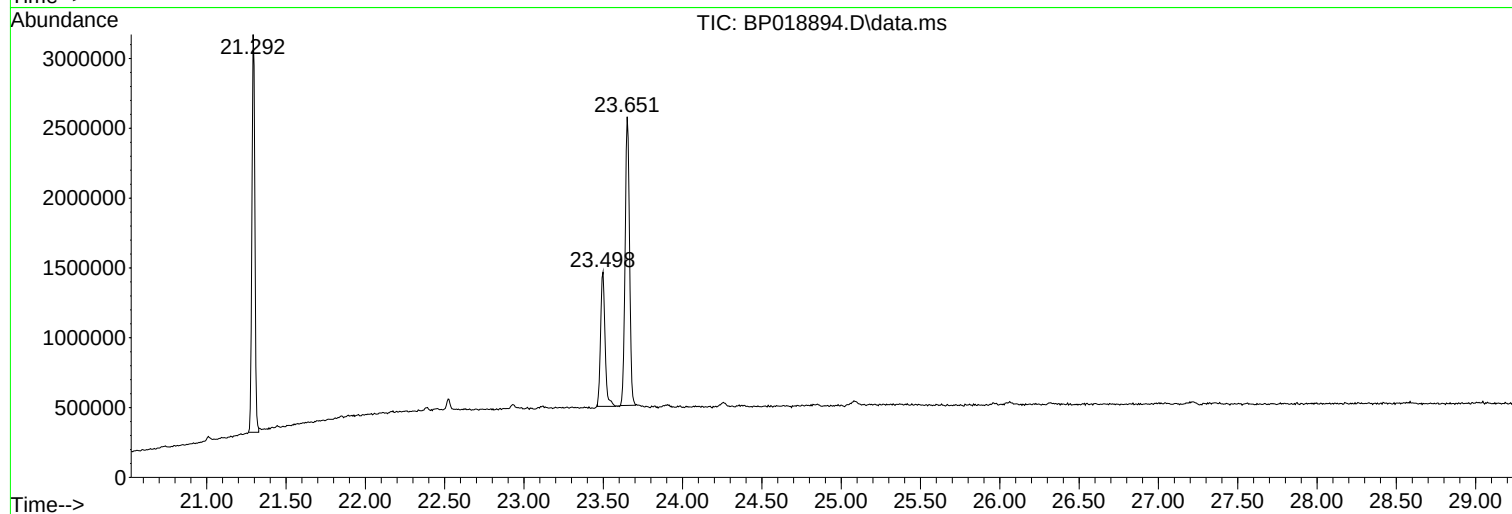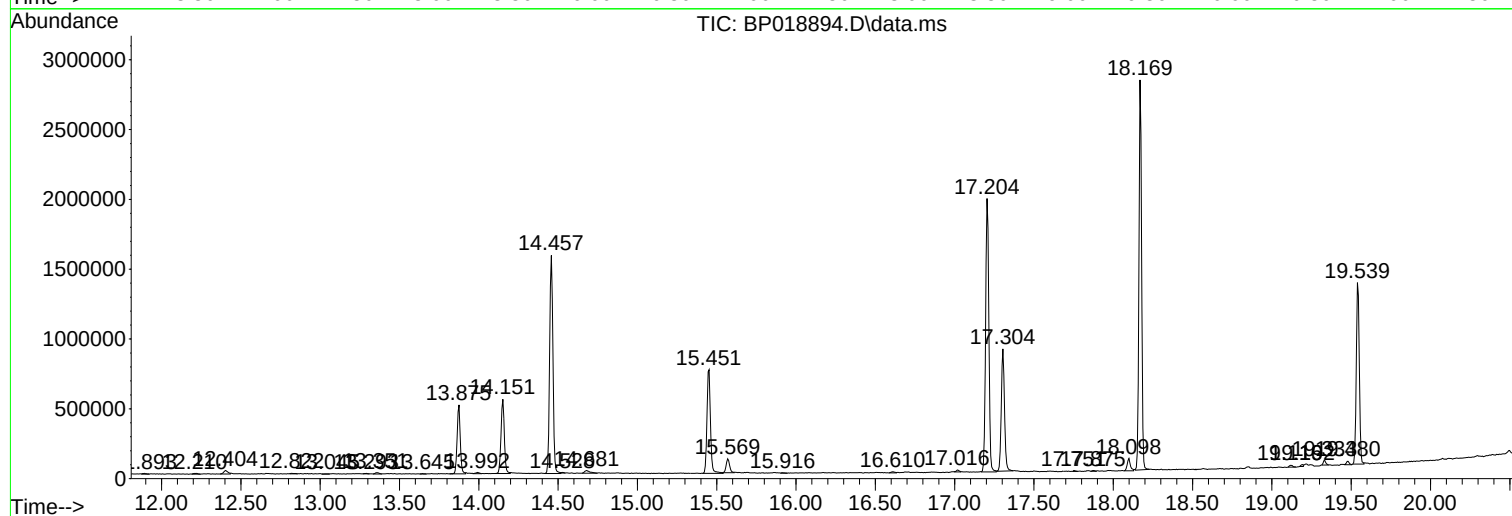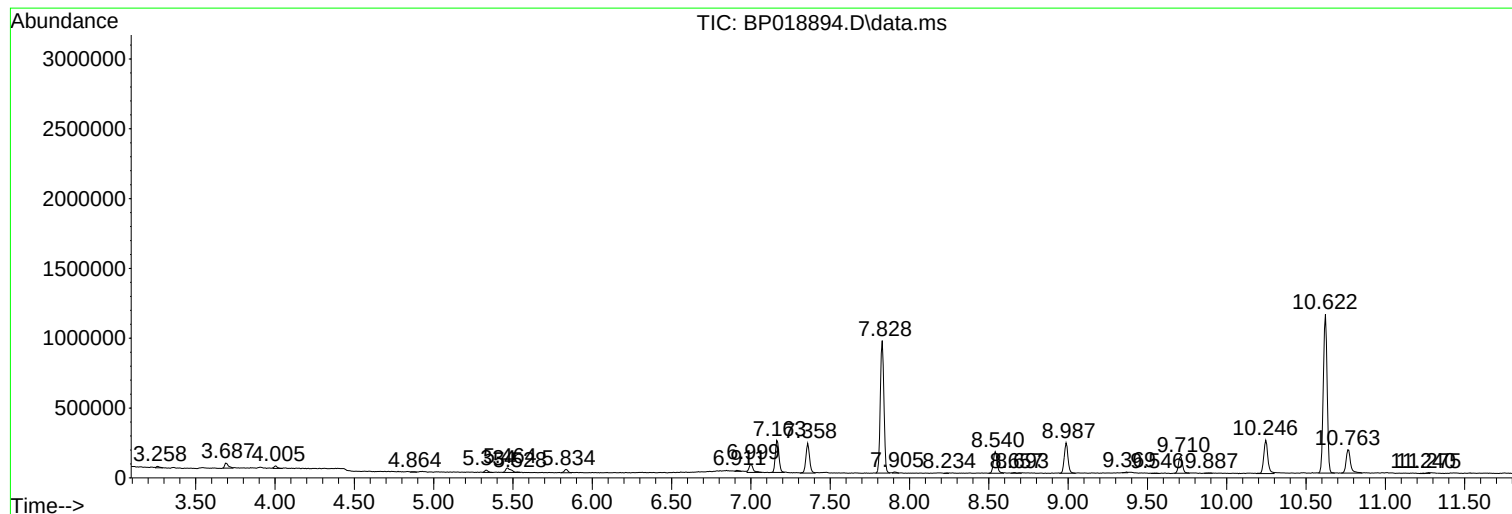

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018894.D
Acq On : 15 Dec 2023 23:27
Operator : MA/JU
Sample : 05627-17DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018894.D
Acq On : 15 Dec 2023 23:27
Operator : MA/JU
Sample : 05627-17DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
