

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121620\
 Data File : BP004325.D
 Acq On : 16 Dec 2020 15:32
 Operator : CG/JU
 Sample : L5067-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54F5

Quant Time: Dec 17 00:28:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 17 00:04:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	254717	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	1063699	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.48	164	674265	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.25	188	1485506	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	1558697	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	1651609	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.33	96	14189	1.96	ng/uL	0.00
5) Phenol-d5	7.00	99	273617	12.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	166944	12.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	235065	14.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	197024	12.37	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	122126	14.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	136363	18.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	231360	14.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	303714	15.51	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	737255	14.31	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	953775	14.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.68	143	101166	11.62	ng/ul	0.00
58) Fluorene-d10	15.48	176	643271	13.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.60	200	82533	11.58	ng/ul	0.00
71) Anthracene-d10	17.35	188	1032480	14.26	ng/ul	0.00
79) Pyrene-d10	19.59	212	1273476	15.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.55	264	1379645	15.86	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	7.03	94	114337	5.197	ng/ul	99
45) Dimethylphthalate	13.93	163	56703	1.080	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121620\
Data File : BP004325.D
Acq On : 16 Dec 2020 15:32
Operator : CG/JU
Sample : L5067-17
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54F5

Quant Time: Dec 17 00:28:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 17 00:04:11 2020
Response via : Initial Calibration

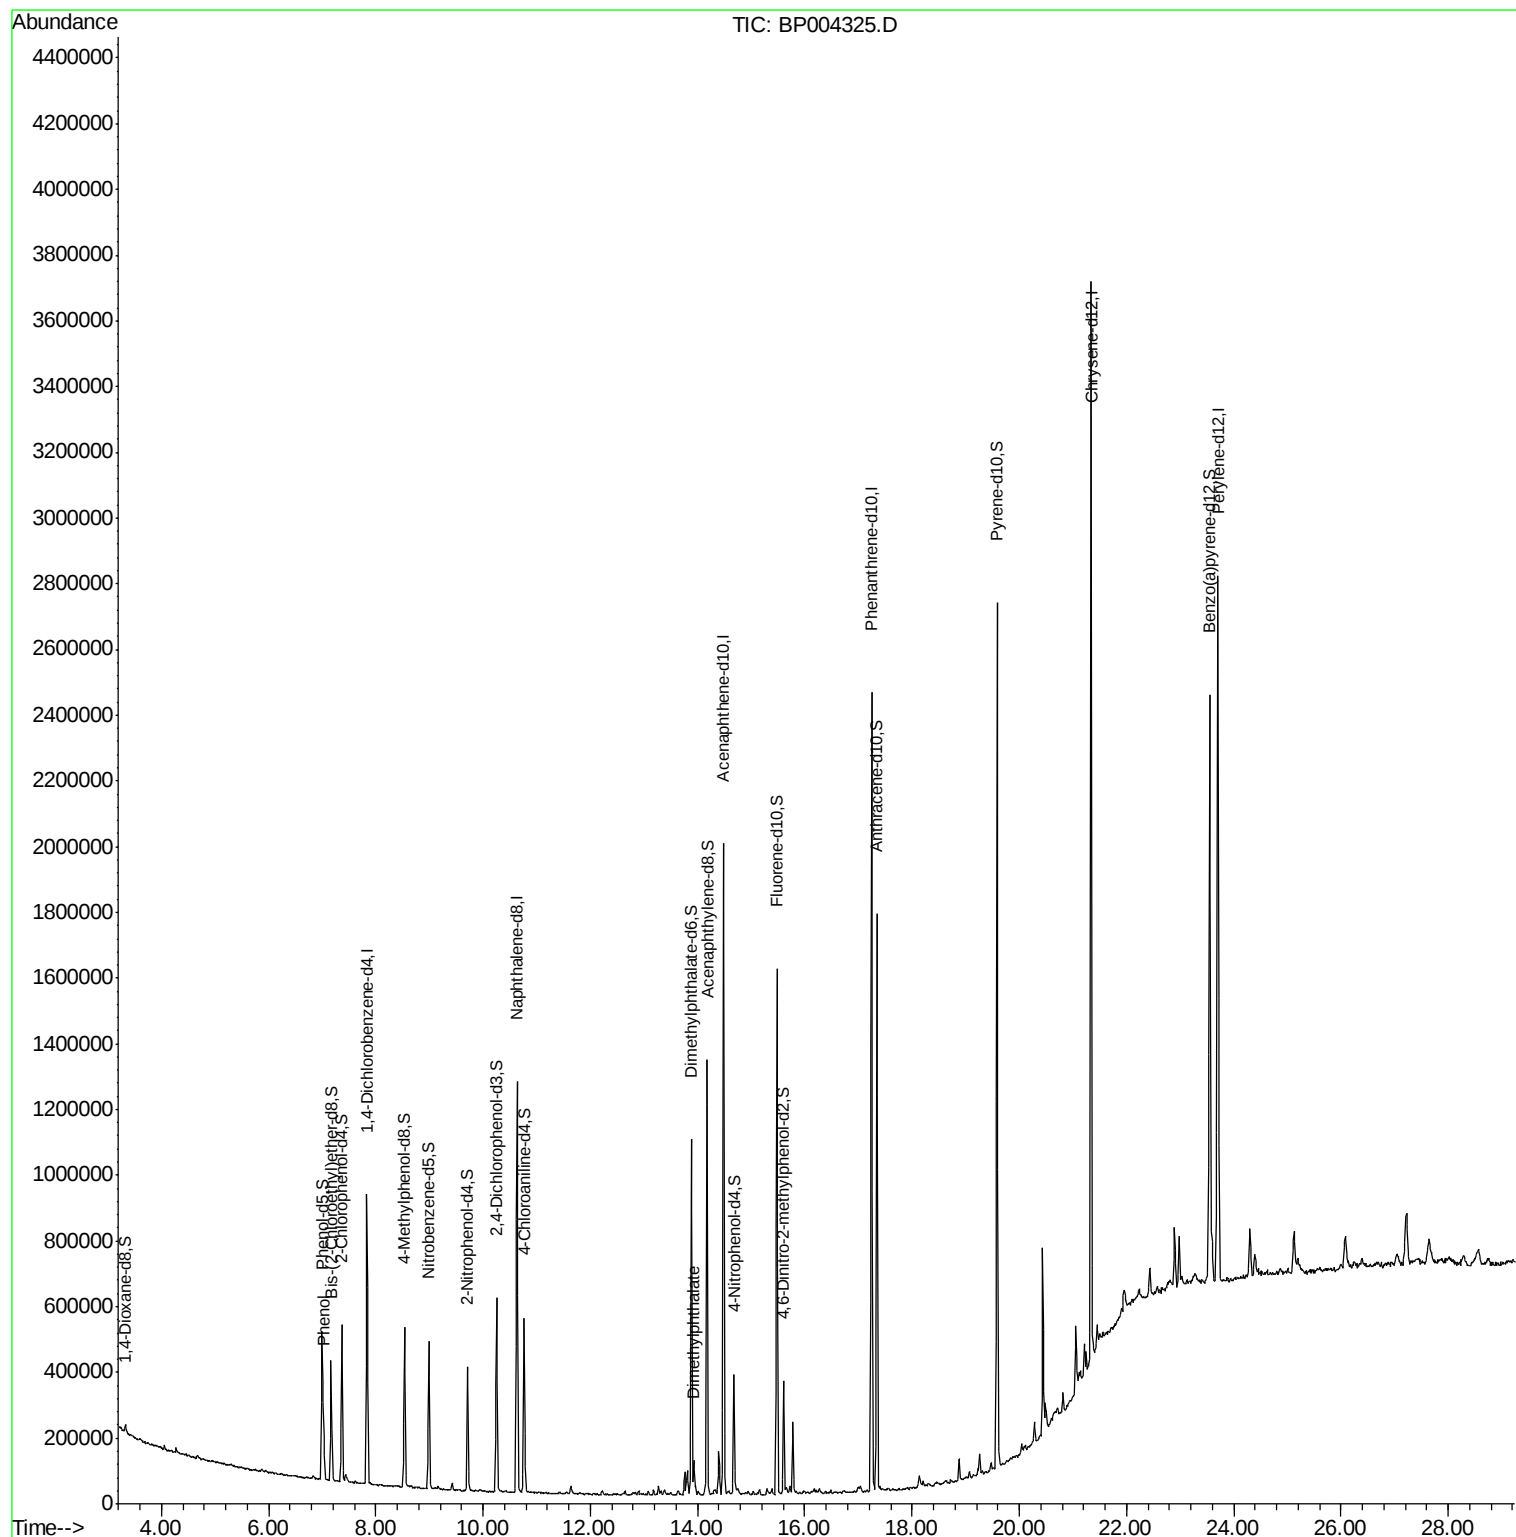

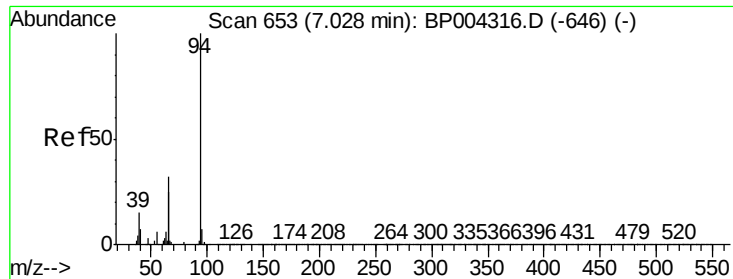

#6

Phenol

Concen: 5.197 ng/ul

RT: 7.03 min Scan# 653

Delta R.T. 0.00 min

Lab File: BP004325.D

Acq: 16 Dec 2020 15:32

Instrument :

BNA_P

ClientSampleId :

A54F5





Tot Ion: 94 Resp: 114337

Ion Ratio Lower Upper

94 100

65 25.3 20.8 31.2

66 33.2 26.5 39.7

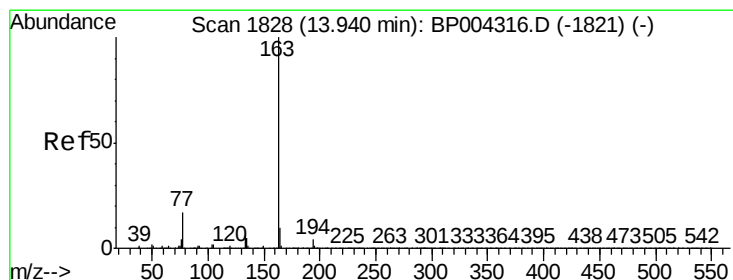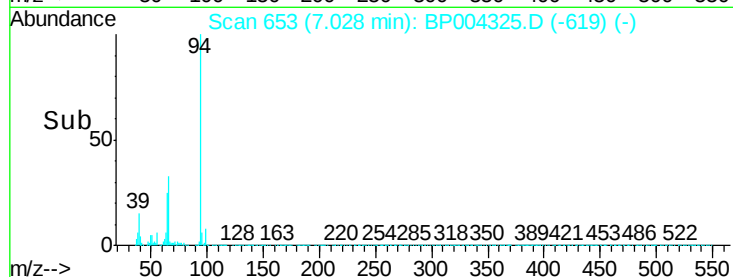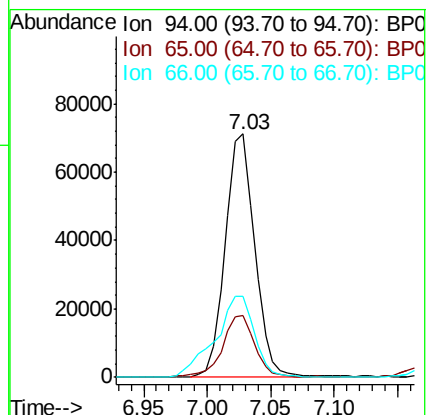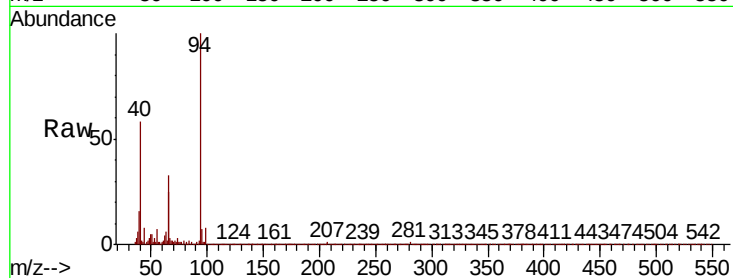

#45

Dimethylphthalate

Concen: 1.080 ng/ul

RT: 13.93 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BP004325.D

Acq: 16 Dec 2020 15:32

Tgt Ion: 163 Resp: 56703

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 11.0 8.4 12.6

