

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121620\
 Data File : BP004333.D
 Acq On : 16 Dec 2020 20:03
 Operator : CG/JU
 Sample : L5067-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54F3

Quant Time: Dec 17 01:00:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 17 00:04:11 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	273983	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	1127038	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.48	164	696784	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.25	188	1553940	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	1664803	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	1766860	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.33	96	37547	4.81	ng/uL	0.00
5) Phenol-d5	7.00	99	815314	35.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	437579	30.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	636289	36.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	629880	36.78	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	324265	35.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	375115	49.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	644028	38.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	889570	42.87	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	1943374	36.49	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	2501819	36.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.68	143	349340	38.84	ng/ul	0.00
58) Fluorene-d10	15.48	176	1693570	35.11	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.60	200	287750	38.60	ng/ul	0.00
71) Anthracene-d10	17.35	188	2754225	36.37	ng/ul	0.00
79) Pyrene-d10	19.59	212	3227212	37.21	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	3524823	37.87	ng/ul	0.01
Target Compounds						
6) Phenol	7.03	94	323226	13.659	ng/ul	100
45) Dimethylphthalate	13.93	163	127370	2.348	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121620\
Data File : BP004333.D
Acq On : 16 Dec 2020 20:03
Operator : CG/JU
Sample : L5067-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54F3

Quant Time: Dec 17 01:00:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 17 00:04:11 2020
Response via : Initial Calibration

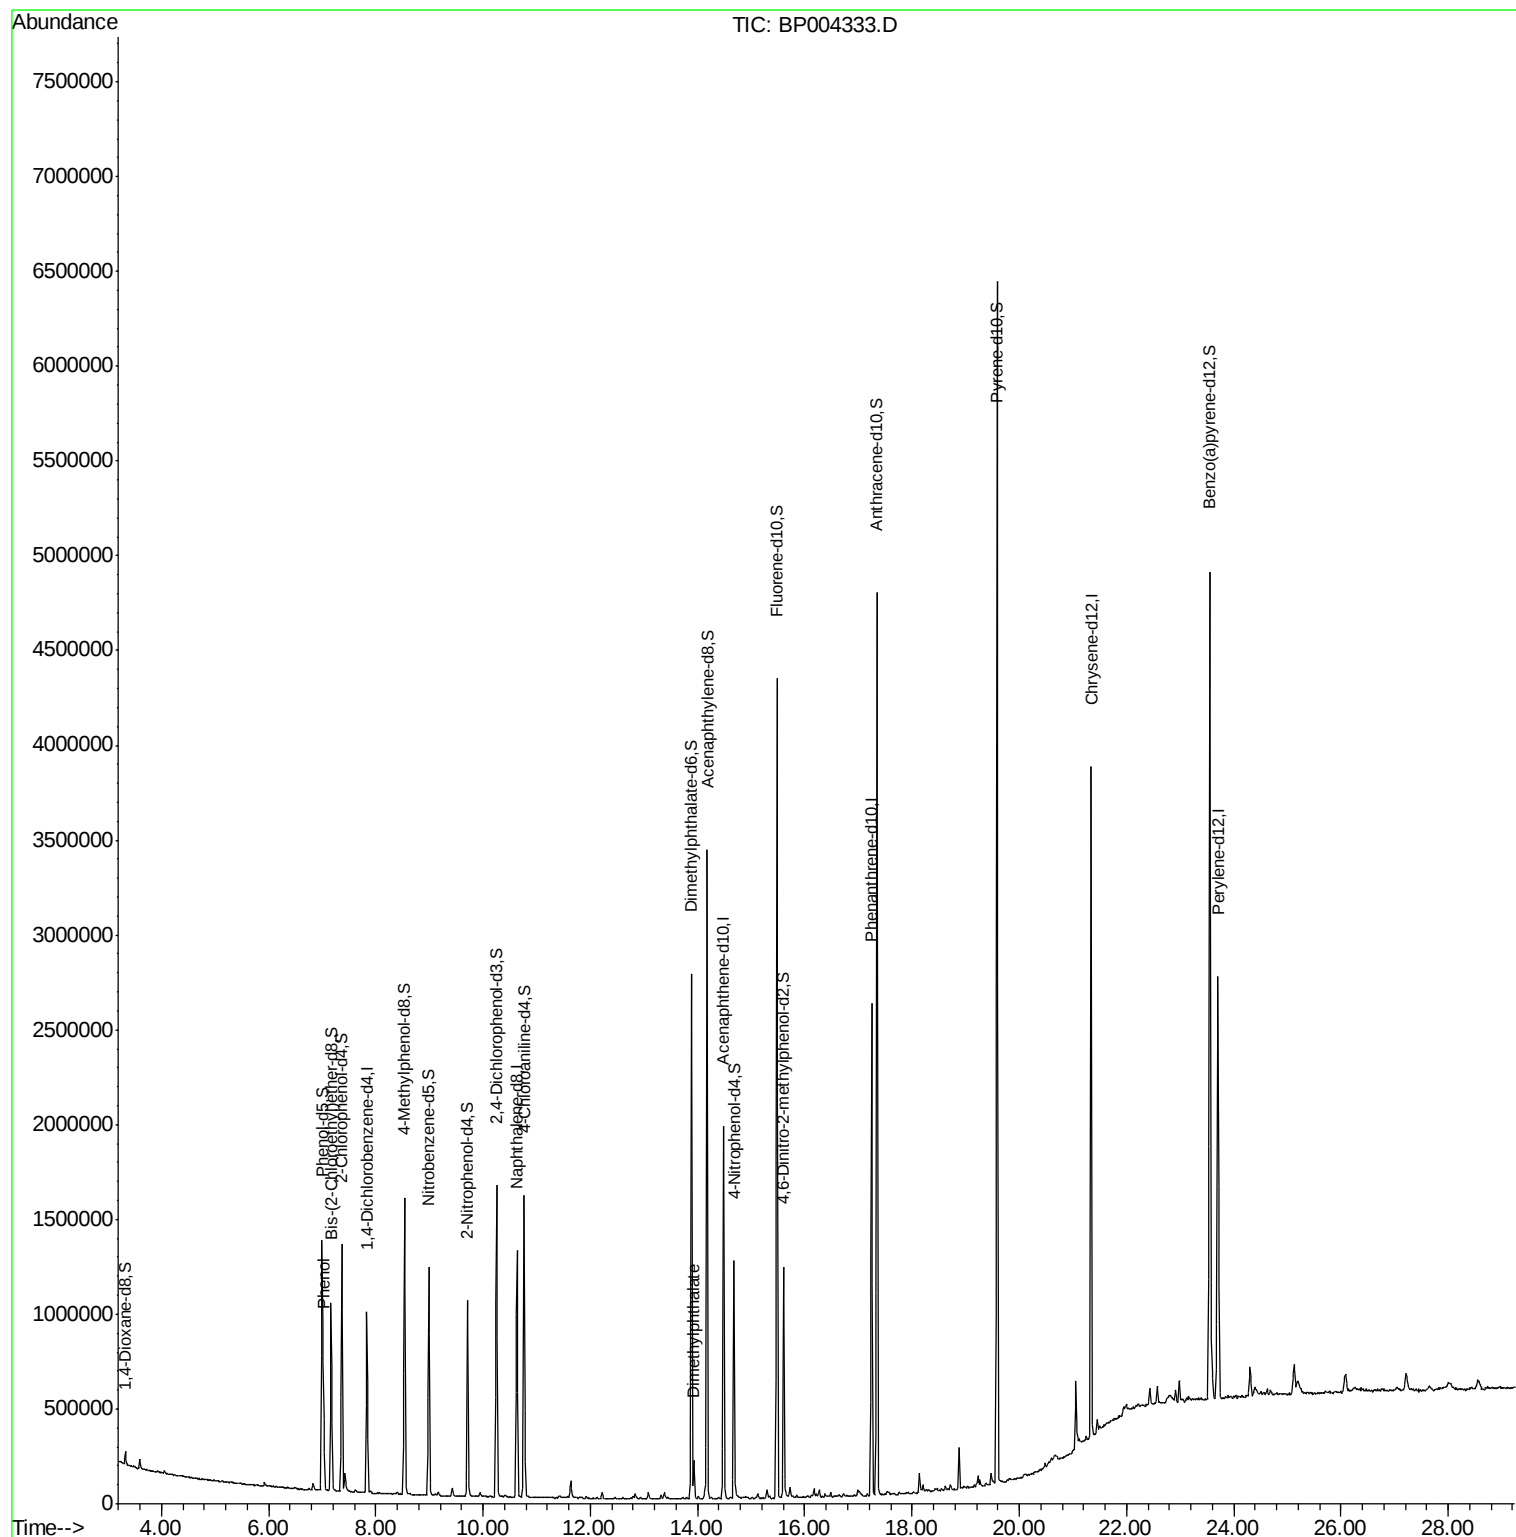

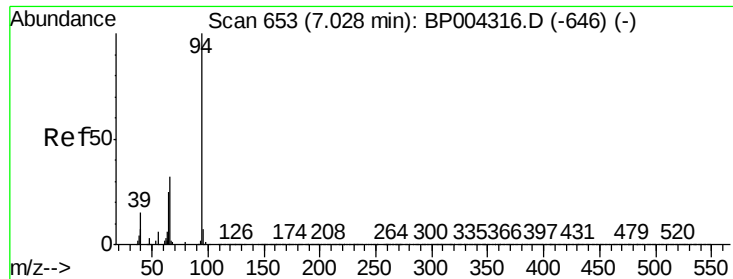

#6

Phenol

Concen: 13.659 ng/ul

RT: 7.03 min Scan# 653

Delta R.T. -0.00 min

Lab File: BP004333.D

Acq: 16 Dec 2020 20:03

Instrument :

BNA_P

ClientSampleId :

A54F3





Tot Ion: 94 Resp: 323226

Ion Ratio Lower Upper

94 100

65 26.1 20.8 31.2

66 33.2 26.5 39.7

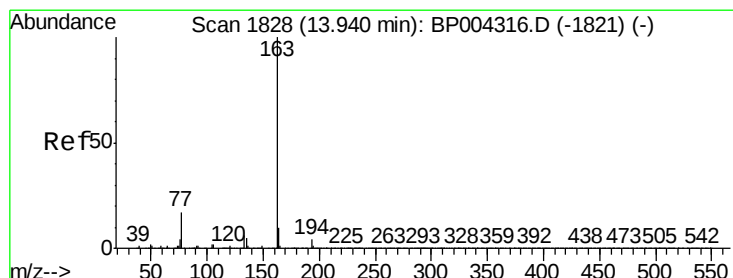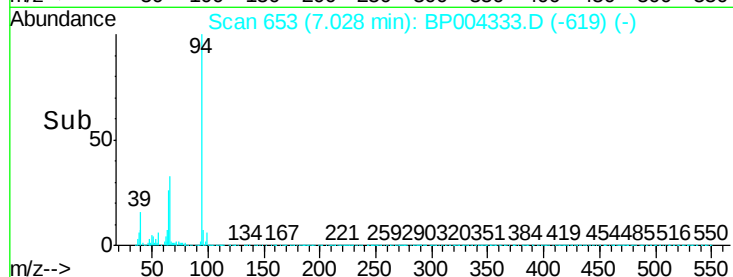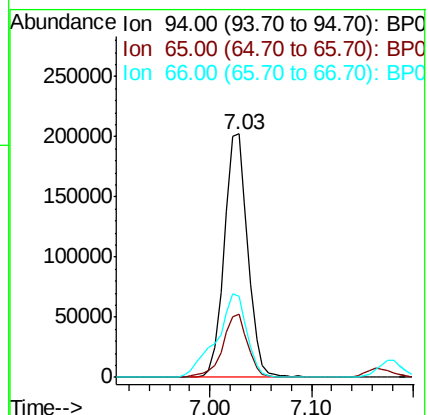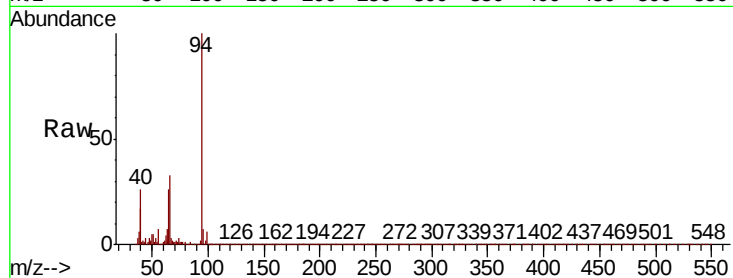

#45

Dimethylphthalate

Concen: 2.348 ng/ul

RT: 13.93 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BP004333.D

Acq: 16 Dec 2020 20:03

Tgt Ion:163 Resp: 127370

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 9.7 8.4 12.6

