

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121720\
 Data File : BP004342.D
 Acq On : 17 Dec 2020 15:58
 Operator : CG/JU
 Sample : L5067-18
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54F6

Quant Time: Dec 17 16:24:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 17 15:20:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	277412	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.63	136	1163803	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.48	164	707177	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.25	188	1534418	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	1545190	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	1671199	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.33	96	43033	5.45	ng/uL	0.00
5) Phenol-d5	7.00	99	885393	38.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	492542	34.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	711005	40.82	ng/ul	-0.01
13) 4-Methylphenol-d8	8.53	113	711218	41.02	ng/ul	-0.01
19) Nitrobenzene-d5	8.99	128	363614	38.15	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.71	143	412854	52.51	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.25	165	714692	41.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	943240	44.02	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	2049688	37.92	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	2698827	39.12	ng/ul	0.00
52) 4-Nitrophenol-d4	14.68	143	342932	37.56	ng/ul	0.00
58) Fluorene-d10	15.48	176	1783686	36.44	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.60	200	276818	37.60	ng/ul	-0.01
71) Anthracene-d10	17.34	188	2838615	37.96	ng/ul	-0.01
79) Pyrene-d10	19.59	212	3245133	40.31	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.55	264	3472198	39.44	ng/ul	-0.01


Target Compounds					Ovalue	
6) Phenol	7.02	94	295911	12.350	ng/ul	100
45) Dimethylphthalate	13.93	163	128319	2.331	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121720\
Data File : BP004342.D
Acq On : 17 Dec 2020 15:58
Operator : CG/JU
Sample : L5067-18
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54F6

Quant Time: Dec 17 16:24:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 17 15:20:40 2020
Response via : Initial Calibration

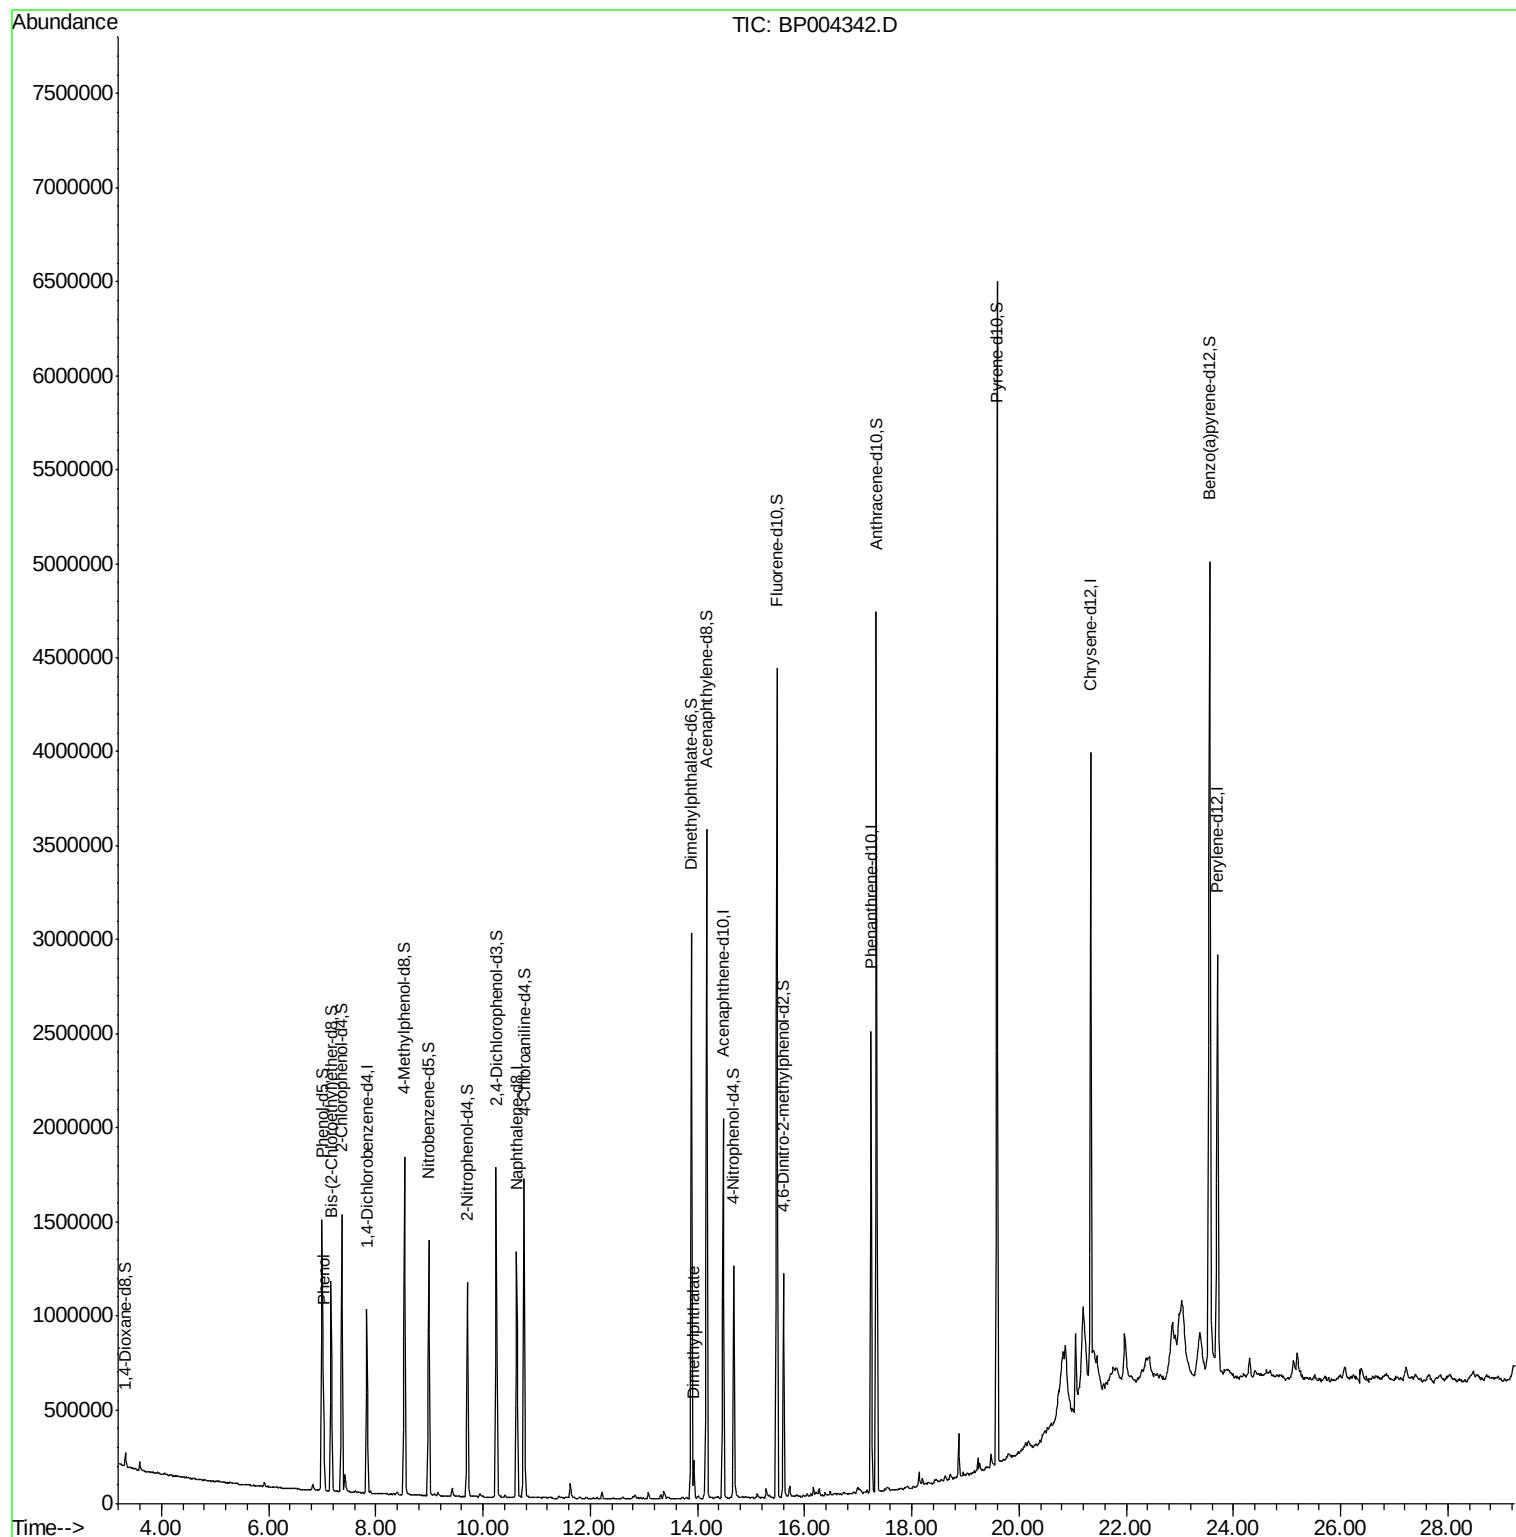

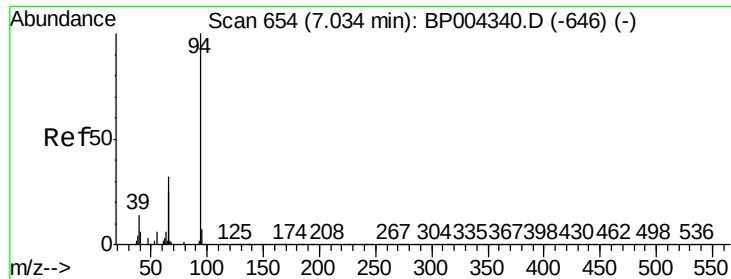





#6

Phenol

Concen: 12.350 ng/ul
 RT: 7.02 min Scan# 652
 Delta R.T. -0.01 min
 Lab File: BP004342.D
 Acq: 17 Dec 2020 15:58

Instrument :
 BNA_P
 ClientSampleId :
 A54F6

Tot Ion:	94	Resp:	295911
Ion	Ratio	Lower	Upper
94	100		
65	26.0	20.8	31.2
66	33.0	26.5	39.7

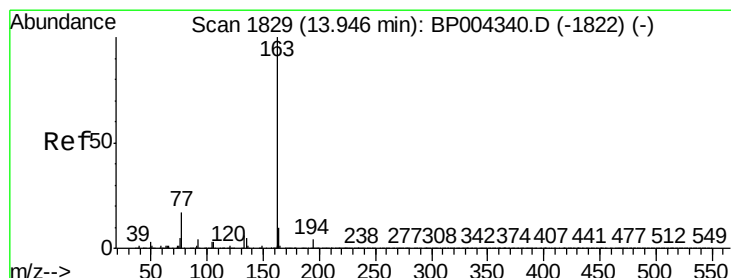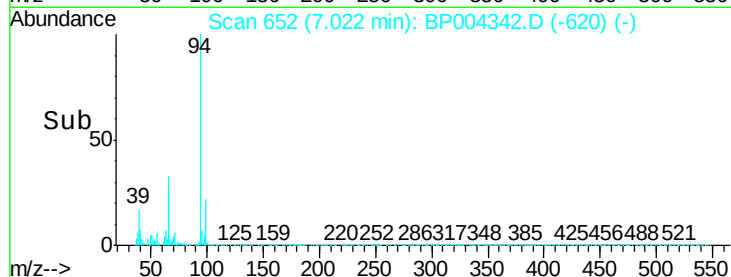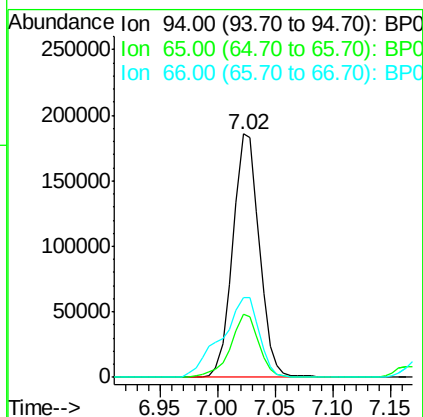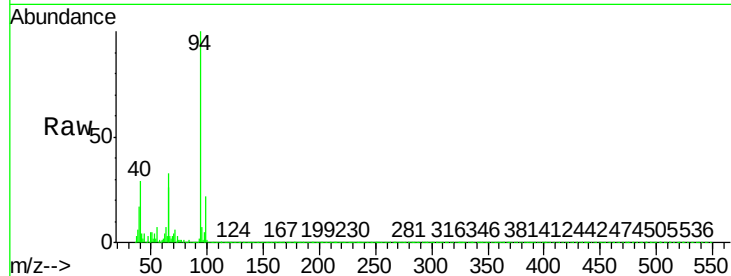

#45

Dimethylphthalate

Concen: 2.331 ng/ul
 RT: 13.93 min Scan# 1827
 Delta R.T. -0.01 min
 Lab File: BP004342.D
 Acq: 17 Dec 2020 15:58

Tgt Ion:	163	Resp:	128319
Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.4	5.2
164	10.9	8.4	12.6

