

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121720\
 Data File : BP004343.D
 Acq On : 17 Dec 2020 16:32
 Operator : CG/JU
 Sample : L5067-20
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54F8

Quant Time: Dec 17 16:58:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 17 15:20:40 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	227986	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.63	136	954408	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.48	164	589495	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.25	188	1297470	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	1370998	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	1472585	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.32	96	37136	5.72	ng/uL	-0.01
5) Phenol-d5	7.00	99	804568	42.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	456286	38.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	650290	45.43	ng/ul	-0.01
13) 4-Methylphenol-d8	8.53	113	611879	42.94	ng/ul	-0.01
19) Nitrobenzene-d5	8.99	128	341765	43.72	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.71	143	386663	59.97	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.25	165	667859	47.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	852804	48.53	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	1938980	43.04	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	2539916	44.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.68	143	325888	42.82	ng/ul	0.00
58) Fluorene-d10	15.48	176	1699510	41.65	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.60	200	262129	42.11	ng/ul	-0.01
71) Anthracene-d10	17.34	188	2753113	43.54	ng/ul	-0.01
79) Pyrene-d10	19.59	212	3228407	45.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	3499432	45.11	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	7.02	94	99337	5.045	ng/ul	97
45) Dimethylphthalate	13.93	163	386118	8.414	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121720\
Data File : BP004343.D
Acq On : 17 Dec 2020 16:32
Operator : CG/JU
Sample : L5067-20
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54F8

Quant Time: Dec 17 16:58:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 17 15:20:40 2020
Response via : Initial Calibration

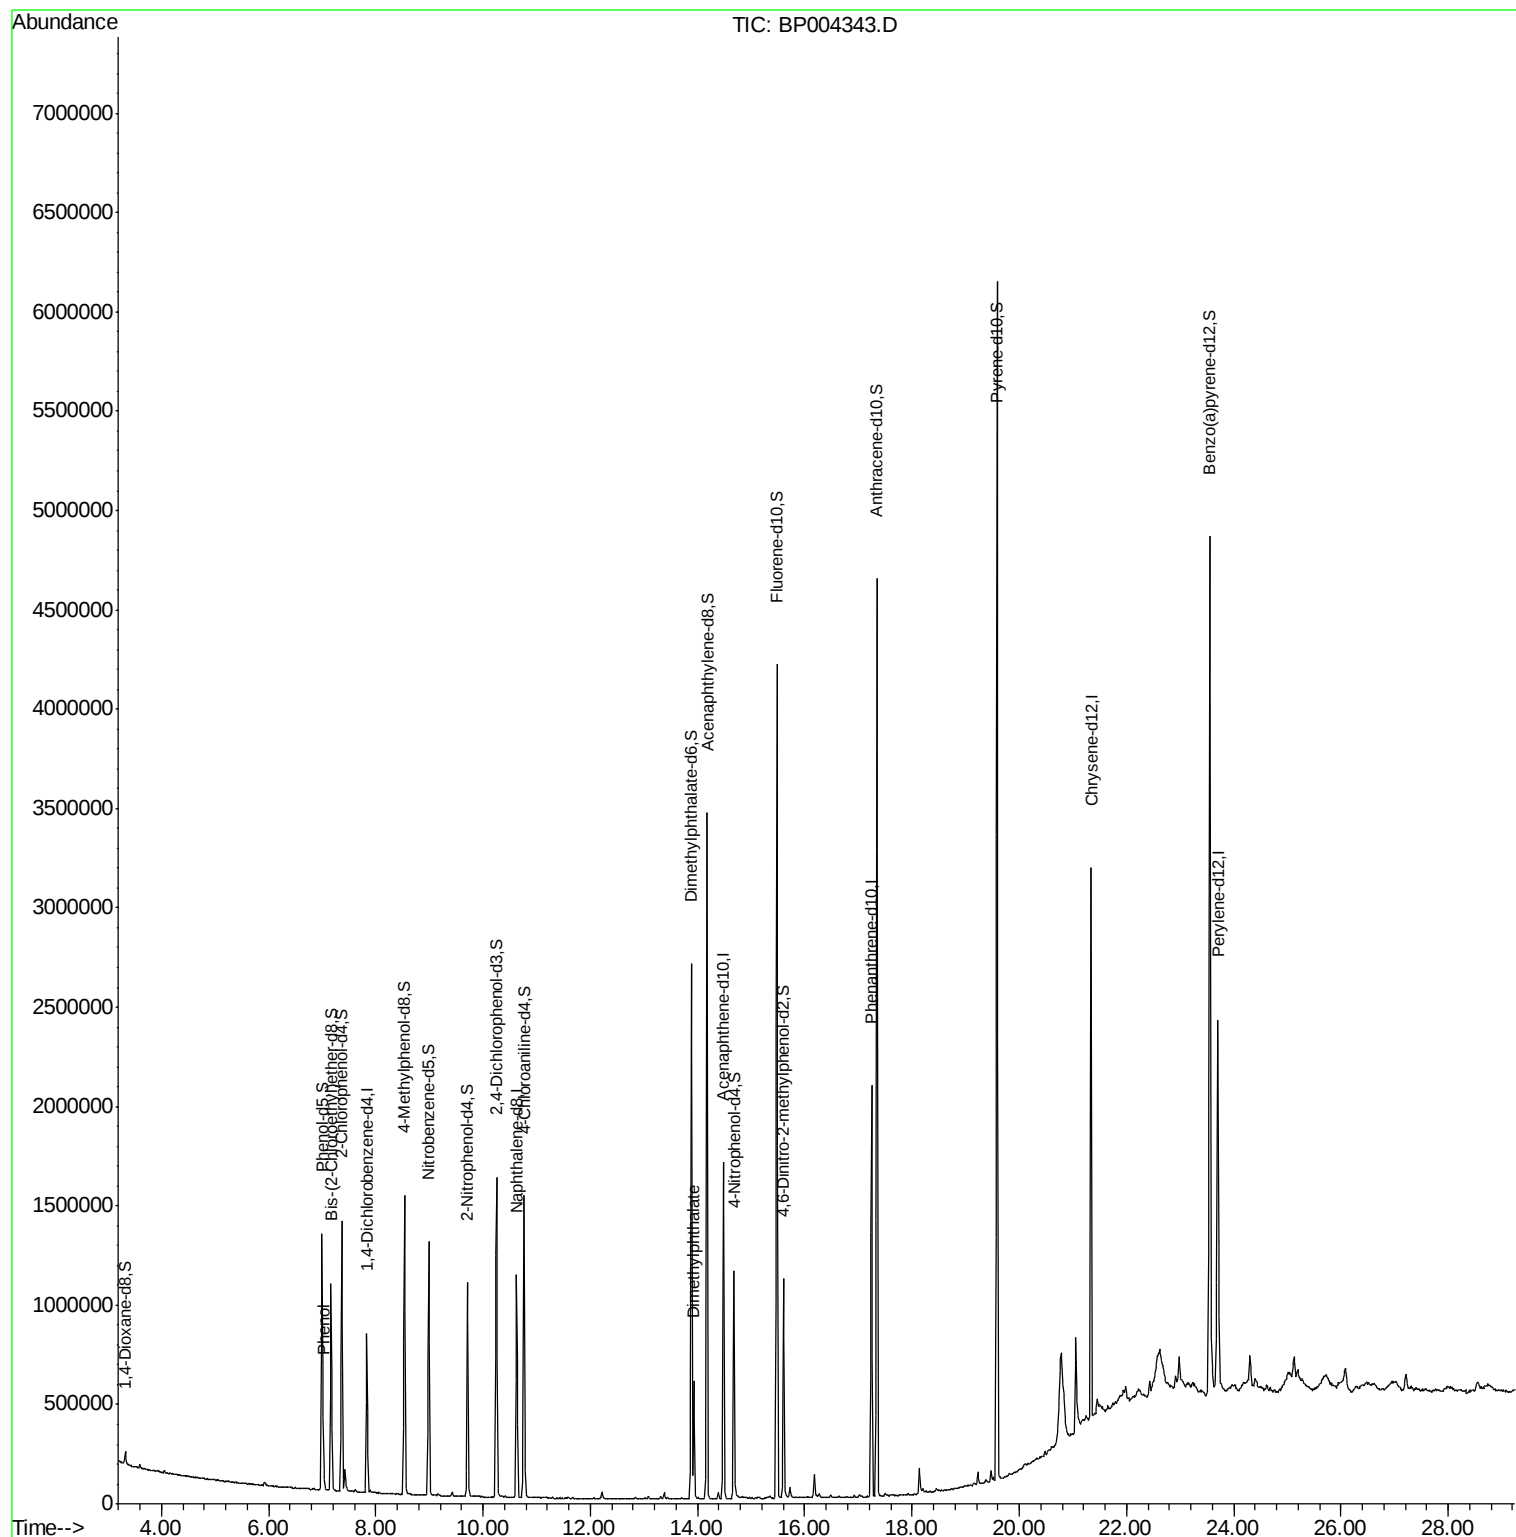

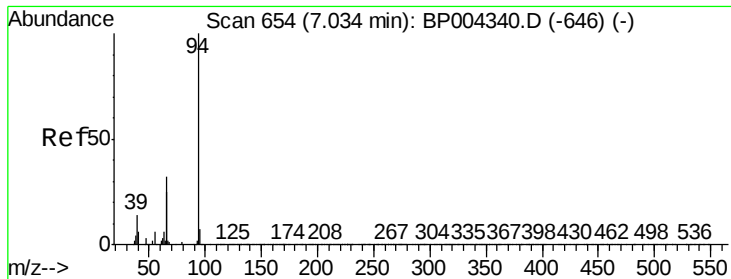

#6

Phenol

Concen: 5.045 ng/ul

RT: 7.02 min Scan# 652

Delta R.T. -0.01 min

Lab File: BP004343.D

Acq: 17 Dec 2020 16:32

Instrument :

BNA_P

ClientSampleId :

A54F8





Tot Ion: 94 Resp: 99337

Ion Ratio Lower Upper

94 100

65 26.8 20.8 31.2

66 35.5 26.5 39.7

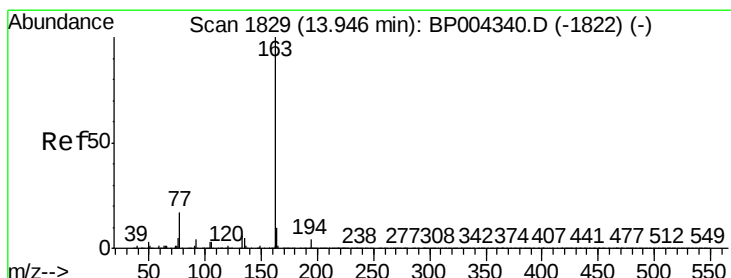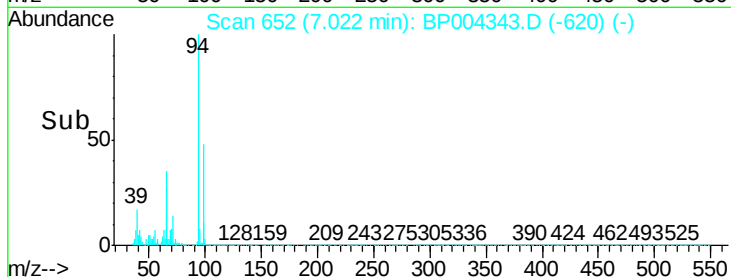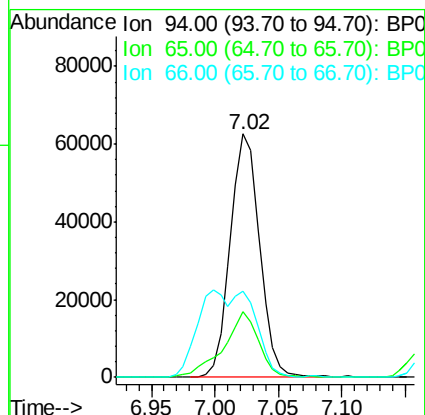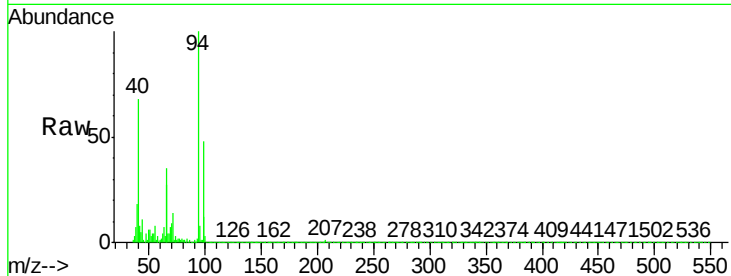

#45

Dimethylphthalate

Concen: 8.414 ng/ul

RT: 13.93 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BP004343.D

Acq: 17 Dec 2020 16:32

Tgt Ion:163 Resp: 386118

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 9.8 8.4 12.6

