


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121721\
 Data File : BP008466.D
 Acq On : 17 Dec 2021 11:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 18 06:49:58 2021

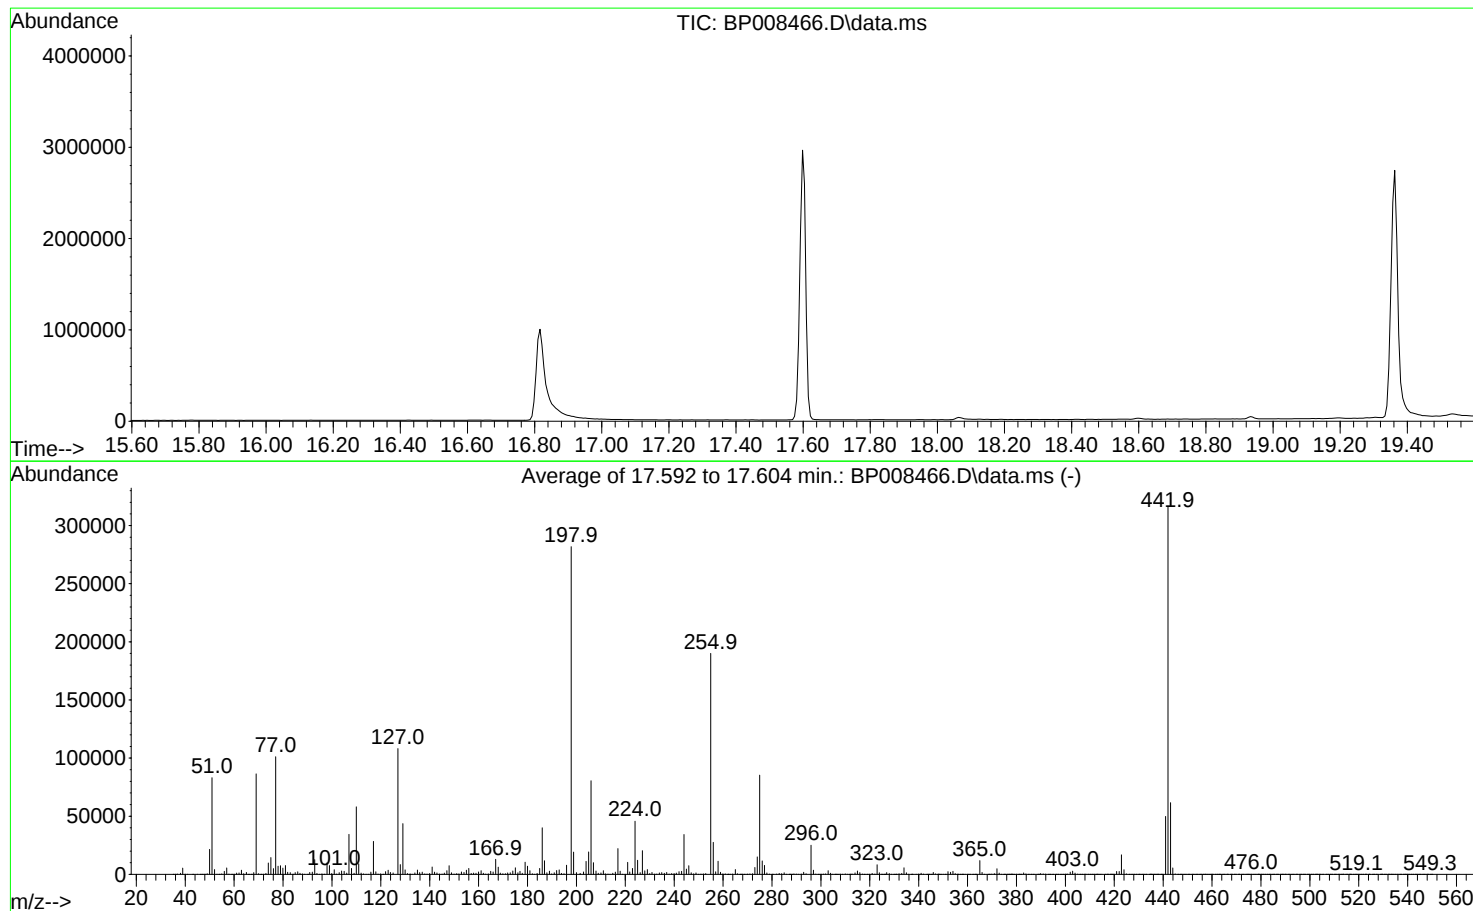




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	83182	PASS
68	69	0.00	2	1.8	1582	PASS
69	198	0.00	100	30.7	86455	PASS
70	69	0.00	2	0.6	509	PASS
127	198	10	80	38.4	108170	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	281806	PASS
199	198	5	9	6.8	19088	PASS
275	198	10	60	30.3	85388	PASS
365	198	1	100	4.2	11812	PASS
441	198	0.01	100	17.7	49813	PASS
442	442	100	100	100.0	316364	PASS
443	442	15	24	19.5	61656	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121721\
Data File : BP008466.D
Acq On : 17 Dec 2021 11:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 20 09:13:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 18 06:49:58 2021
Response via : Initial Calibration

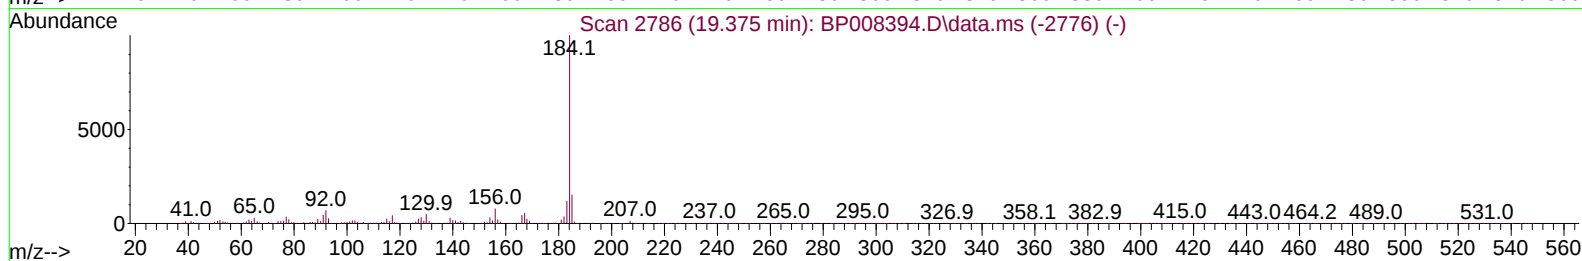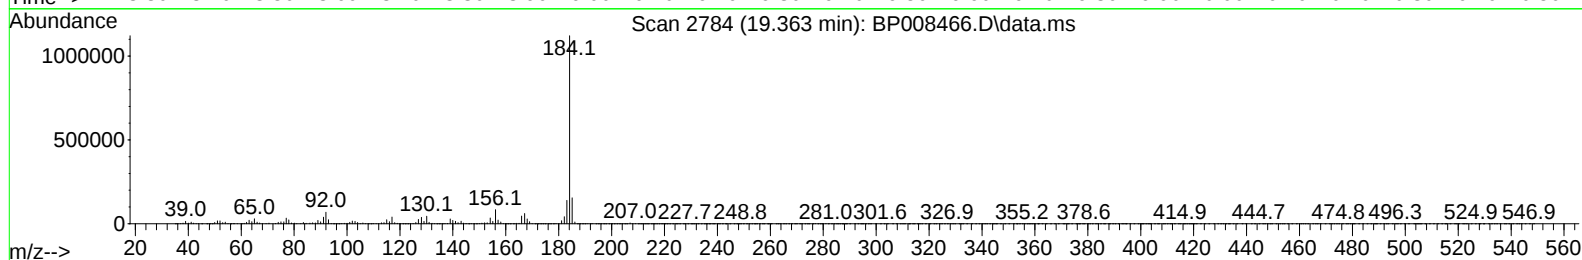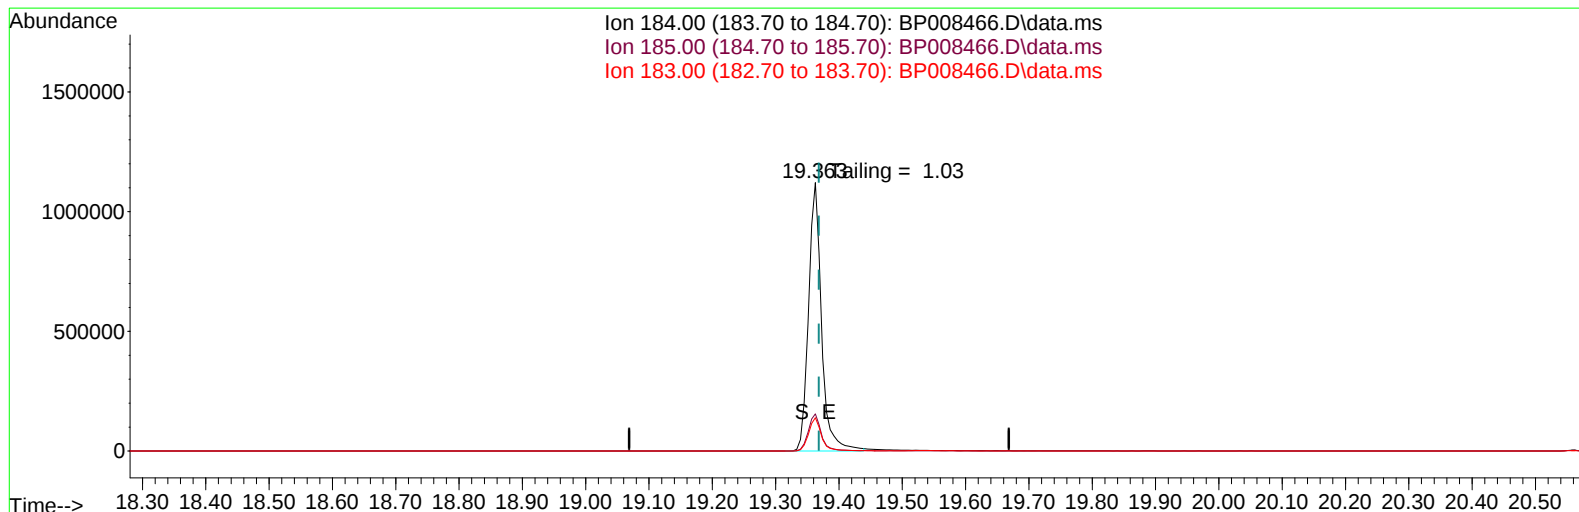

TIC: BP008466.D\data.ms

(77) Benzidine

19.363min (-0.006) 786827.18 ng




response 1636139

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.82
183.00	11.40	12.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121721\
Data File : BP008466.D
Acq On : 17 Dec 2021 11:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 20 09:13:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 18 06:49:58 2021
Response via : Initial Calibration

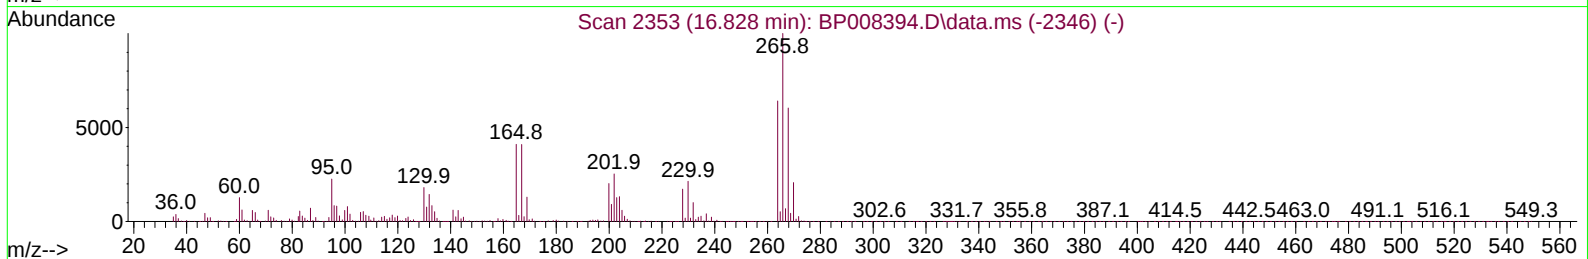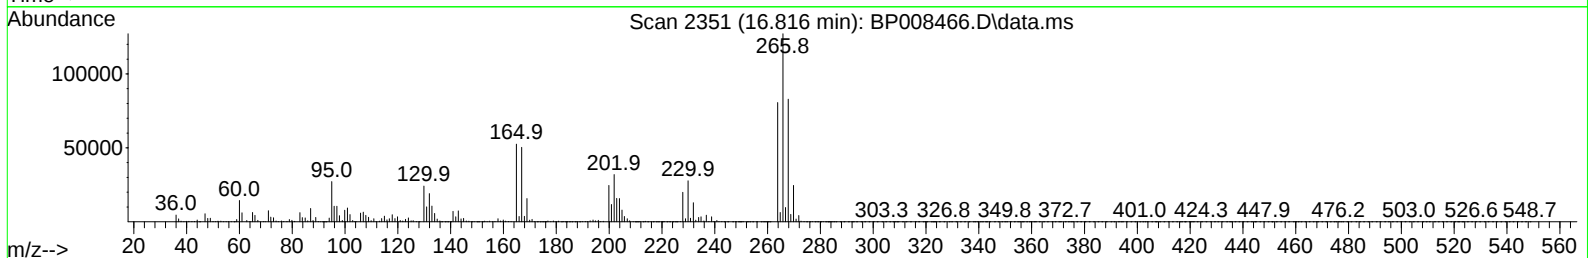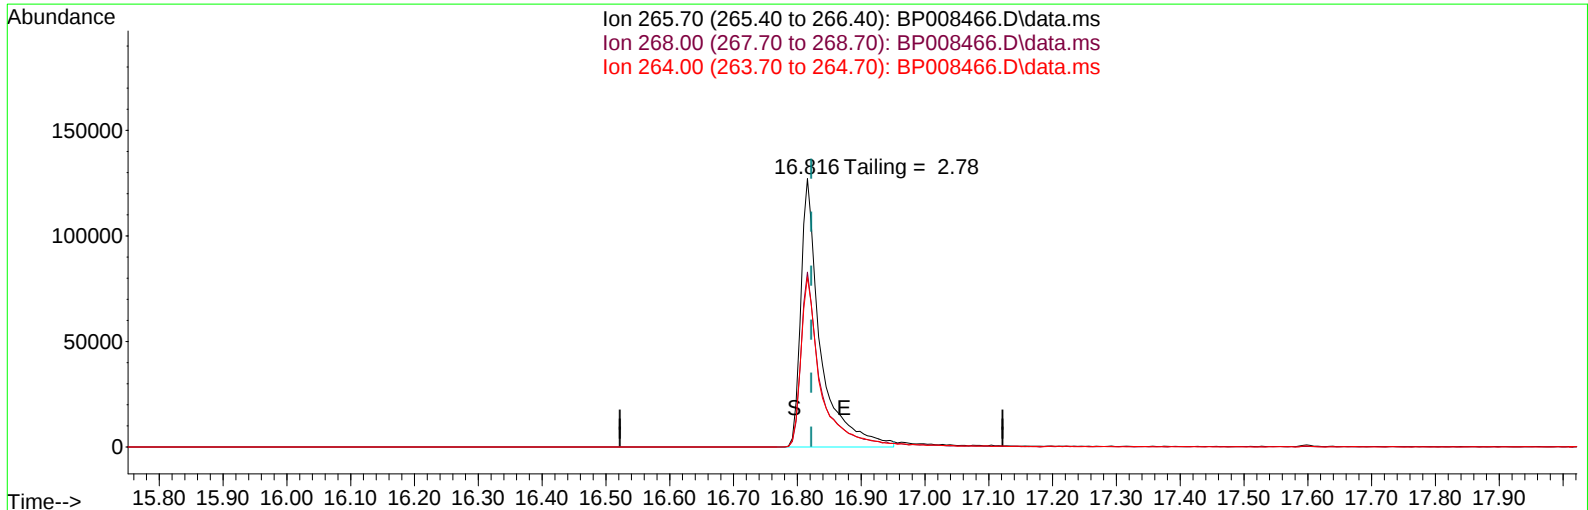

TIC: BP008466.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.006) 1364772.13 ng

response 279965

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	65.16
264.00	61.90	63.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/17/2021	BNA_P	<u>BP008466.D</u>
Compound Name	Response	Retention Time
DDT	983997	20.55
DDD	3668	20.13
DDE	1211	19.64
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4879	988876	0.49

Instrument :
BNA_P
ClientSampleId :
DFTPP