
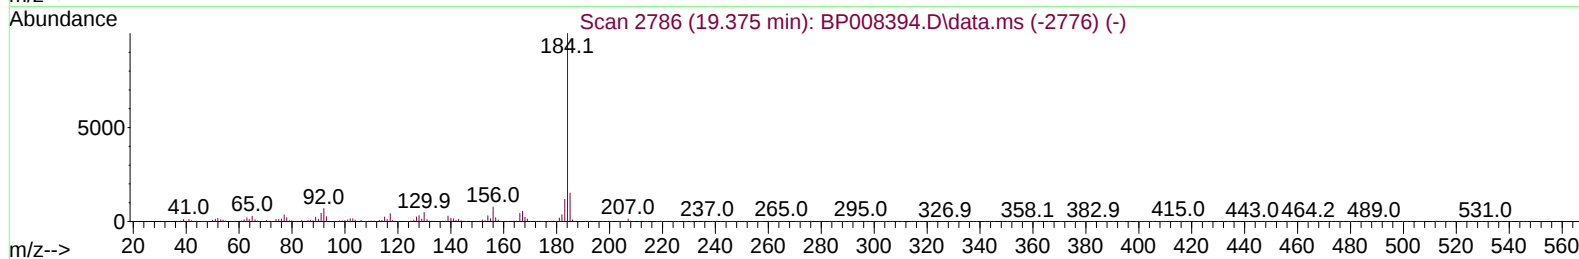
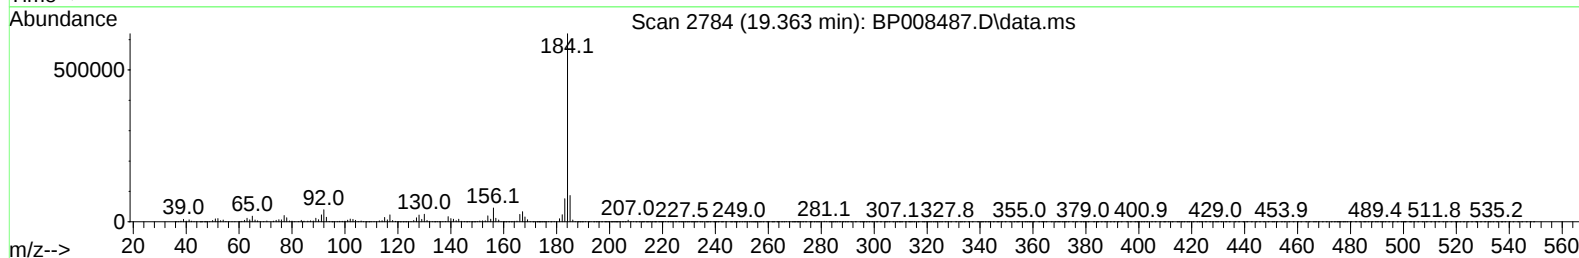


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121821\
 Data File : BP008487.D
 Acq On : 18 Dec 2021 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 01:58:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 18 06:49:58 2021
 Response via : Initial Calibration

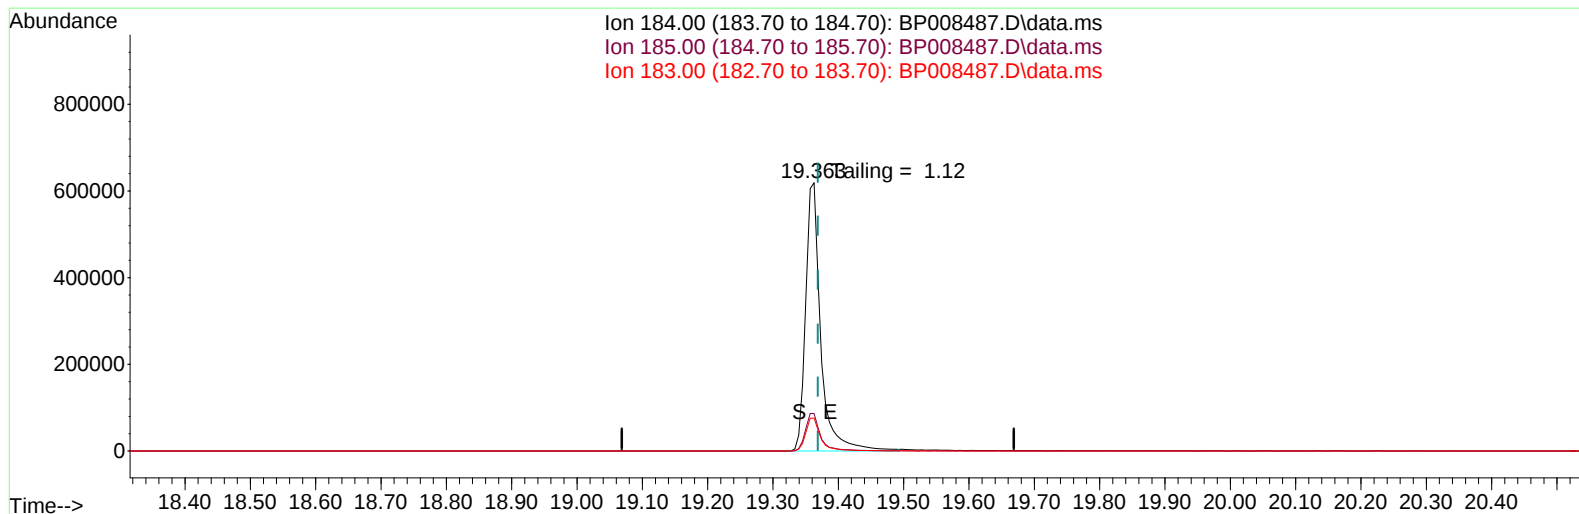




TIC: BP008487.D\data.ms

(77) Benzidine**19.363min (-0.006) 3422089.49 ng****response 1006645**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.95
183.00	11.40	12.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121821\
 Data File : BP008487.D
 Acq On : 18 Dec 2021 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 01:58:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 18 06:49:58 2021
 Response via : Initial Calibration

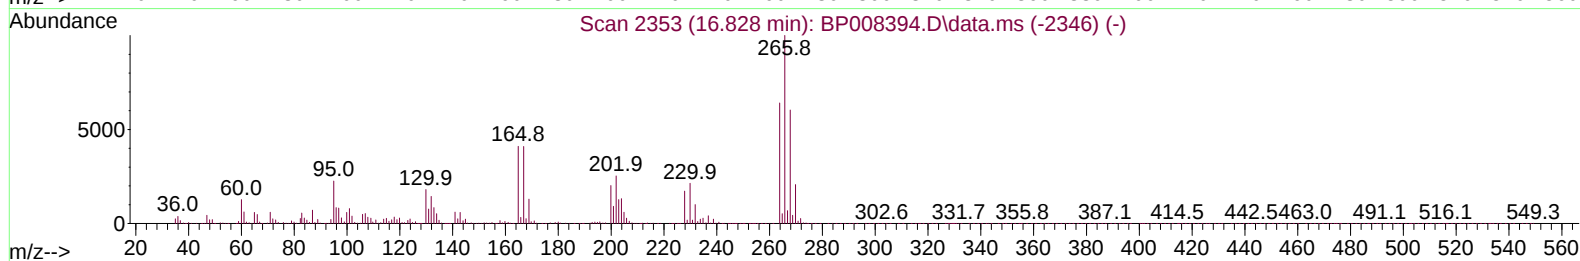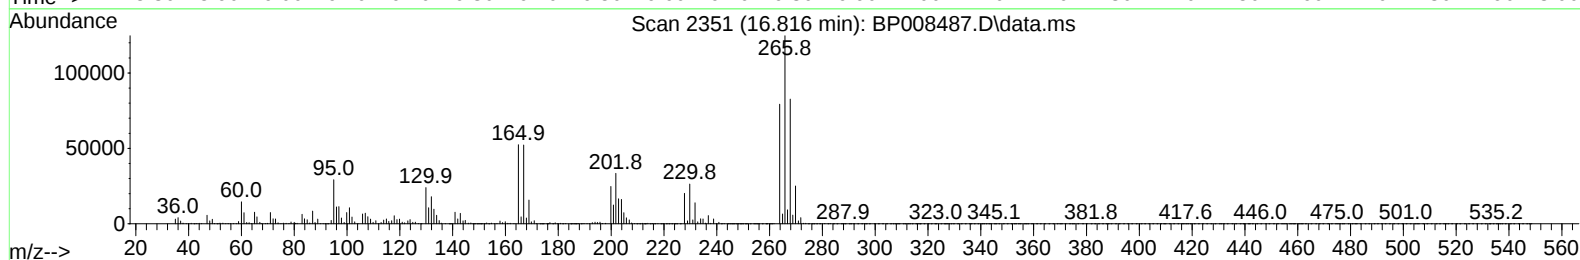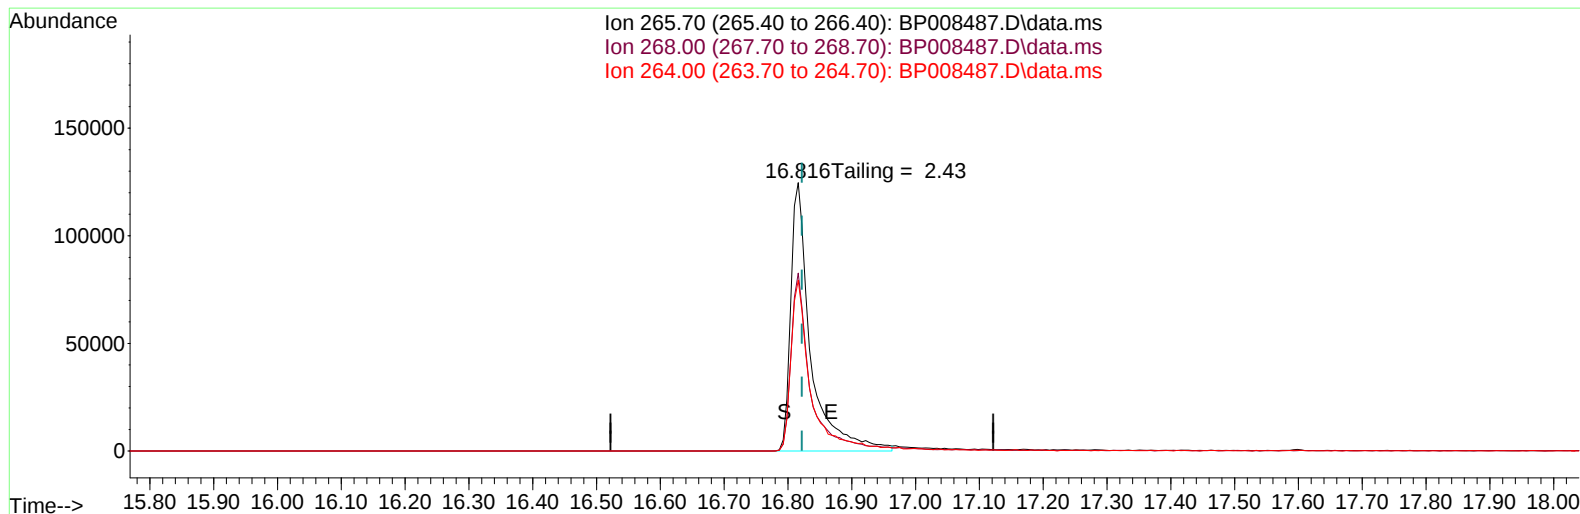

TIC: BP008487.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.006) 2406632.38 ng

response 277700

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.33
264.00	61.90	63.62
0.00	0.00	0.00