


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121821\
 Data File : BP008487.D
 Acq On : 18 Dec 2021 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 18 06:49:58 2021

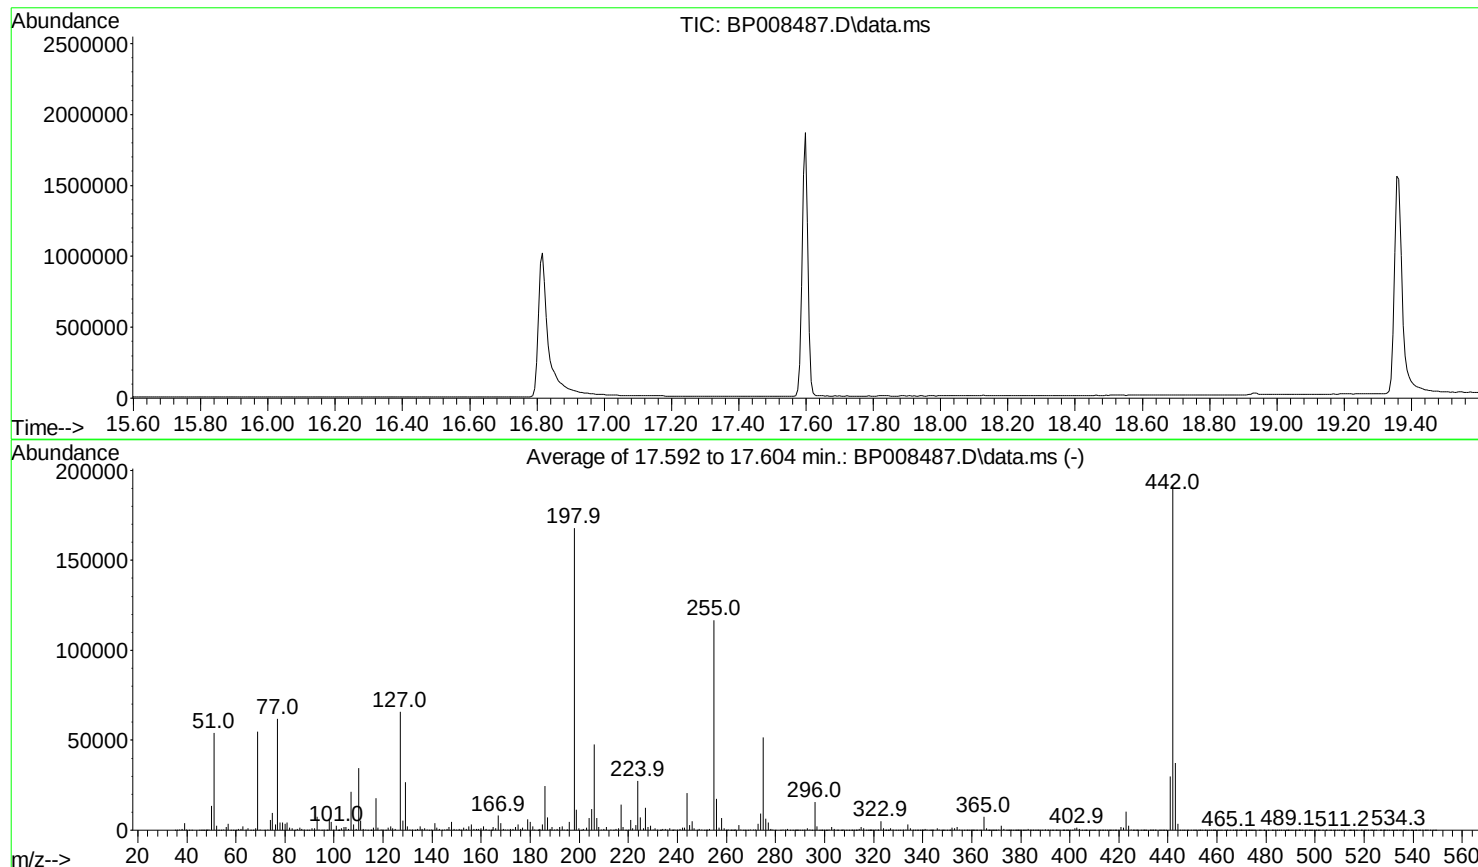




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2472

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	32.1	53900	PASS
68	69	0.00	2	2.0	1077	PASS
69	198	0.00	100	32.6	54687	PASS
70	69	0.00	2	0.6	338	PASS
127	198	10	80	39.3	65934	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	167963	PASS
199	198	5	9	6.8	11475	PASS
275	198	10	60	30.8	51725	PASS
365	198	1	100	4.5	7580	PASS
441	198	0.01	100	17.8	29956	PASS
442	442	100	100	100.0	191381	PASS
443	442	15	24	19.5	37381	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121821\
 Data File : BP008487.D
 Acq On : 18 Dec 2021 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 20 01:58:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 18 06:49:58 2021
 Response via : Initial Calibration

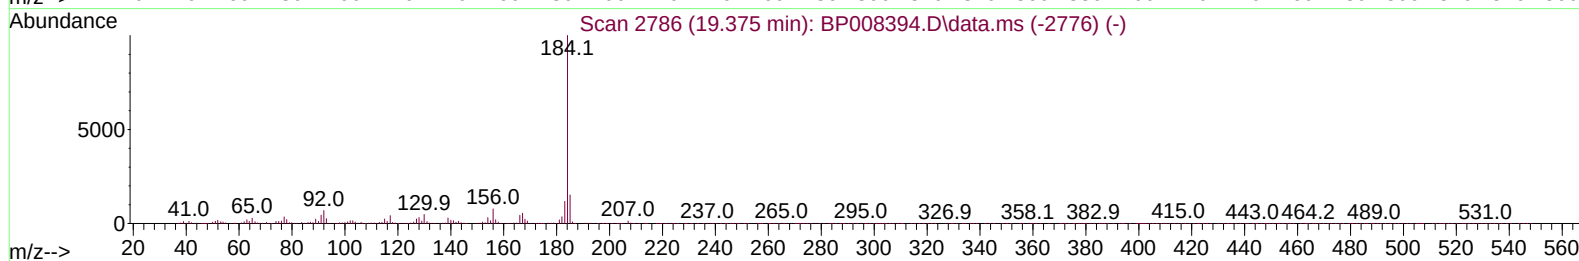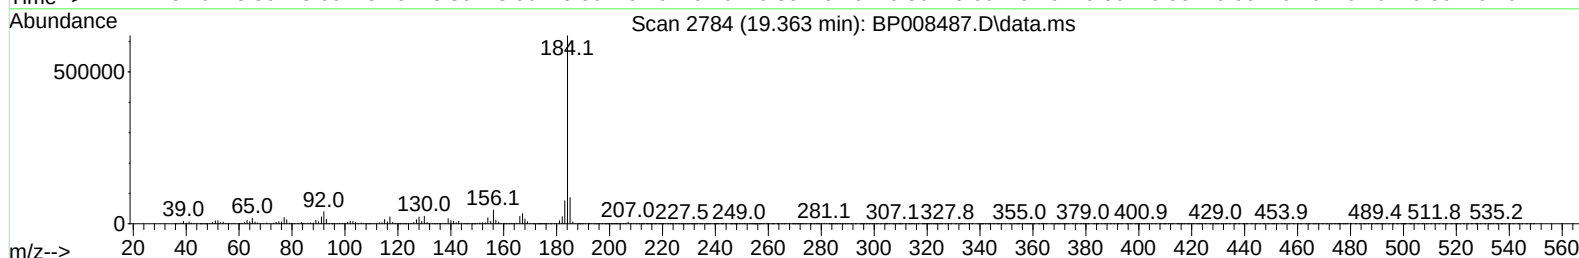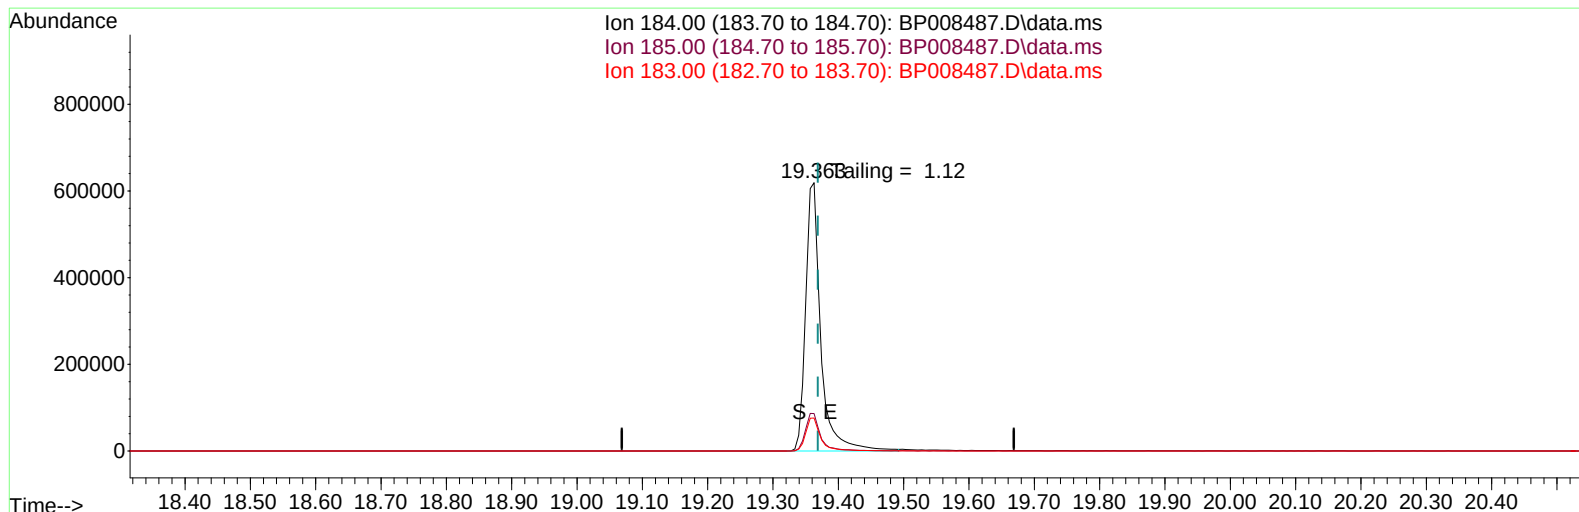

TIC: BP008487.D\data.ms

(77) Benzidine

19.363min (-0.006) 3422089.49 ng




response 1006645

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.95
183.00	11.40	12.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121821\
 Data File : BP008487.D
 Acq On : 18 Dec 2021 13:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 20 01:58:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 18 06:49:58 2021
 Response via : Initial Calibration

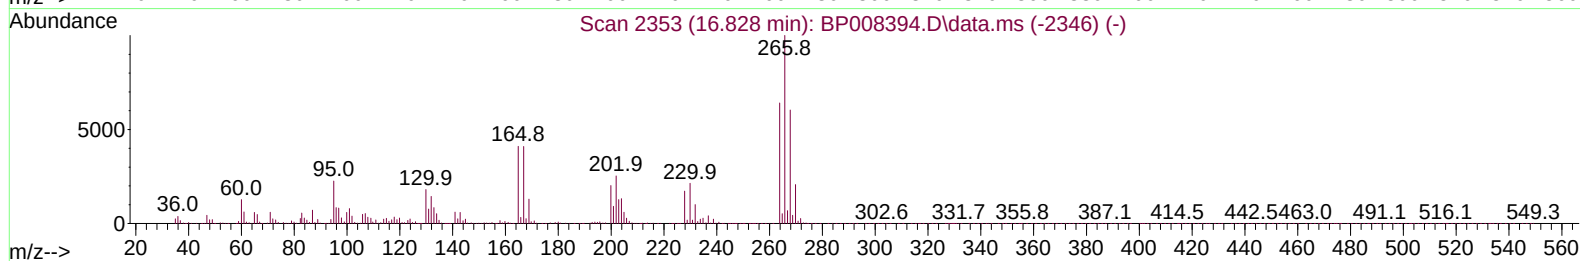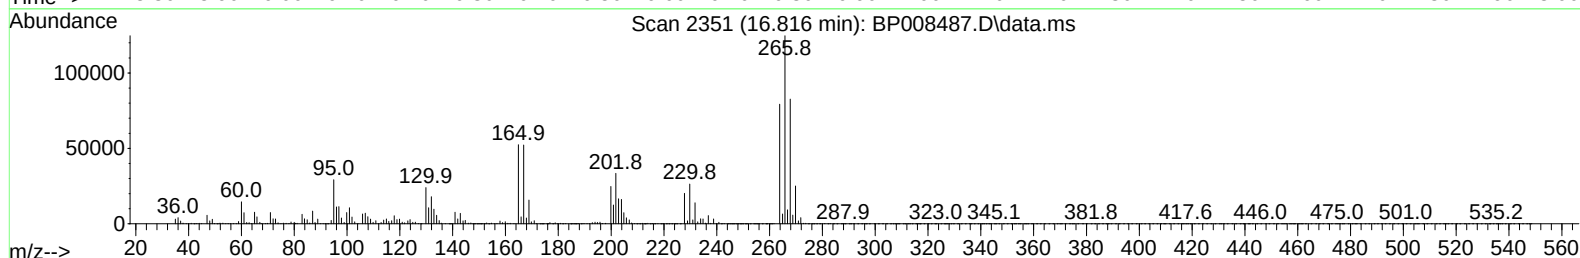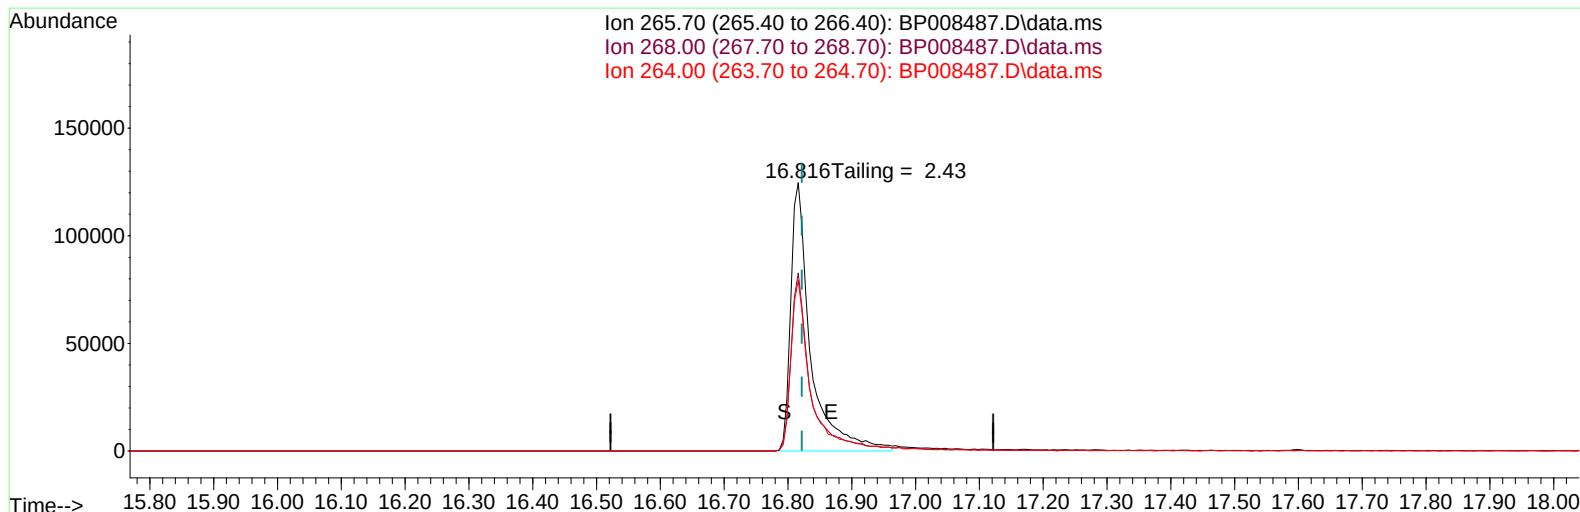

TIC: BP008487.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.006) 2406632.38 ng

response 277700

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.33
264.00	61.90	63.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/18/2021	BNA_P	<u>BP008487.D</u>
Compound Name	Response	Retention Time
DDT	585912	20.557
DDD	7575	20.175
DDE	2418	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9993	595905	1.68