

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018939.D
 Acq On : 19 Dec 2023 10:01
 Operator : MA/JU
 Sample : 05682-01 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLD6

Quant Time: Dec 19 21:39:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	197683	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	696402	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	412721	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	957561	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1008462	20.000	ng/ul	-0.01
88) Perylene-d12	23.674	264	1162208	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	16725	2.883	ng/uL	0.00
4) Pyridine-d5	3.681	84	205351	13.216	ng/ul	0.00
7) Phenol-d5	7.005	99	162057	8.169	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.169	67	387081	32.921	ng/ul	0.00
11) 2-Chlorophenol-d4	7.364	132	436751	28.214	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	271217	16.893	ng/ul	-0.01
21) Nitrobenzene-d5	8.993	128	262647	42.375	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	279978	43.569	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	477409	36.333	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	565889	32.953	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	1478141	40.128	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	1726694	42.570	ng/ul	0.00
54) 4-Nitrophenol-d4	14.687	143	52777	8.729	ng/ul	0.00
60) Fluorene-d10	15.457	176	1342665	43.424	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.587	200	125604	21.876	ng/ul	0.00
73) Anthracene-d10	17.310	188	2270352	45.100	ng/ul	0.00
81) Pyrene-d10	19.551	212	2893082	36.854	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.522	264	2982950	44.019	ng/ul	-0.01
Target Compounds						
72) Phenanthrene	17.257	178	110037	1.903	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018939.D
Acq On : 19 Dec 2023 10:01
Operator : MA/JU
Sample : 05682-01 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLD6

Quant Time: Dec 19 21:39:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 19 05:28:03 2023
Response via : Initial Calibration

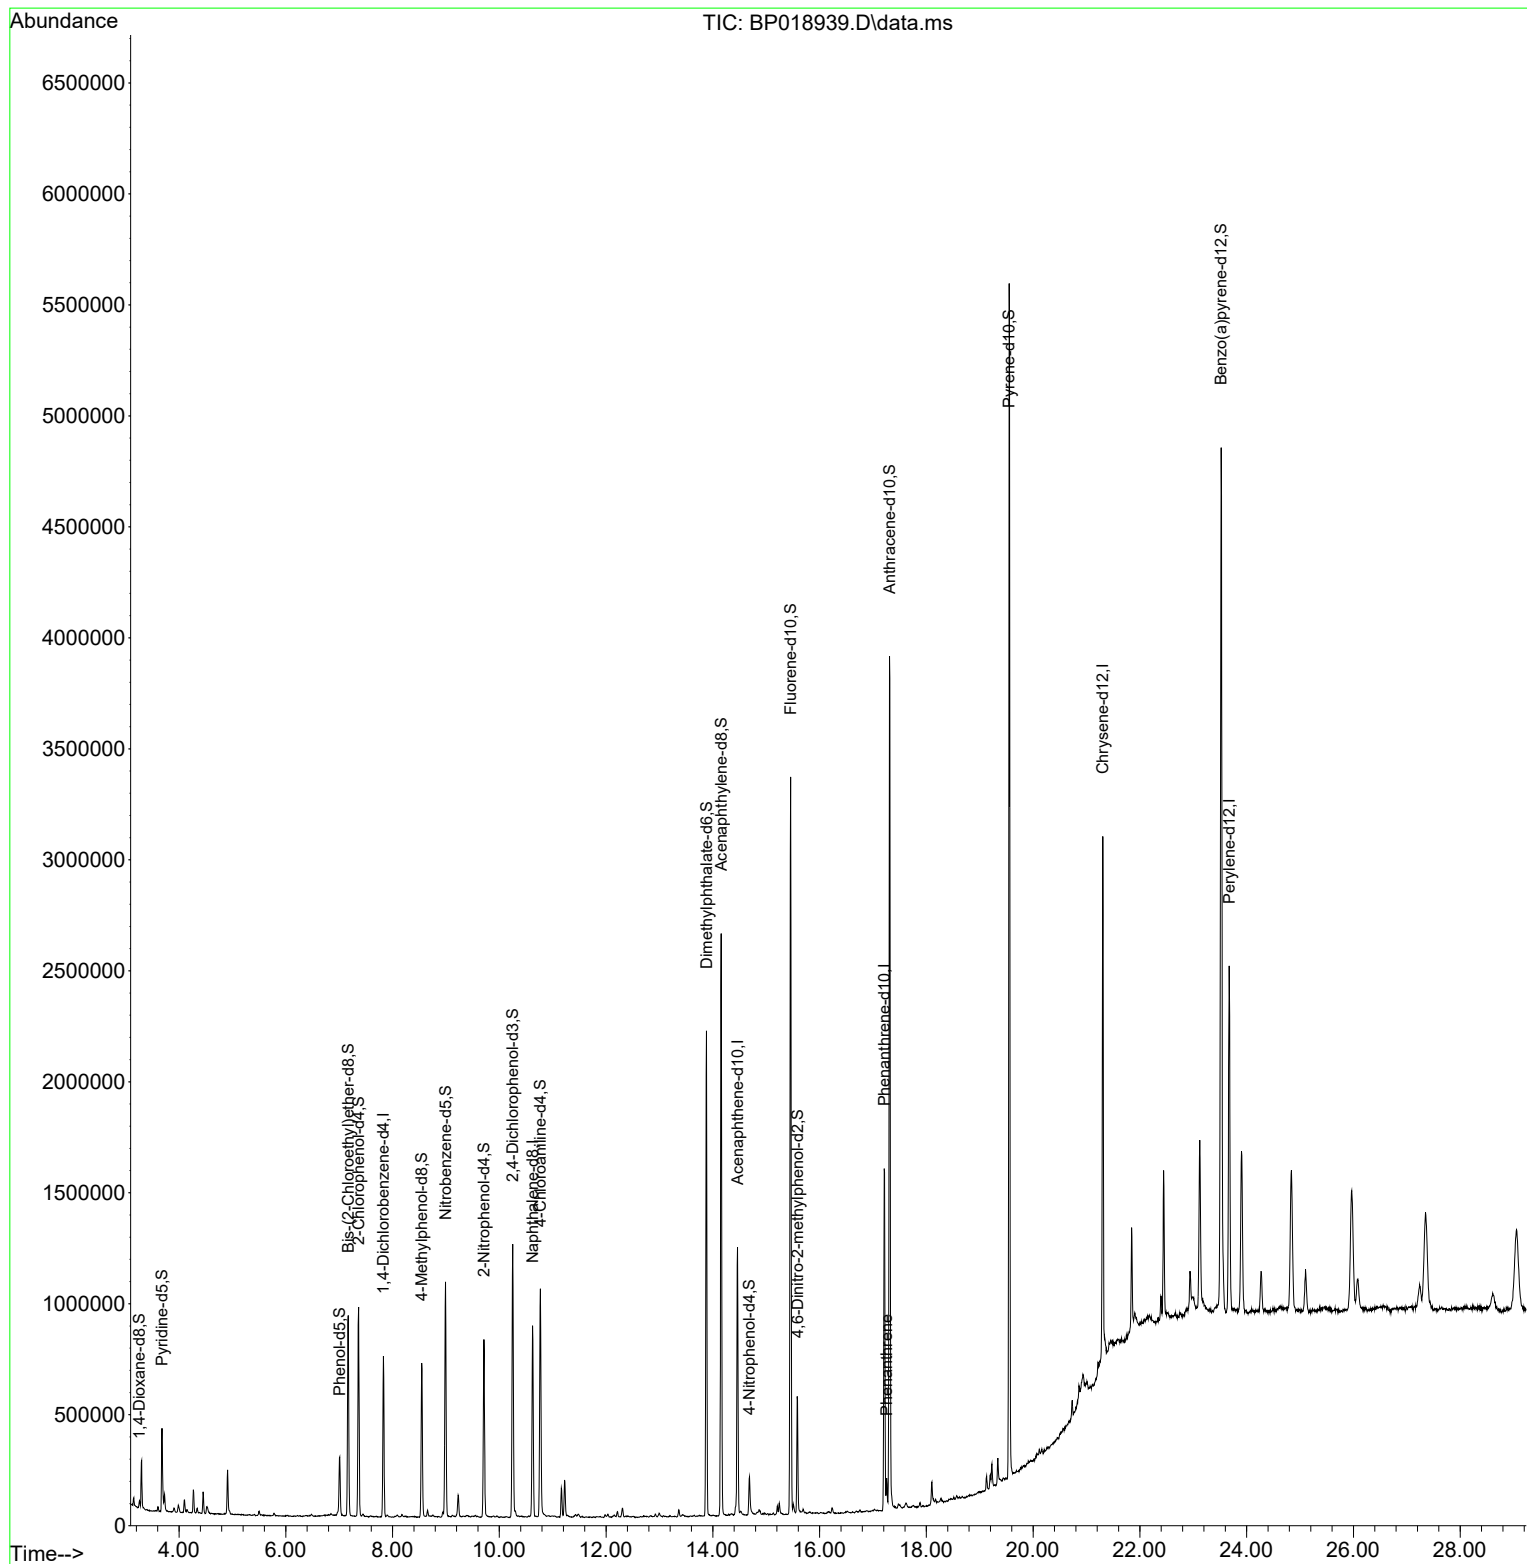

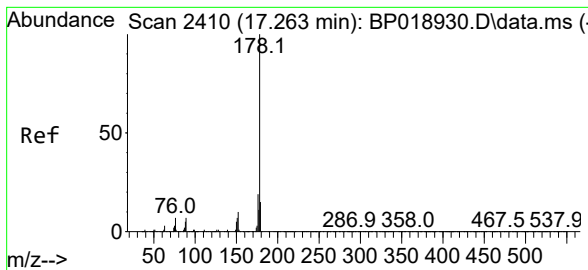

#72
 Phenanthrene
 Concen: 1.903 ng/ul
 RT: 17.257 min Scan# 2410
 Delta R.T. -0.006 min
 Lab File: BP018939.D
 Acq: 19 Dec 2023 10:01

Instrument :
 BNA_P
 ClientSampleId :
 DCLD6

Tgt Ion:	178	Resp:	110037
Ion Ratio	Lower	Upper	
178	100		
179	15.2	12.3	18.5
176	18.0	15.4	23.2

