

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018943.D
 Acq On : 19 Dec 2023 12:17
 Operator : MA/JU
 Sample : 05823-01 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AW7

Quant Time: Dec 19 21:40:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	195753	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	765392	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.463	164	497612	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1142620	20.000	ng/ul	0.00
79) Chrysene-d12	21.304	240	1136943	20.000	ng/ul	-0.01
88) Perylene-d12	23.674	264	1311500	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	11995	2.088	ng/uL	0.00
4) Pyridine-d5	3.681	84	146621	9.529	ng/ul	0.00
7) Phenol-d5	7.005	99	126616	6.445	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.169	67	302111	25.948	ng/ul	0.00
11) 2-Chlorophenol-d4	7.363	132	339301	22.135	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	219550	13.810	ng/ul	-0.01
21) Nitrobenzene-d5	8.993	128	210716	30.932	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	225474	31.925	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	403780	27.959	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	455018	24.109	ng/ul	0.00
46) Dimethylphthalate-d6	13.881	166	1355145	30.513	ng/ul	0.00
49) Acenaphthylene-d8	14.157	160	1574193	32.189	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	48473	6.649	ng/ul	0.00
60) Fluorene-d10	15.457	176	1264506	33.919	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	100636	14.689	ng/ul	-0.01
73) Anthracene-d10	17.310	188	2194324	36.530	ng/ul	0.00
81) Pyrene-d10	19.551	212	2682165	30.306	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.521	264	2770451	36.229	ng/ul	-0.01
Target Compounds						
					Qvalue	
30) Naphthalene	10.675	128	71507	1.540	ng/ul	99
47) Dimethylphthalate	13.922	163	48894	1.118	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018943.D
Acq On : 19 Dec 2023 12:17
Operator : MA/JU
Sample : 05823-01 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AW7

Quant Time: Dec 19 21:40:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 19 05:28:03 2023
Response via : Initial Calibration




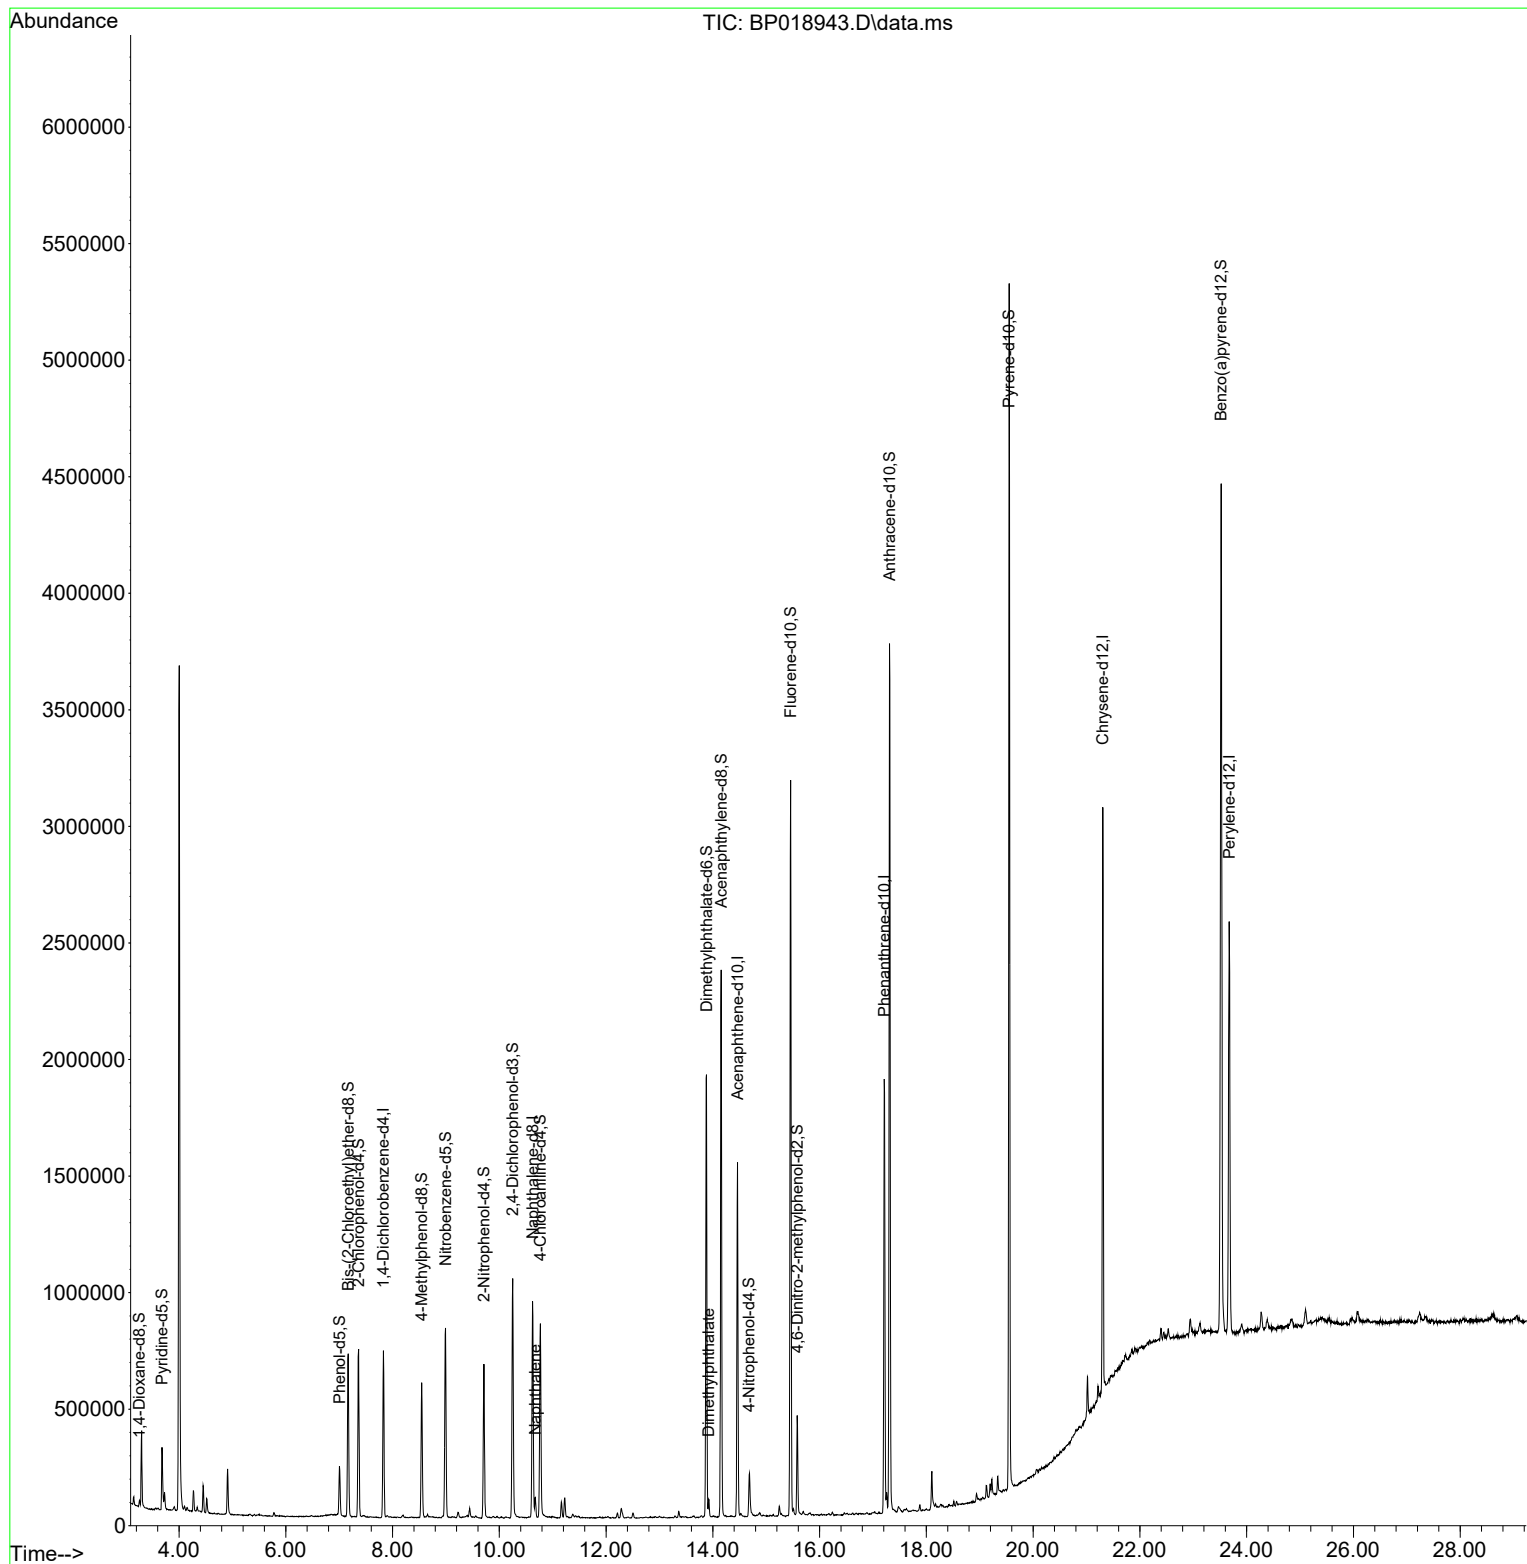


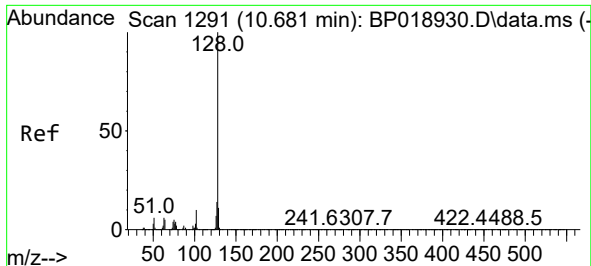

#30
Naphthalene
Concen: 1.540 ng/ul
RT: 10.675 min Scan# 1290
Delta R.T. -0.006 min
Lab File: BP018943.D
Acq: 19 Dec 2023 12:17

Instrument :
BNA_P
ClientSampleId :
C0AW7

Tgt Ion:128 Resp: 71507
Ion Ratio Lower Upper
128 100
129 10.8 8.9 13.3
127 12.5 10.5 15.7

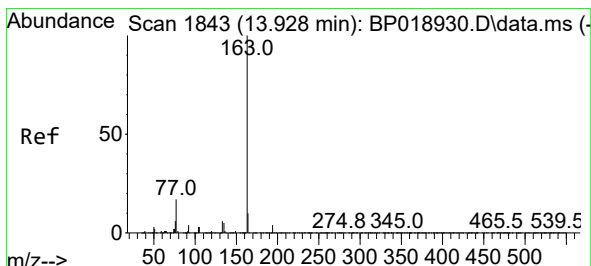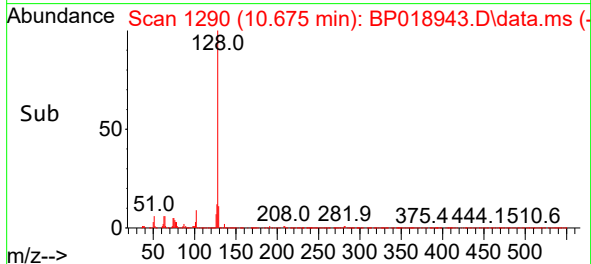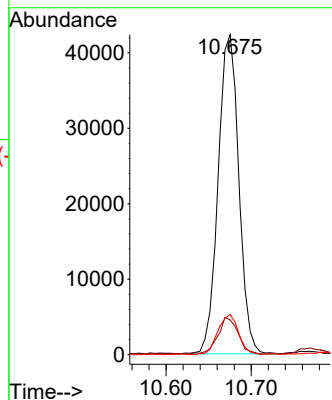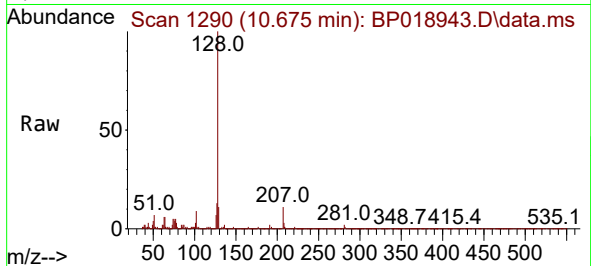

#47
Dimethylphthalate
Concen: 1.118 ng/ul
RT: 13.922 min Scan# 1842
Delta R.T. -0.006 min
Lab File: BP018943.D
Acq: 19 Dec 2023 12:17

Tgt Ion:163 Resp: 48894
Ion Ratio Lower Upper
163 100
194 3.9 3.2 4.8
164 10.4 8.0 12.0

