

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 21:38:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

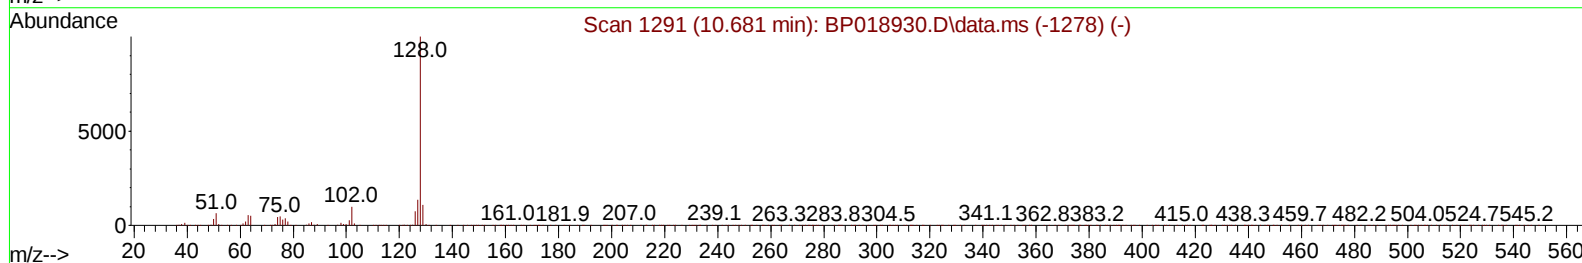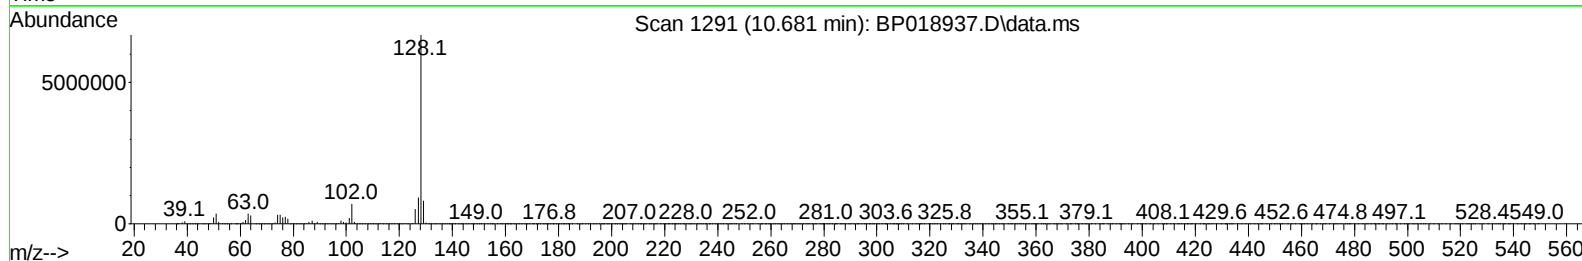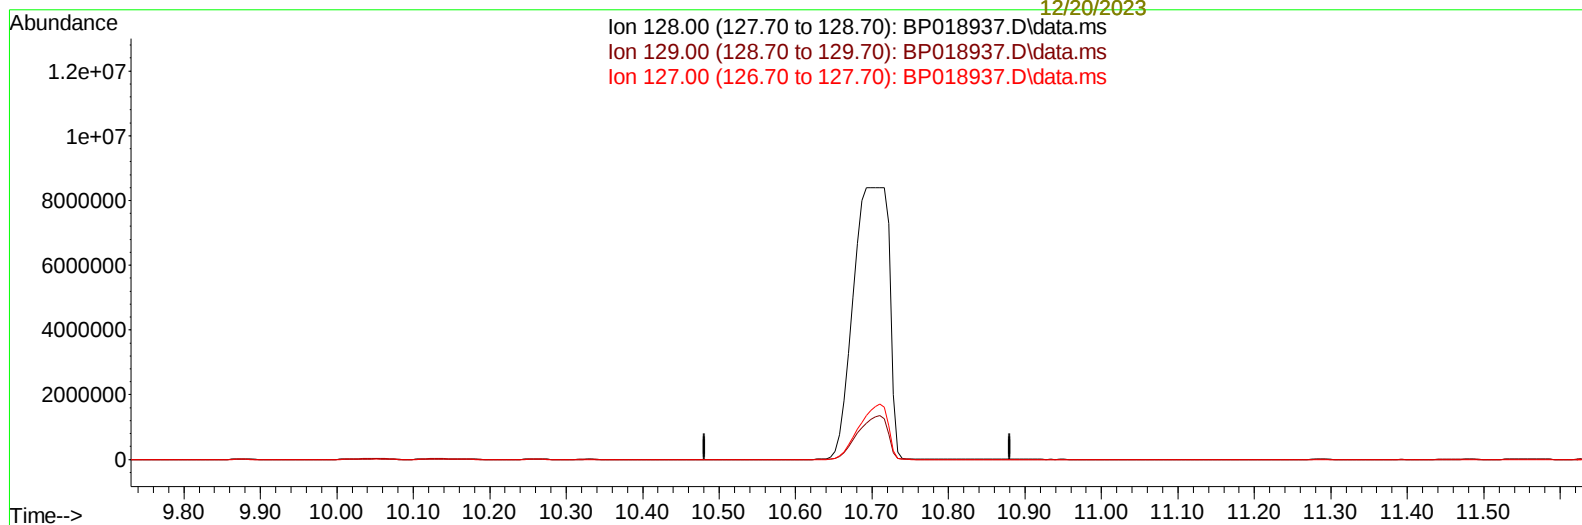

TIC: BP018937.D\data.ms

(30) Naphthalene

10.681min (-10.681) 0.00 ng/u1

response 0

Ion	Exp%	Act%
128.00	100.00	0.00
129.00	11.10	0.00#
127.00	13.10	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 21:38:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

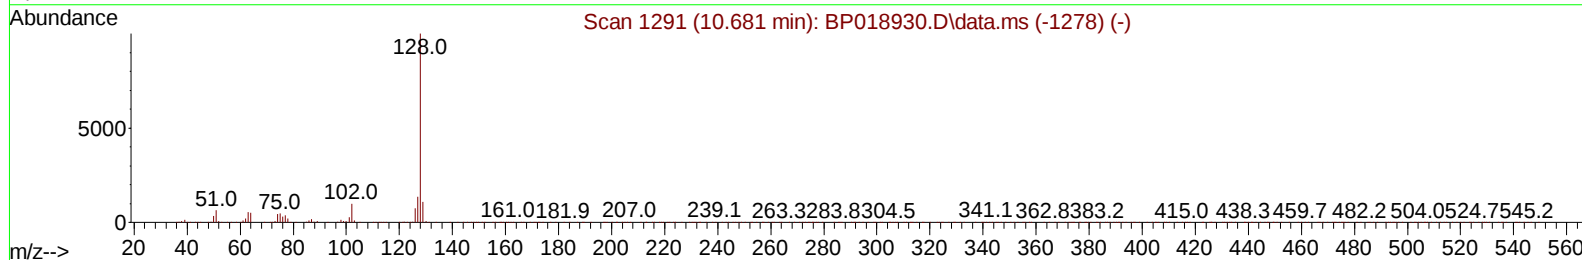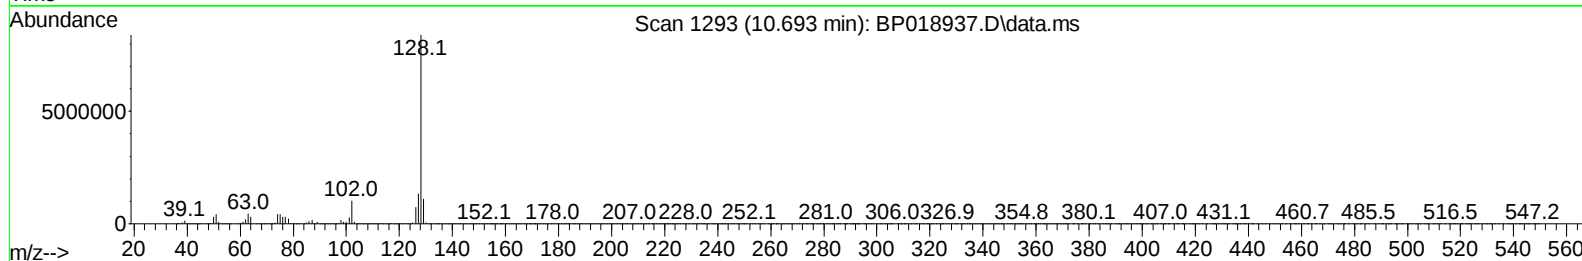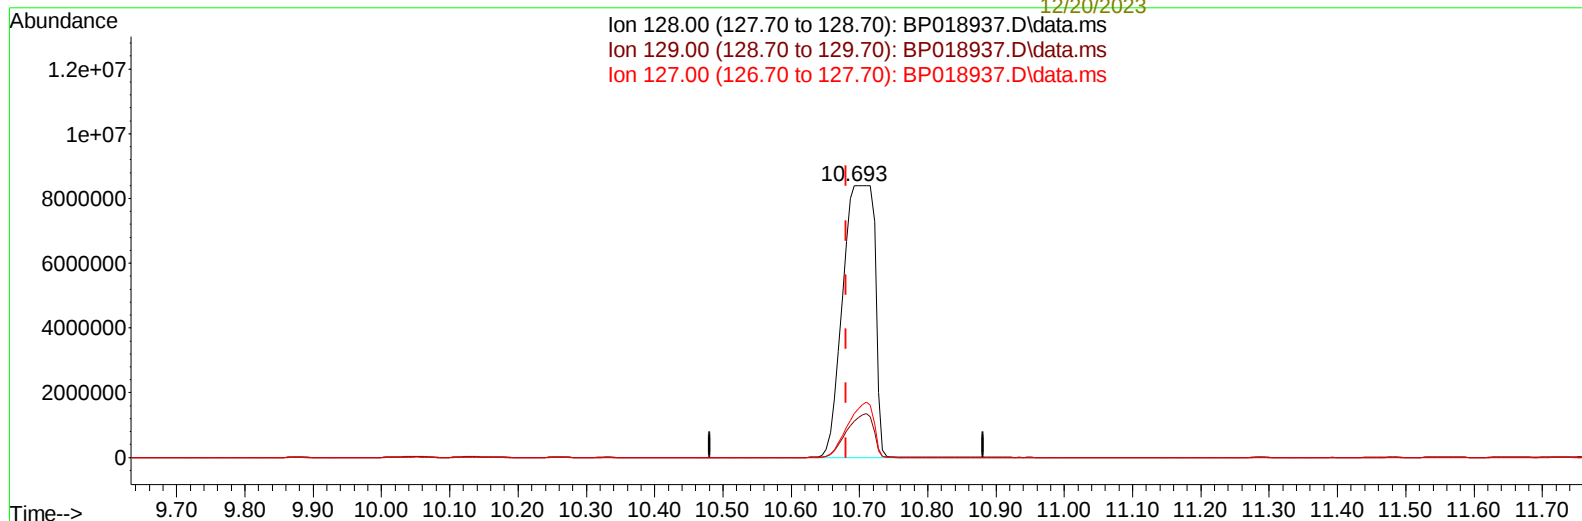

TIC: BP018937.D\data.ms

(30) Naphthalene

10.693min (+ 0.012) 609.77 ng/u1 m

response 27316913

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	11.10	13.39#
127.00	13.10	16.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Quant Time: Dec 19 21:56:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Supervised By :mohammad
 ahmed
 12/20/2023

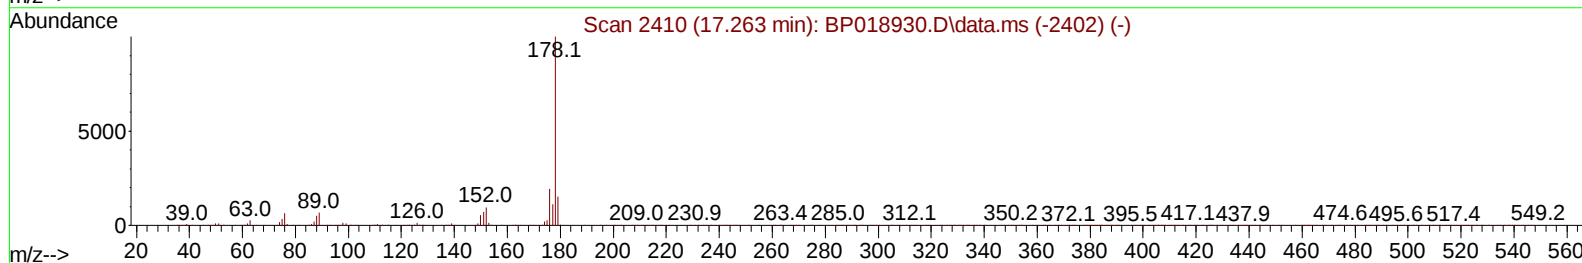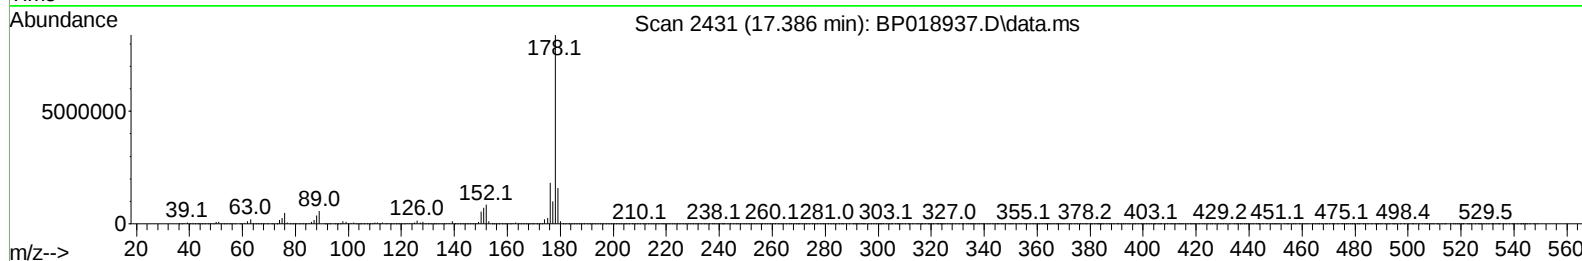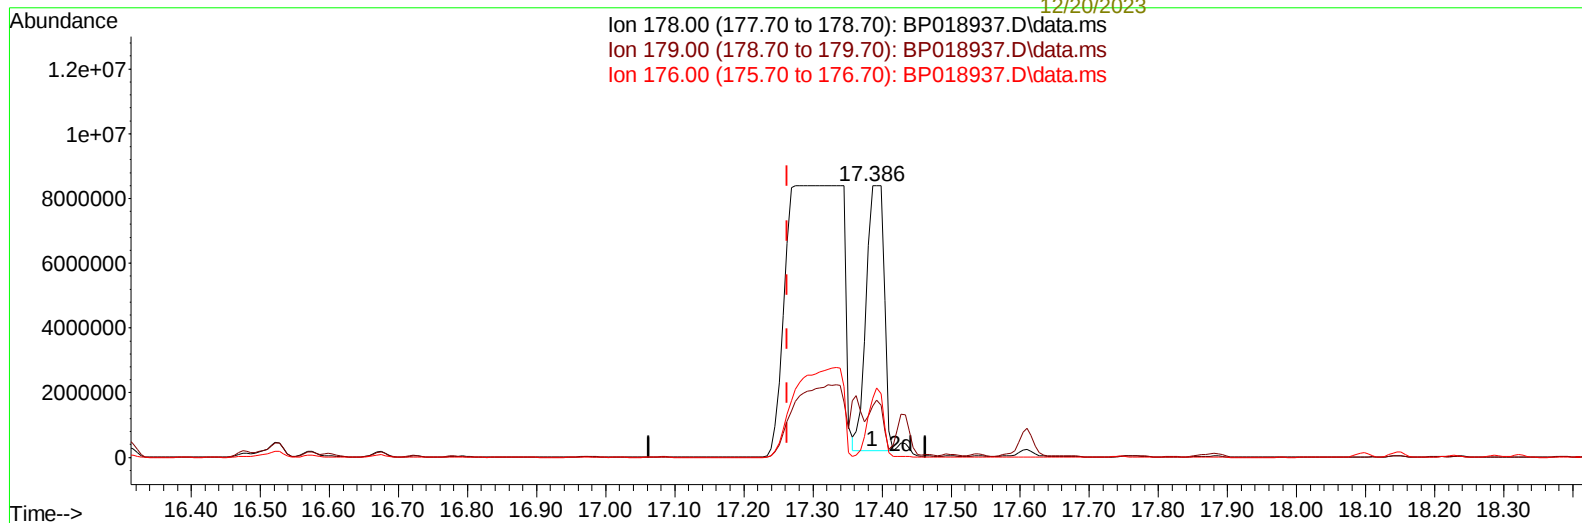

TIC: BP018937.D\data.ms

(72) Phenanthrene

17.386min (+ 0.124) 271.67 ng/u1

response 14582076

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.40	18.90#
176.00	19.30	21.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Quant Time: Dec 19 21:56:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Supervised By :mohammad
 ahmed
 12/20/2023

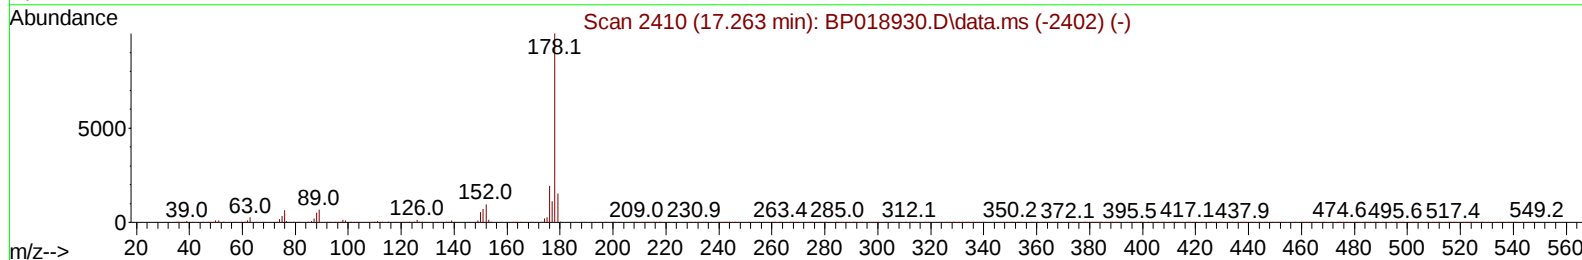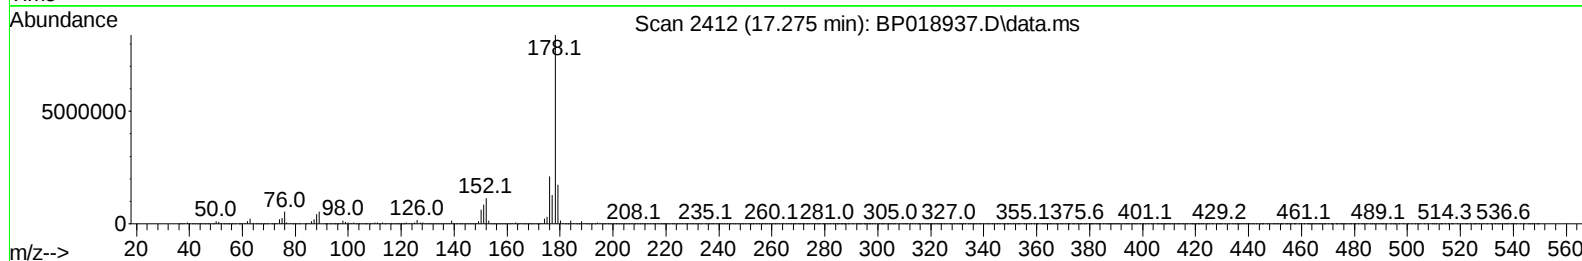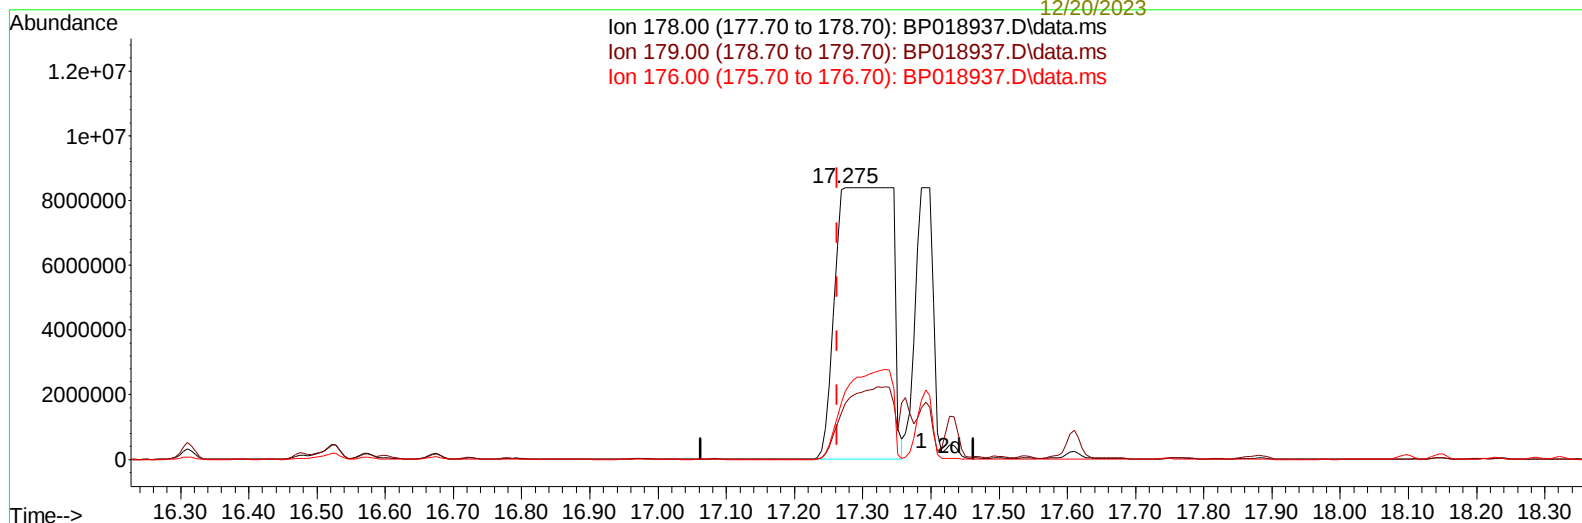

TIC: BP018937.D\data.ms

(72) Phenanthrene

17.275min (+ 0.012) 877.61 ng/u1 m

response 47106724

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.40	20.67#
176.00	19.30	25.17#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL




Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 21:58:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Ion 188.00 (187.70 to 188.70): BP018937.D\data.ms
 Ion 94.00 (93.70 to 94.70): BP018937.D\data.ms
 Ion 80.00 (79.70 to 80.70): BP018937.D\data.ms

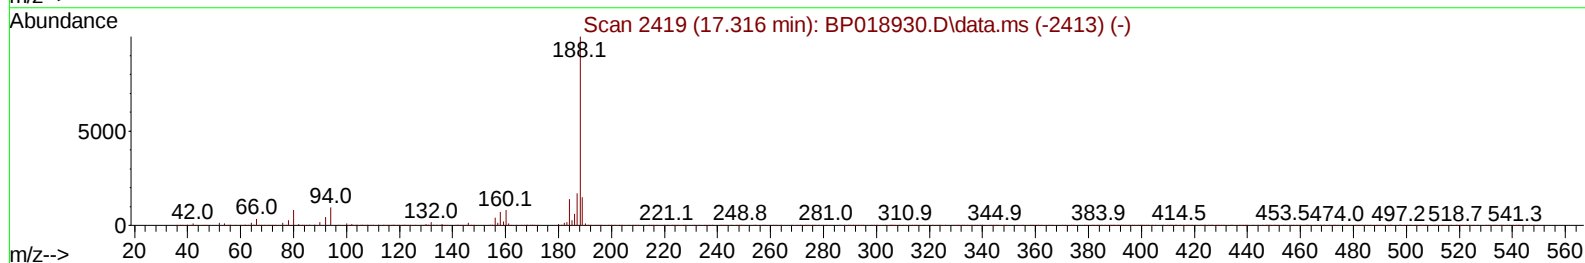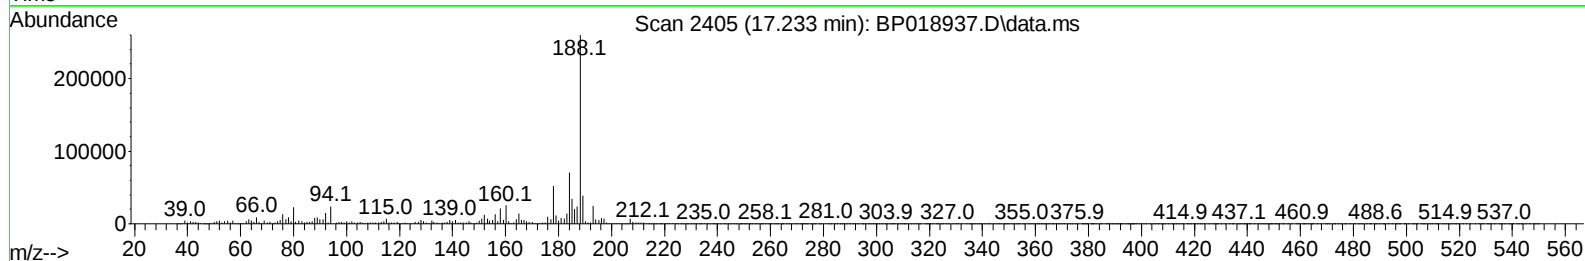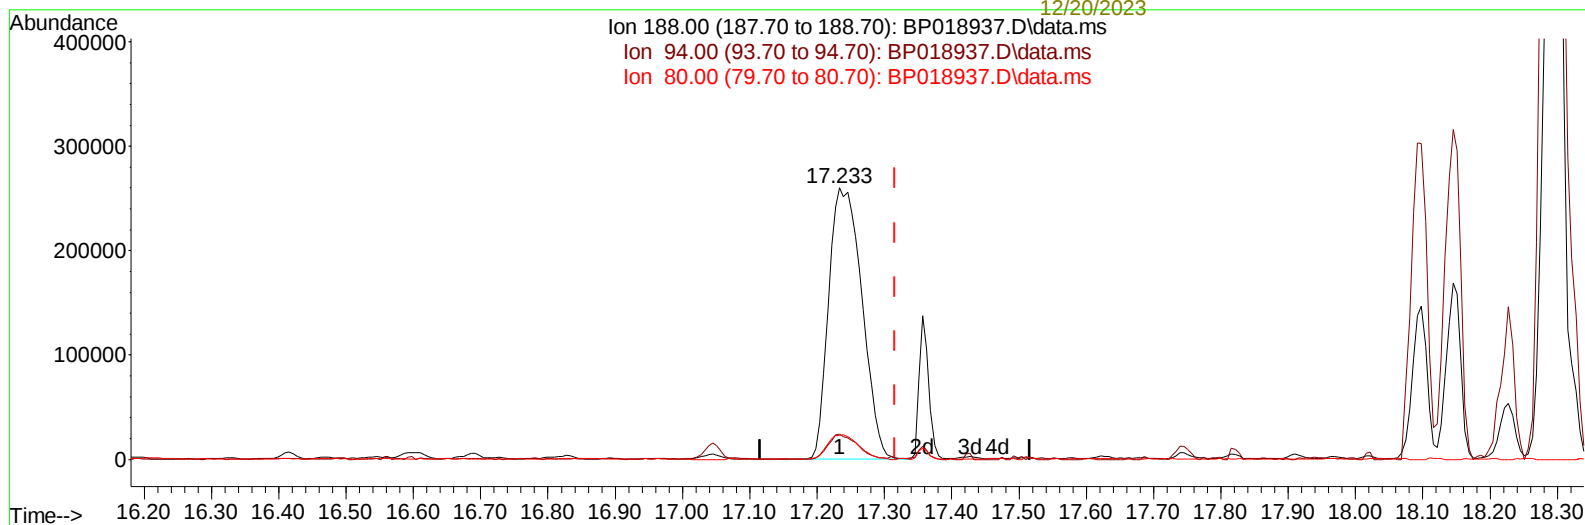

TIC: BP018937.D\data.ms

(73) Anthracene-d10 (S)

17.233min (-0.082) 19.02 ng/u1

response 888742

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.30	9.24
80.00	10.20	9.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018937.D
Acq On : 19 Dec 2023 08:53
Operator : MA/JU
Sample : 05626-10DL 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1




Instrument :
BNA_P
ClientSampleId :
DCLF6DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 21:58:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 19 05:28:03 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/20/2023
Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
ahmed
12/20/2023

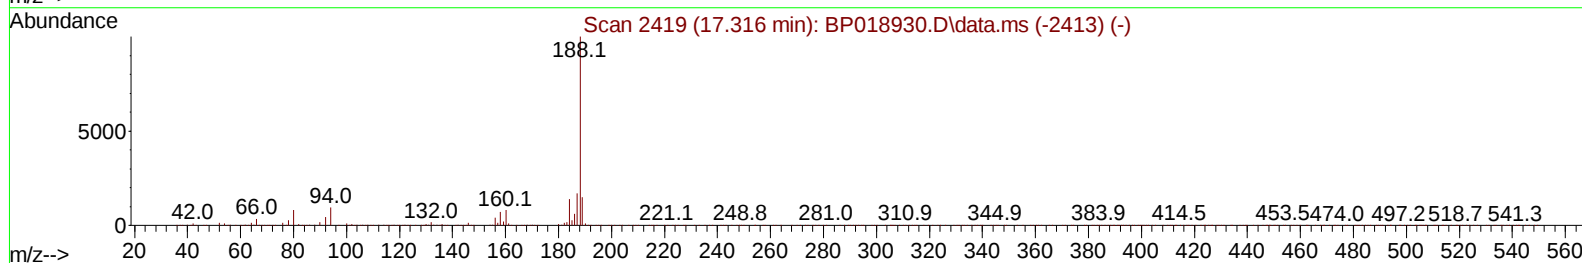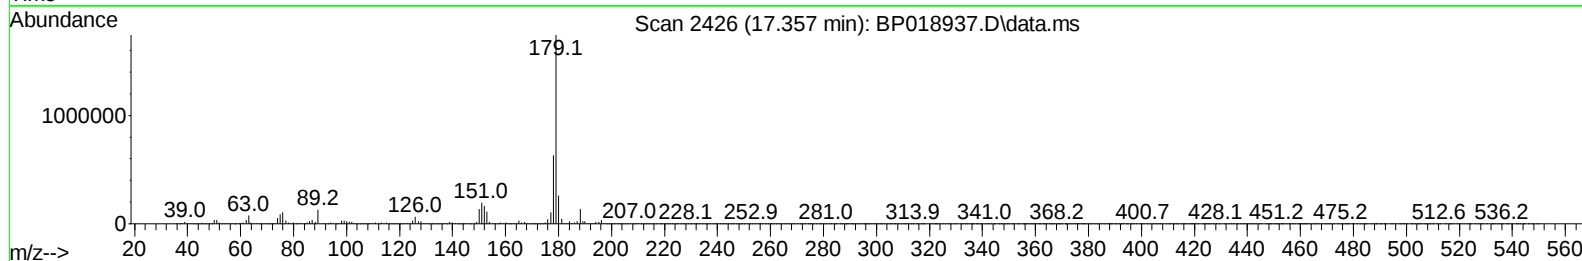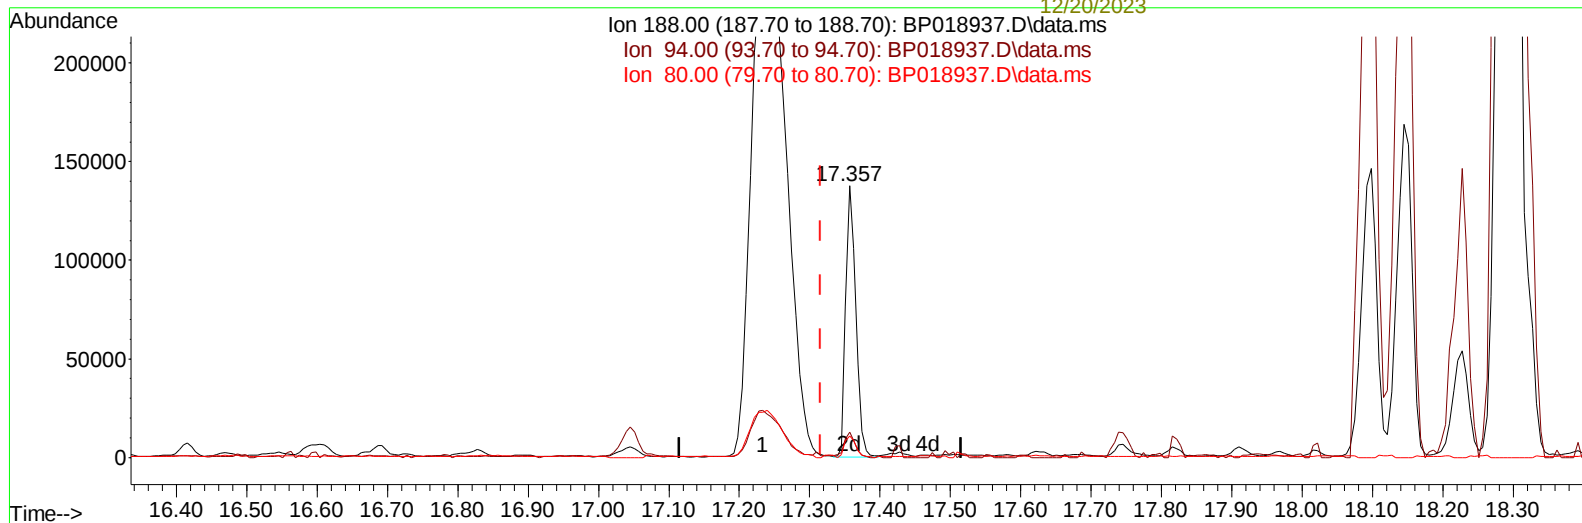

TIC: BP018937.D\data.ms

(73) Anthracene-d10 (S)

17.357min (+ 0.041) 2.94 ng/u1 m

response 137581

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.30	9.25
80.00	10.20	7.85#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 21:58:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

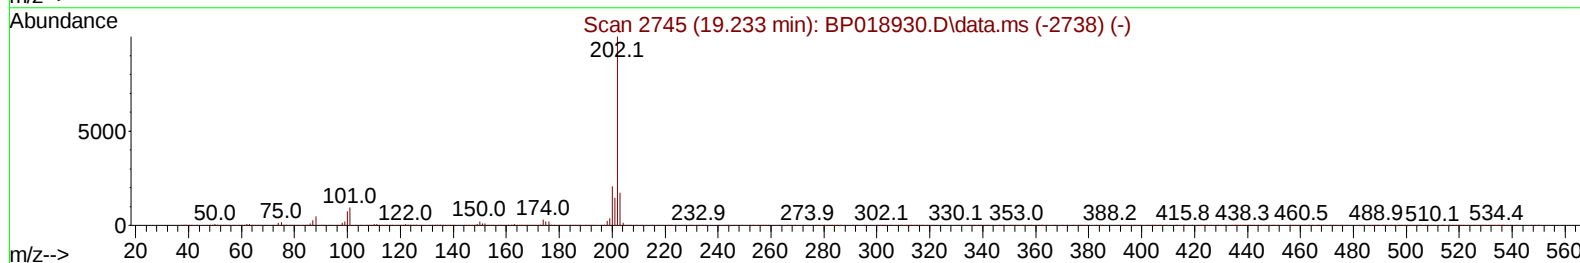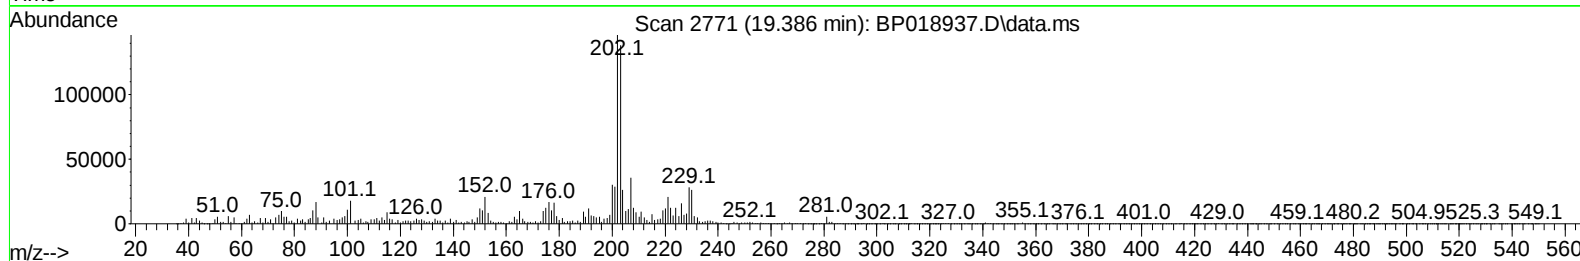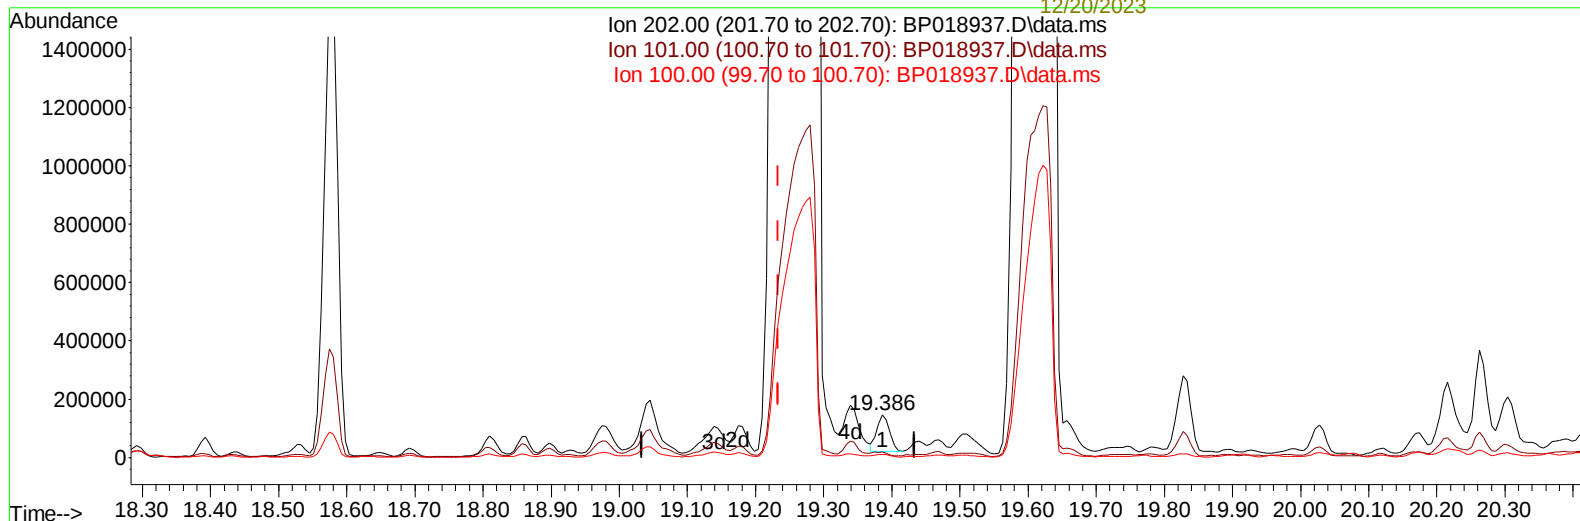

TIC: BP018937.D\data.ms

(80) Fluoranthene

19.386min (+ 0.153) 1.86 ng/u1

response 160917

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.40	12.31
100.00	8.90	7.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Quant Time: Dec 19 21:58:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Supervised By :mohammad
 ahmed
 12/20/2023

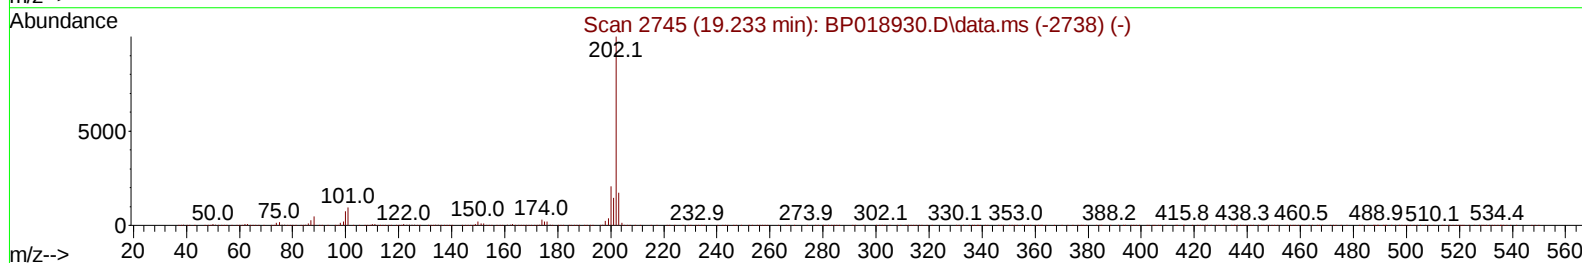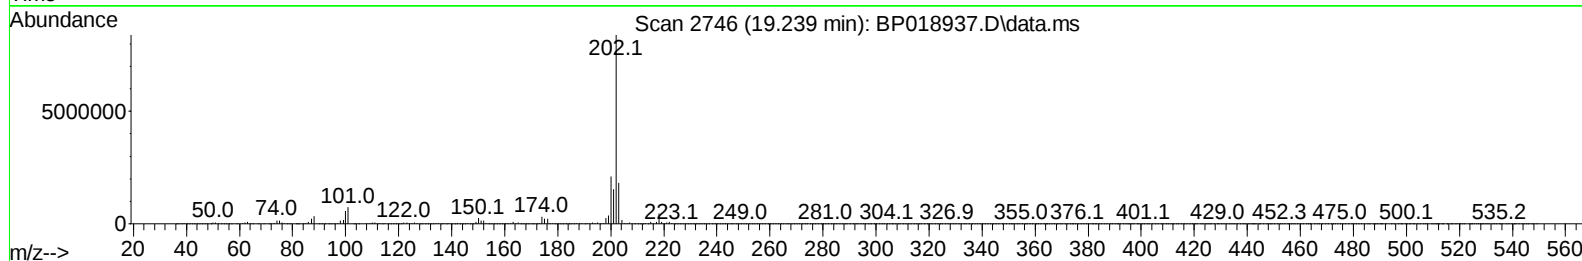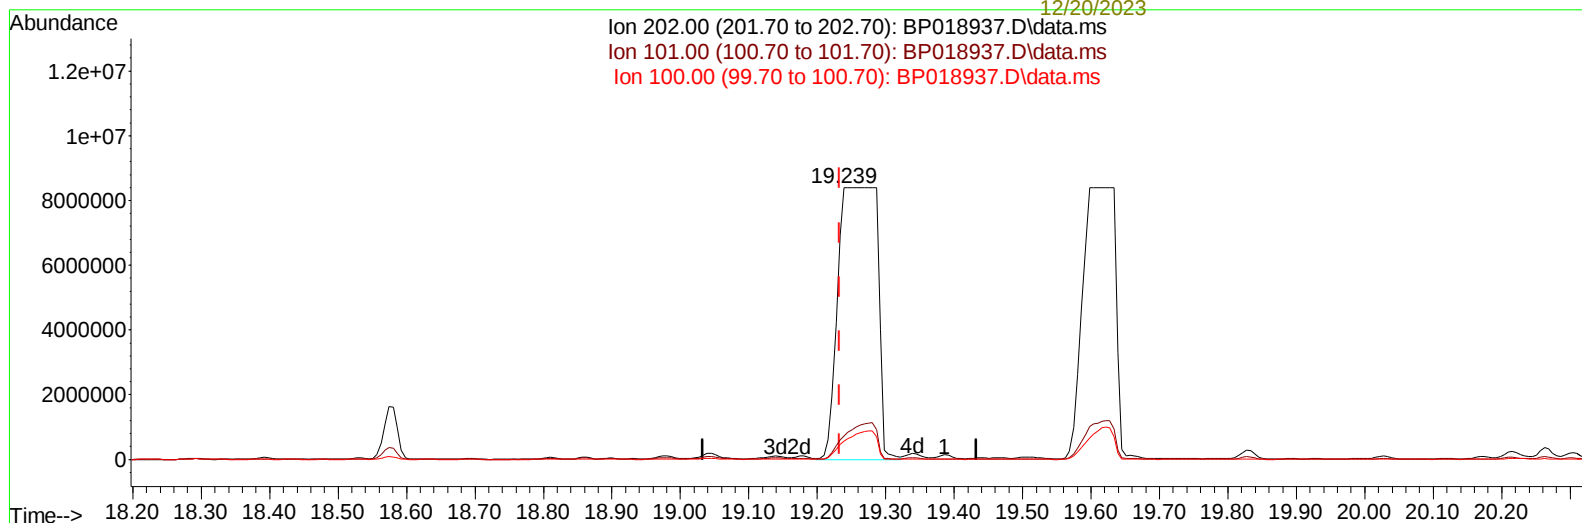

TIC: BP018937.D\data.ms

(80) Fluoranthene

19.239min (+ 0.006) 384.02 ng/u1 m

response 33192875

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.40	8.72#
100.00	8.90	6.72#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 21:59:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

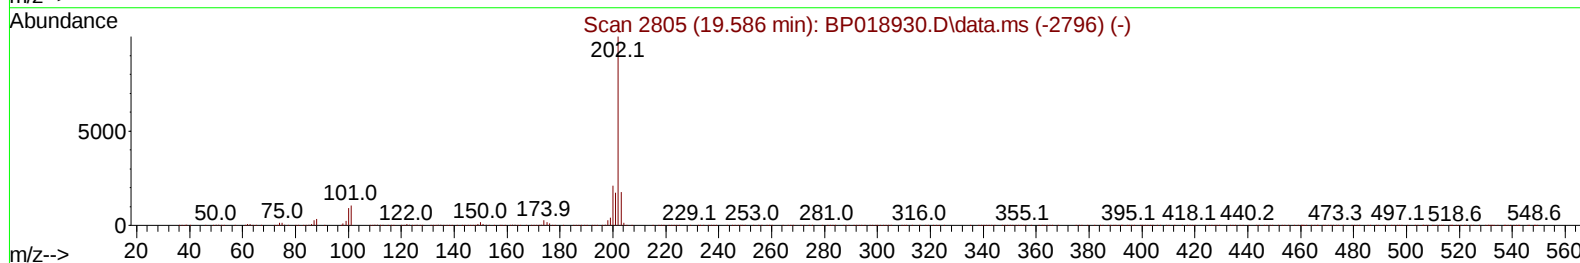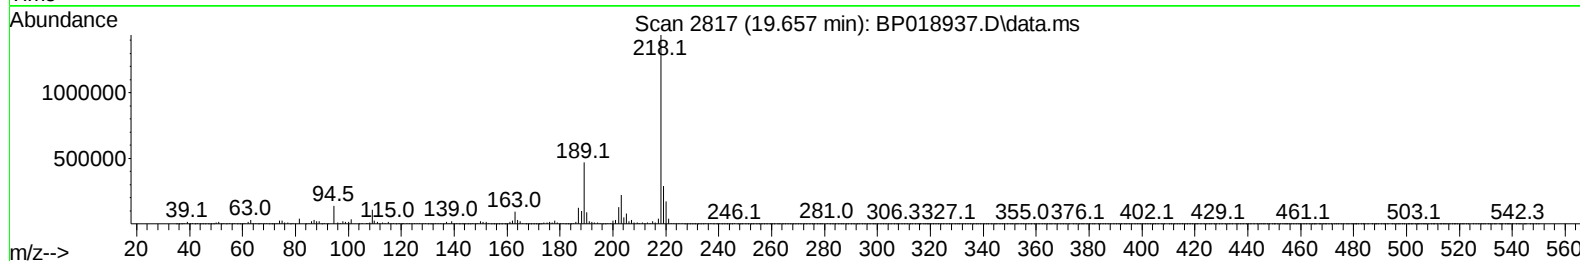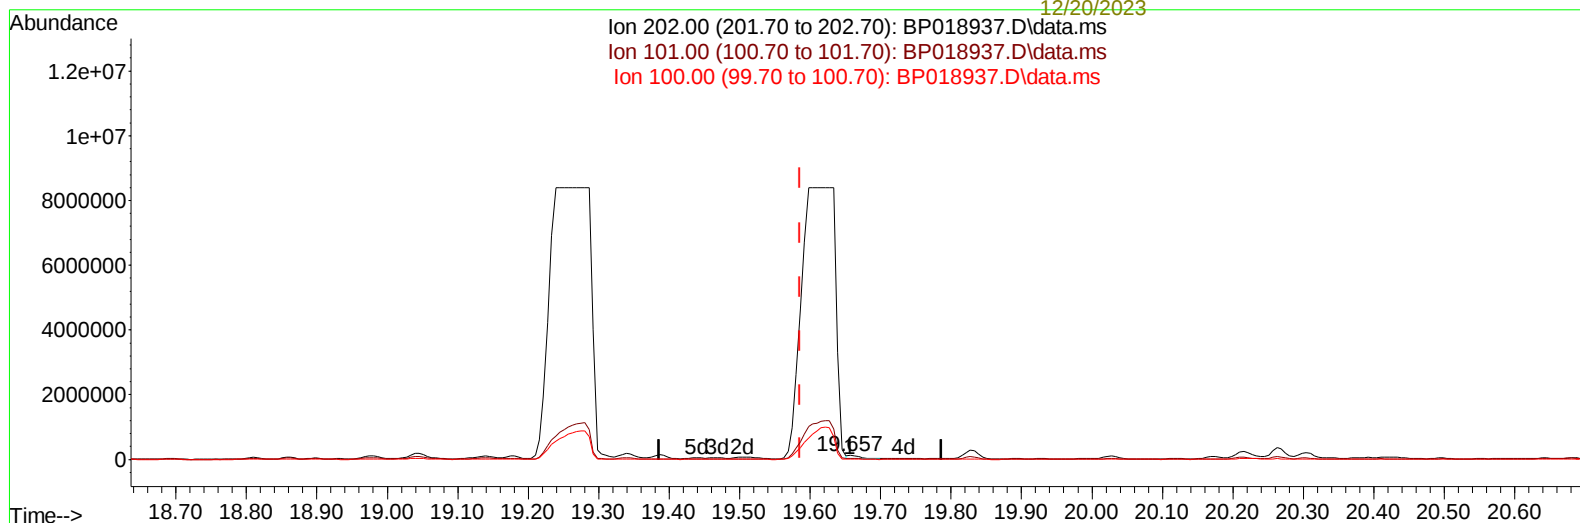

TIC: BP018937.D\data.ms

(82) Pyrene

19.657min (+ 0.071) 1.27 ng/u1

response 110645

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.70	25.88#
100.00	11.40	11.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Quant Time: Dec 19 21:59:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Supervised By :mohammad
 ahmed
 12/20/2023

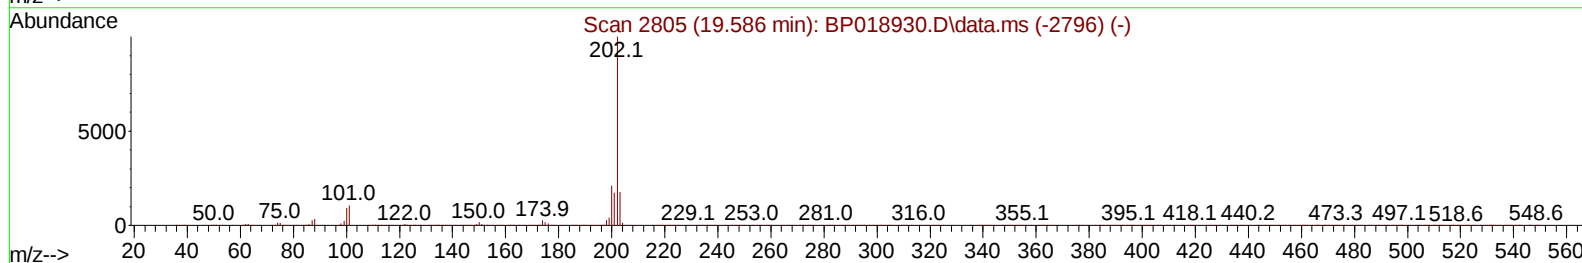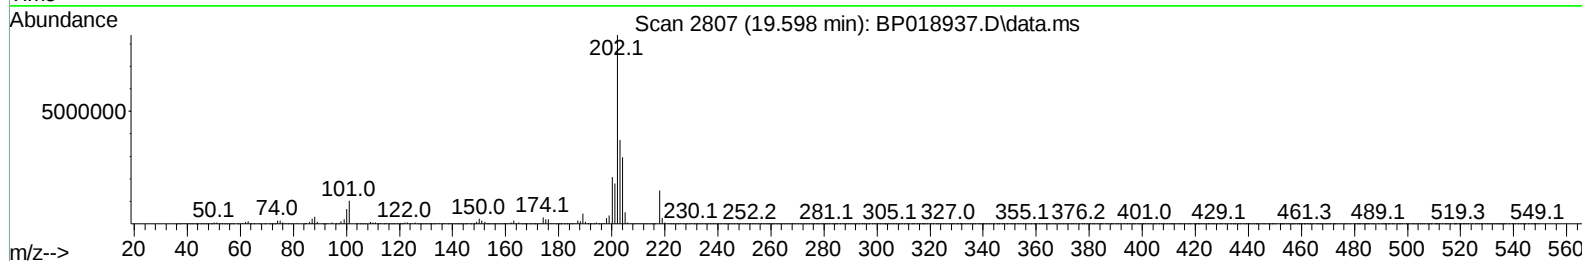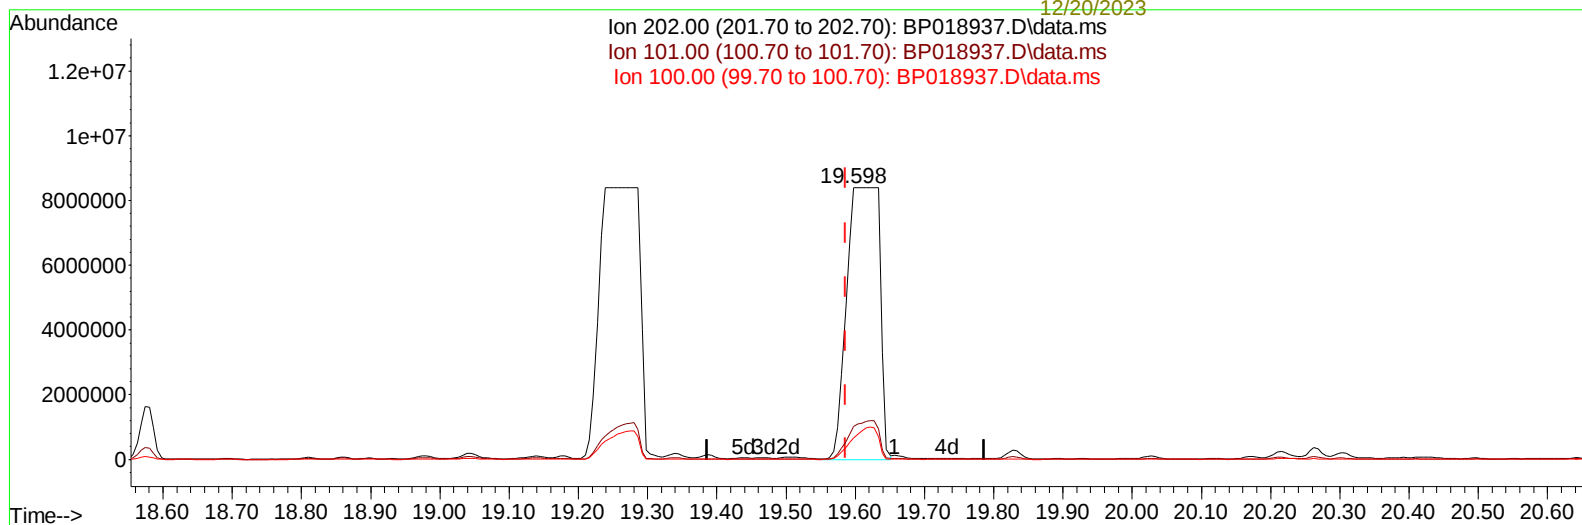

TIC: BP018937.D\data.ms

(82) Pyrene

19.598min (+ 0.012) 314.66 ng/u1 m

response 27437906

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.70	12.14
100.00	11.40	7.92#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL




Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 21:59:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Ion 228.00 (227.70 to 228.70): BP018937.D\data.ms
 Ion 226.00 (225.70 to 226.70): BP018937.D\data.ms
 Ion 229.00 (228.70 to 229.70): BP018937.D\data.ms

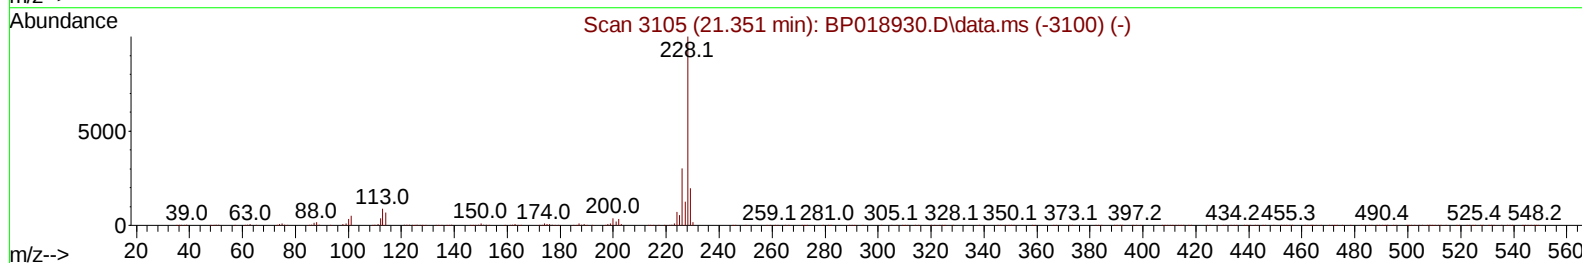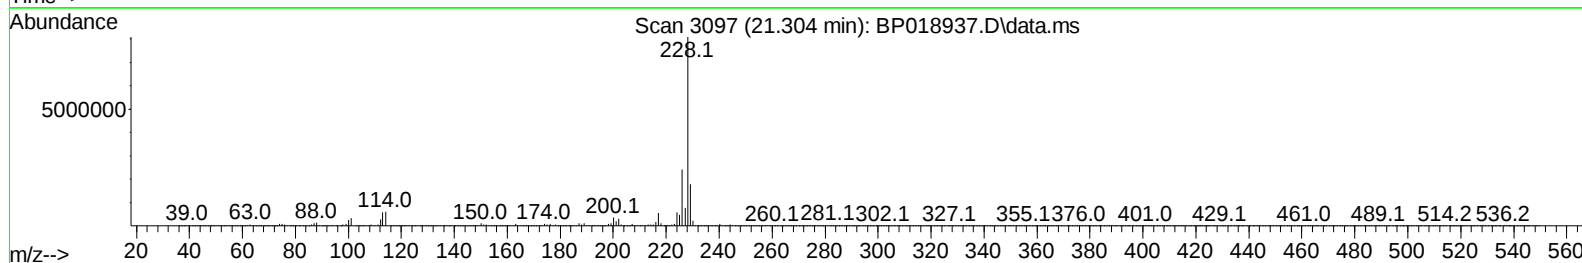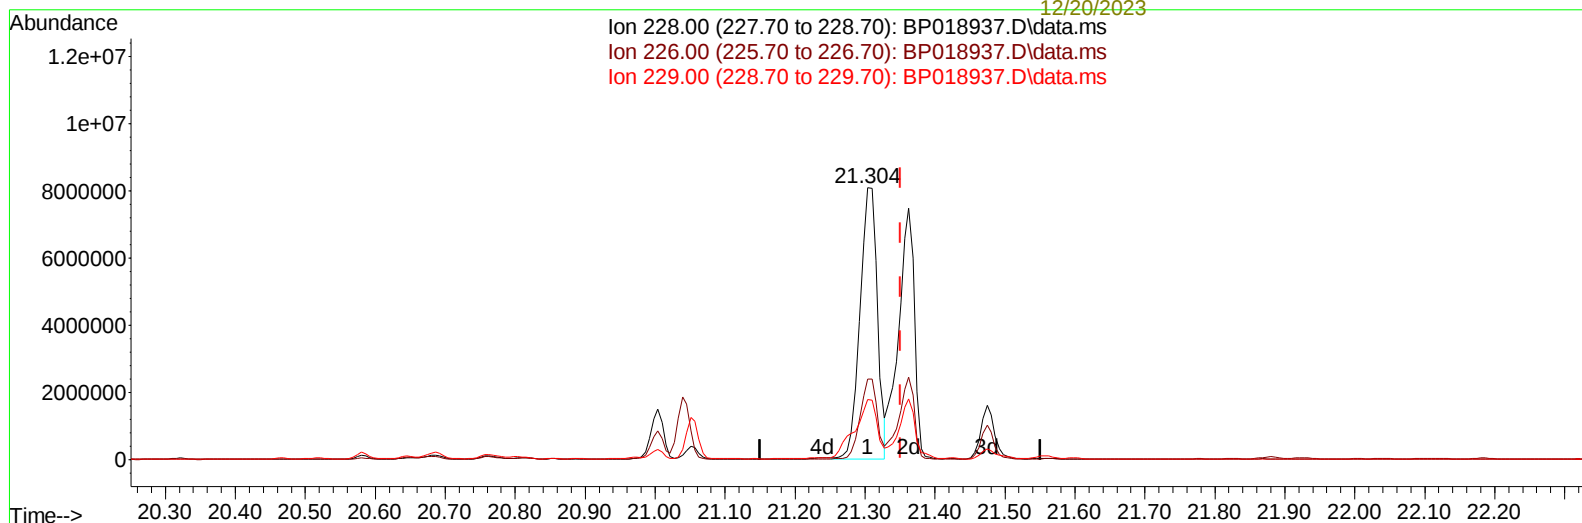

TIC: BP018937.D\data.ms

(87) Chrysene

21.304min (-0.047) 198.76 ng/u1

response 13956265

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.90	29.69
229.00	19.50	21.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL




Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 21:59:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Ion 228.00 (227.70 to 228.70): BP018937.D\data.ms
 Ion 226.00 (225.70 to 226.70): BP018937.D\data.ms
 Ion 229.00 (228.70 to 229.70): BP018937.D\data.ms

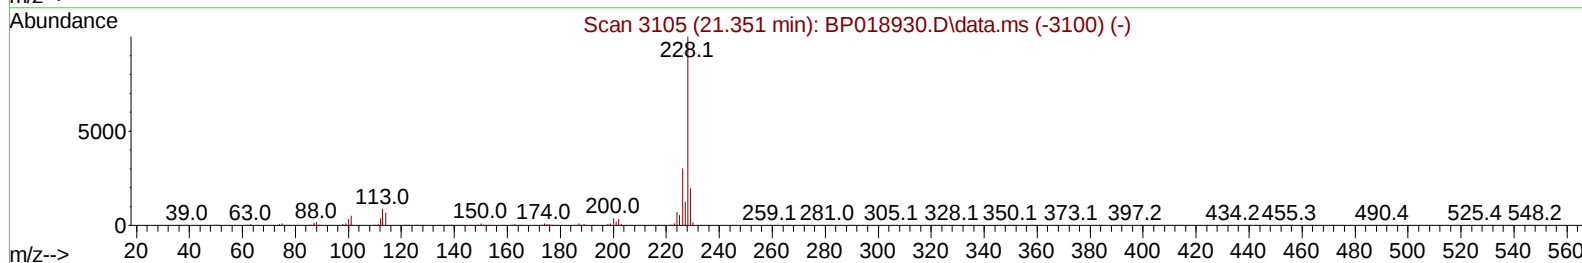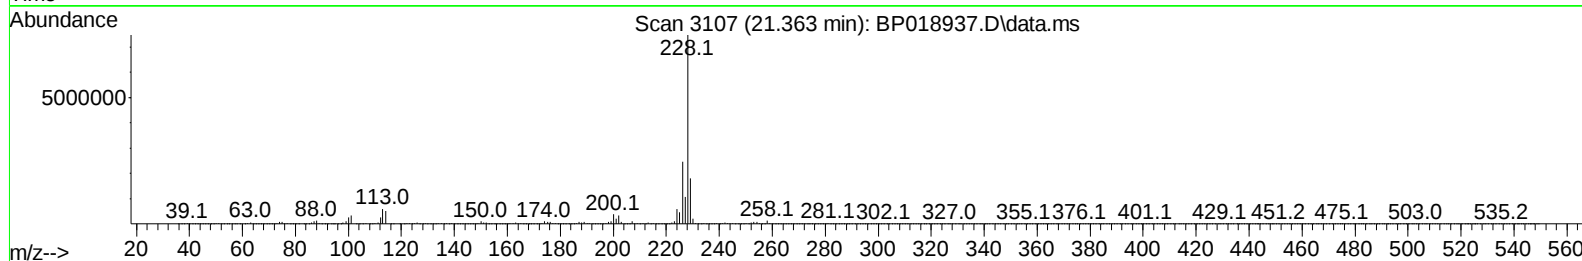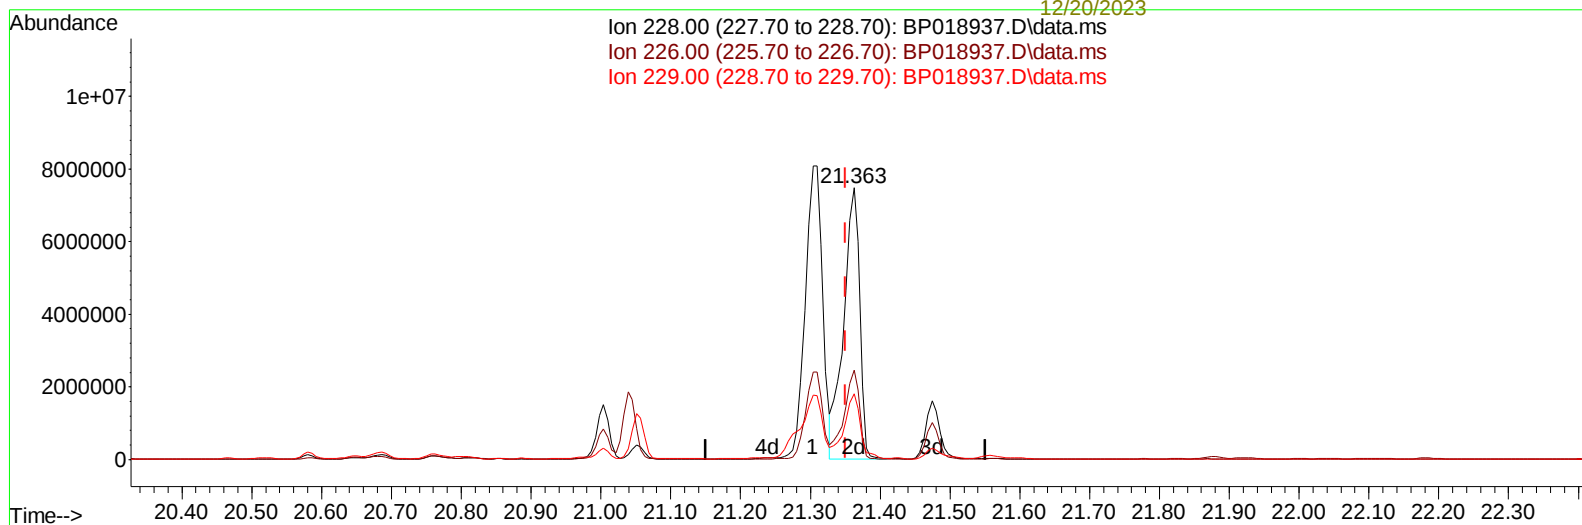

TIC: BP018937.D\data.ms

(87) Chrysene

21.363min (+ 0.012) 170.66 ng/u1 m

response 11983352

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.90	32.85
229.00	19.50	24.11#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1




Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 21:59:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

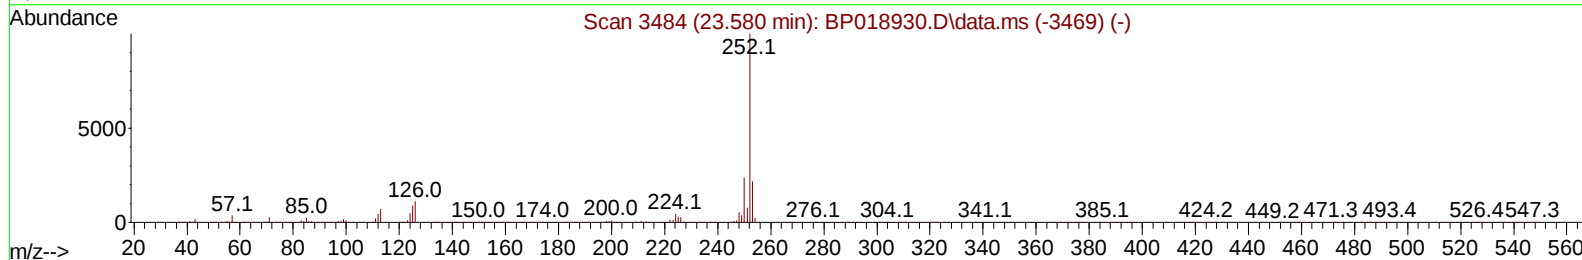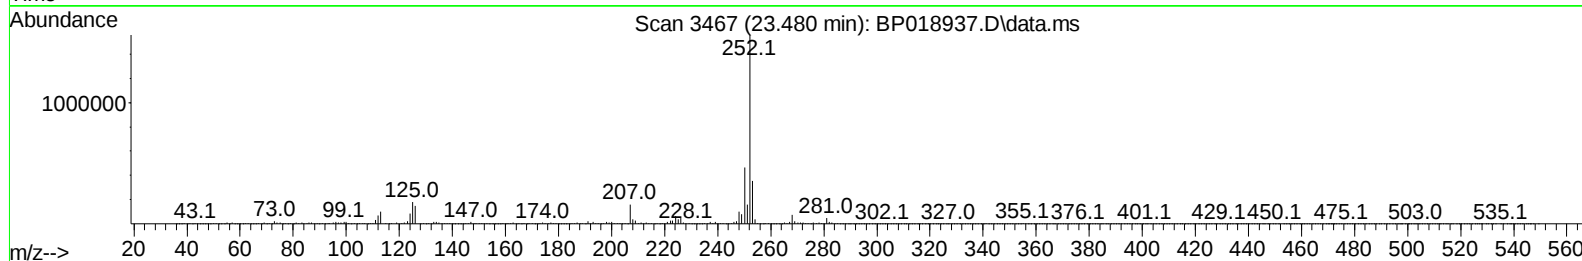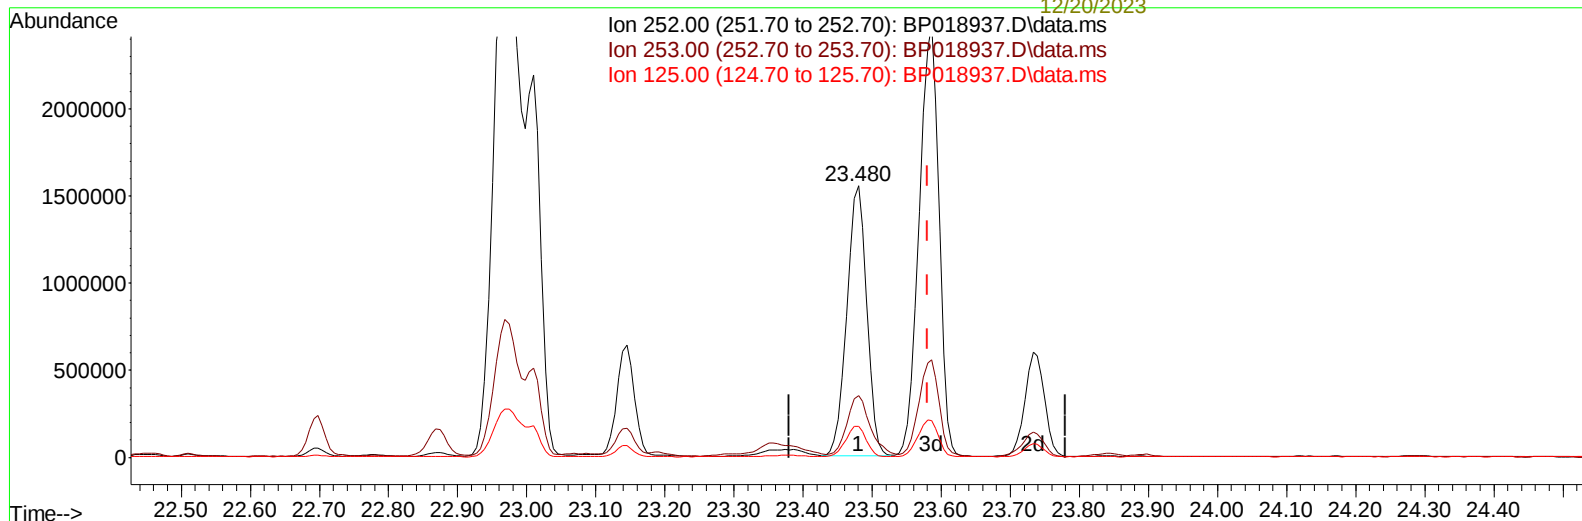

TIC: BP018937.D\data.ms

(93) Benzo(a)pyrene (C)

23.480min (-0.100) 36.95 ng/u1

response 3092152

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.30	22.87
125.00	11.50	11.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL




Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 21:59:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Ion 252.00 (251.70 to 252.70): BP018937.D\data.ms
 Ion 253.00 (252.70 to 253.70): BP018937.D\data.ms
 Ion 125.00 (124.70 to 125.70): BP018937.D\data.ms

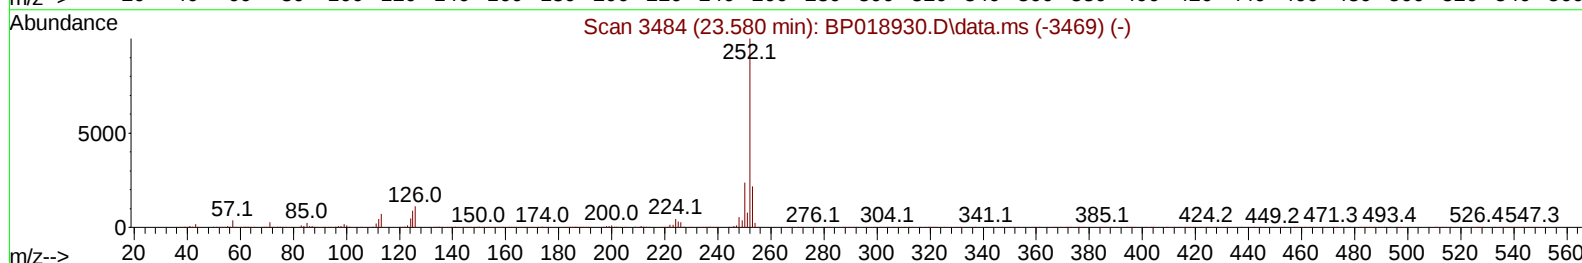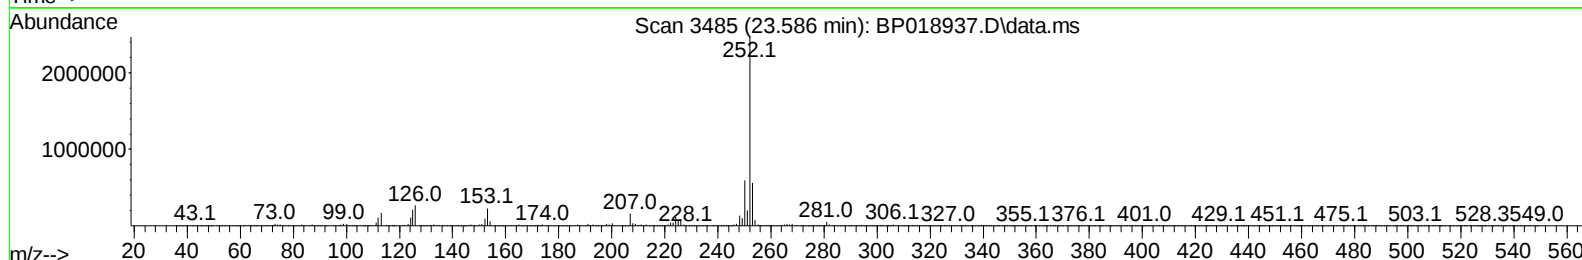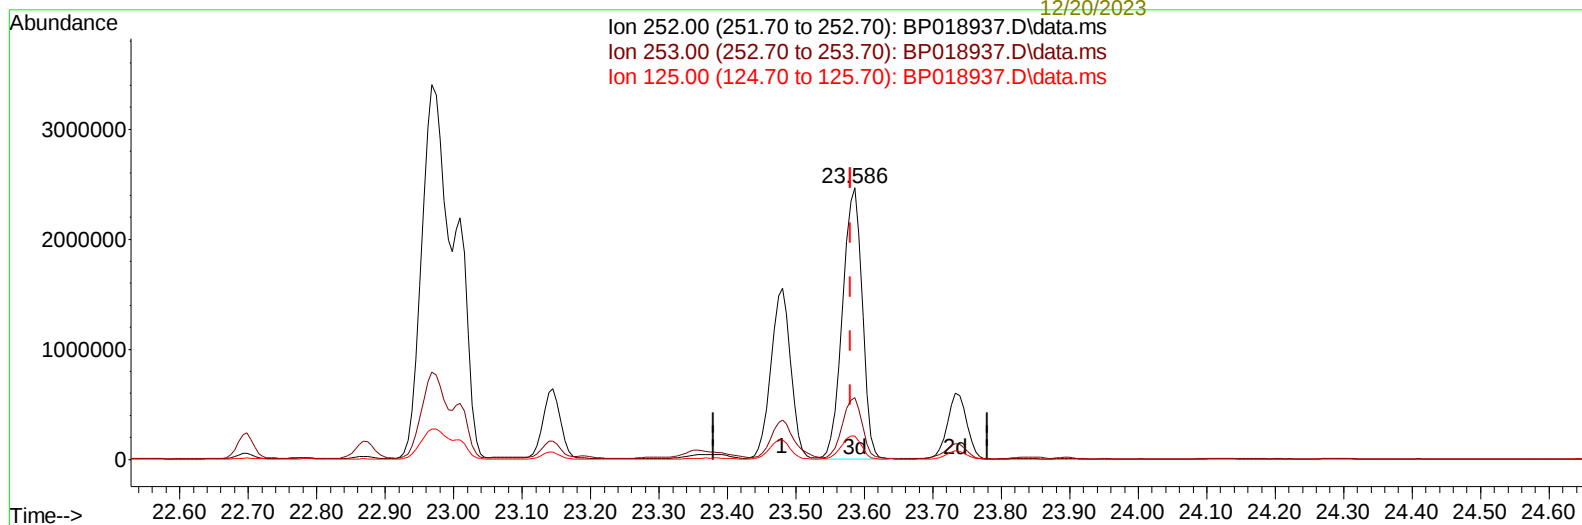

TIC: BP018937.D\data.ms

(93) Benzo(a)pyrene (C)

23.586min (+ 0.006) 59.04 ng/ul m

response 4940191

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.30	22.75
125.00	11.50	8.61#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018937.D
 Acq On : 19 Dec 2023 08:53
 Operator : MA/JU
 Sample : 05626-10DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
 Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
 ahmed
 12/20/2023

Quant Time: Dec 19 22:00:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 19 05:28:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	208500	20.000	ng/ul	0.00
20) Naphthalene-d8	10.634	136	738482	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.469	164	506152	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	888742	20.000	ng/ul	0.02
79) Chrysene-d12	21.321	240	939396	20.000	ng/ul	# 0.00
88) Perylene-d12	23.686	264	1242109	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	2348	0.384	ng/uL	0.00
4) Pyridine-d5	3.687	84	21265	1.298	ng/ul	0.00
7) Phenol-d5	7.010	99	48036	2.296	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	28032	2.260	ng/ul	0.00
11) 2-Chlorophenol-d4	7.363	132	39015	2.390	ng/ul	0.00
15) 4-Methylphenol-d8	8.552	113	36490	2.155	ng/ul	0.00
21) Nitrobenzene-d5	8.993	128	20085	3.056	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	17177	2.521	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.257	165	36194	2.598	ng/ul	0.00
31) 4-Chloroaniline-d4	10.781	131	44384	2.437	ng/ul	0.00
46) Dimethylphthalate-d6	13.892	166	127138	2.814	ng/ul	0.01
49) Acenaphthylene-d8	14.157	160	120505	2.423	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.463	176	100426	2.648	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.357	188	137581m	2.945	ng/ul	0.04
81) Pyrene-d10	19.569	212	173807	2.377	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.527	264	202385	2.794	ng/ul	0.00
Target Compounds						
						Qvalue
30) Naphthalene	10.693	128	27316913m	609.765	ng/ul	
36) 2-Methylnaphthalene	12.316	142	16148278	508.807	ng/ul	100
37) 1-Methylnaphthalene	12.522	142	9268882	289.190	ng/ul	99
50) Acenaphthylene	14.192	152	999773	17.876	ng/ul#	88
52) Acenaphthene	14.569	153	22831552	617.430	ng/ul	98
61) Fluorene	15.551	166	23872879	587.033	ng/ul	99
72) Phenanthrene	17.275	178	47106724m	877.613	ng/ul	
74) Anthracene	17.386	178	14582076	271.026	ng/ul#	93
80) Fluoranthene	19.239	202	33192875m	384.015	ng/ul	
82) Pyrene	19.598	202	27437906m	314.661	ng/ul	
85) Benzo(a)anthracene	21.304	228	13805882	181.062	ng/ul	95
87) Chrysene	21.363	228	11983352m	170.661	ng/ul	
90) Benzo(b)fluoranthene	22.968	252	8588173	93.776	ng/ul	96
91) Benzo(k)fluoranthene	23.010	252	2792617	31.515	ng/ul	97
93) Benzo(a)pyrene	23.586	252	4940191m	59.036	ng/ul	
94) Indeno(1,2,3-cd)pyrene	26.145	276	1646639	16.469	ng/ul#	93
95) Dibenzo(a,h)anthracene	26.145	278	452623	5.442	ng/ul#	78
96) Benzo(g,h,i)perylene	26.903	276	692699	8.609	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018937.D
Acq On : 19 Dec 2023 08:53
Operator : MA/JU
Sample : 05626-10DL 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLF6DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/20/2023
Supervised By :mohammad ahmed 12/20/2023

Supervised By :mohammad
ahmed
12/20/2023

Quant Time: Dec 19 22:00:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 19 05:28:03 2023
Response via : Initial Calibration

