

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018899.D
 Acq On : 18 Dec 2023 10:40
 Operator : MA/JU
 Sample : PB157755BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK755

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	37	rVB	117050	149296	1.44%	0.176%
2	3.675	95	100	115	rBV	1314558	2005420	19.38%	2.367%
3	4.005	152	156	161	rVB2	22823	34743	0.34%	0.041%
4	4.334	209	212	219	rVB2	25520	40131	0.39%	0.047%
5	6.999	658	665	676	rVB	1515685	2327168	22.49%	2.747%
6	7.163	686	693	704	rVB	1257352	1959667	18.94%	2.313%
7	7.358	719	726	736	rBV	1551117	2390896	23.10%	2.823%
8	7.828	799	806	815	rBV	1179357	1840667	17.79%	2.173%
9	8.540	919	927	942	rBV	1843747	2903297	28.06%	3.427%
10	8.987	995	1003	1015	rBV	1333055	2164023	20.91%	2.555%
11	9.710	1117	1126	1136	rBV	1000683	1632726	15.78%	1.927%
12	10.246	1209	1217	1231	rBV	1678421	2882706	27.86%	3.403%
13	10.622	1272	1281	1288	rBV	1435526	2345709	22.67%	2.769%
14	10.763	1297	1305	1323	rBV	1730502	2987858	28.87%	3.527%
15	10.951	1334	1337	1344	rVB9	5671	10794	0.10%	0.013%
16	12.210	1545	1551	1558	rVB2	28644	52612	0.51%	0.062%
17	12.281	1558	1563	1569	rBV8	6613	12497	0.12%	0.015%
18	12.504	1592	1601	1606	rBV9	6765	11693	0.11%	0.014%
19	13.257	1721	1729	1732	rBV9	8847	17192	0.17%	0.020%
20	13.298	1732	1736	1739	rVV2	7492	12478	0.12%	0.015%
21	13.363	1739	1747	1752	rVB4	23255	50599	0.49%	0.060%
22	13.875	1825	1834	1841	rBV	2968802	4068236	39.31%	4.803%
23	14.151	1873	1881	1897	rBV	3362460	4874012	47.10%	5.754%
24	14.457	1926	1933	1941	rBV	1920707	2801400	27.07%	3.307%
25	14.663	1962	1968	1984	rBV	1066595	1753200	16.94%	2.070%
26	14.863	1998	2002	2008	rVB3	9449	17306	0.17%	0.020%
27	15.451	2095	2102	2109	rBV	4476709	6133984	59.27%	7.241%
28	15.504	2109	2111	2116	rVV5	21512	29646	0.29%	0.035%
29	15.575	2116	2123	2134	rVV	1025274	1425830	13.78%	1.683%
30	15.692	2139	2143	2146	rBV2	19038	22943	0.22%	0.027%
31	16.239	2230	2236	2240	rVB9	5977	11095	0.11%	0.013%
32	16.404	2261	2264	2272	rVB9	6627	12955	0.13%	0.015%
33	16.510	2277	2282	2285	rBV6	8081	10955	0.11%	0.013%
34	16.686	2306	2312	2318	rBV6	7512	14425	0.14%	0.017%
35	17.210	2394	2401	2411	rBV	2265249	3193579	30.86%	3.770%
36	17.310	2411	2418	2435	rVV	4766012	6735171	65.08%	7.951%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018899.D
Acq On : 18 Dec 2023 10:40
Operator : MA/JU
Sample : PB157755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK755

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.104	2549	2553	2556	rBV6	13891	19340	0.19%	0.023%
38	18.428	2603	2608	2614	rBV7	13301	22452	0.22%	0.027%
39	19.122	2722	2726	2731	rBV2	62415	83768	0.81%	0.099%
40	19.192	2734	2738	2742	rBV	60432	86915	0.84%	0.103%
41	19.551	2792	2799	2811	rBV	6539934	8778702	84.83%	10.363%
42	21.304	3092	3097	3106	rBV	3209089	4029070	38.93%	4.756%
43	23.516	3466	3473	3488	rVB2	5273303	10348418	100.00%	12.217%
44	23.668	3492	3499	3511	rVB	2250969	4402597	42.54%	5.197%




Sum of corrected areas: 84708171

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018899.D
Acq On : 18 Dec 2023 10:40
Operator : MA/JU
Sample : PB157755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK755

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

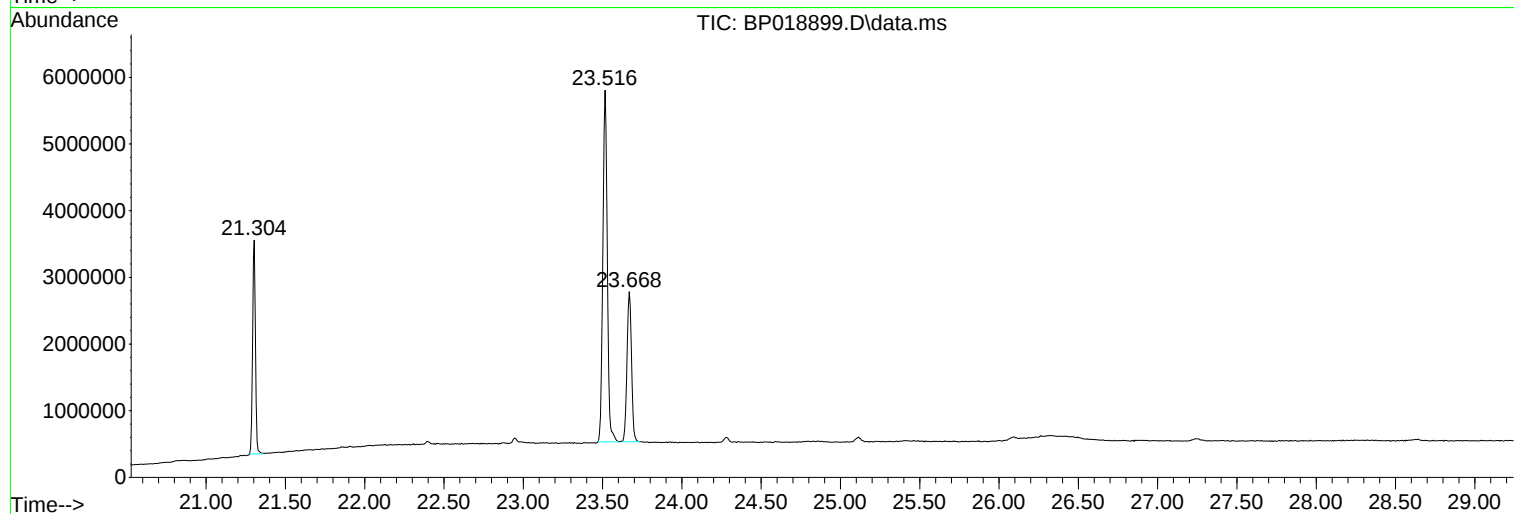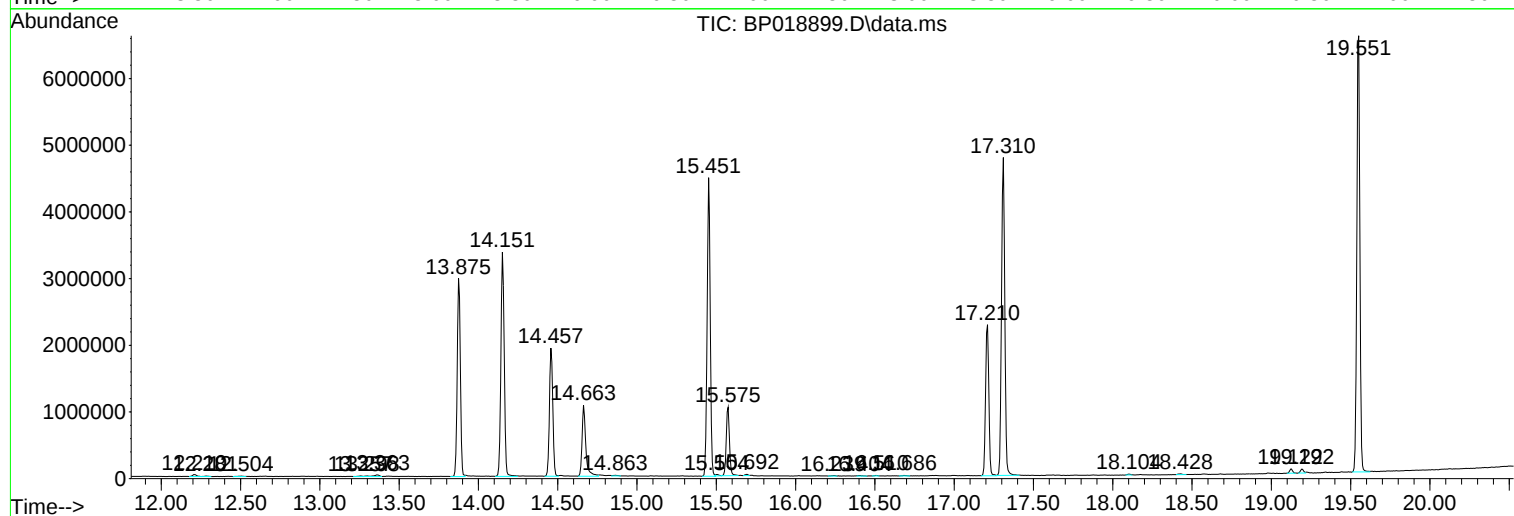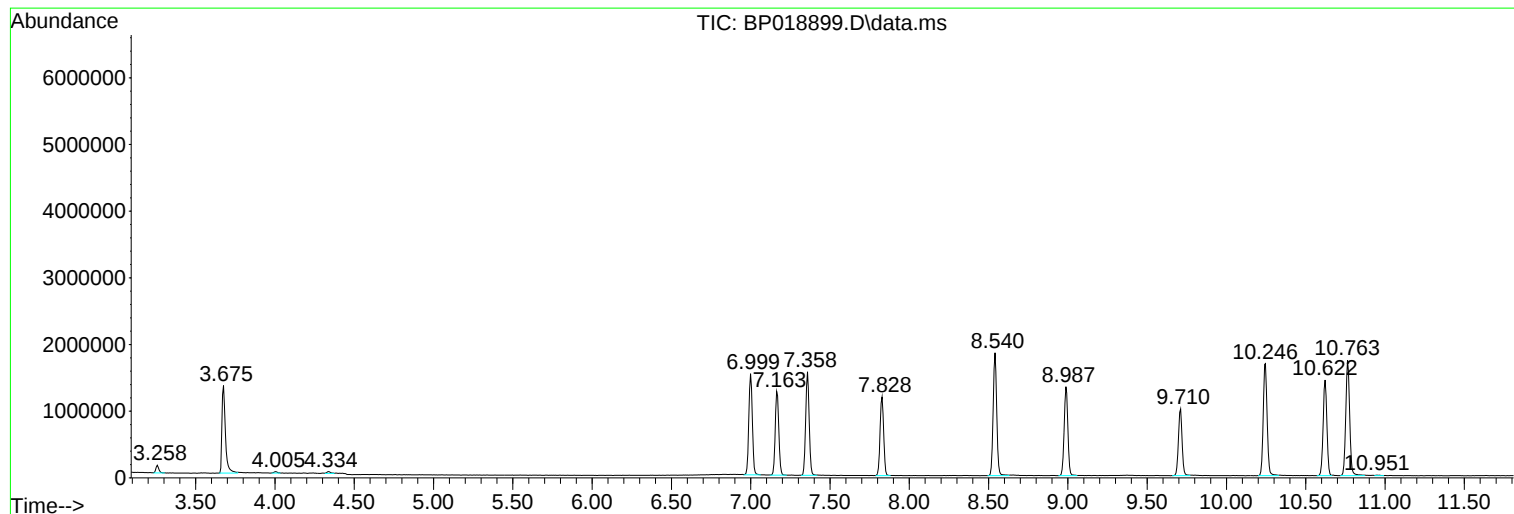

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018899.D
Acq On : 18 Dec 2023 10:40
Operator : MA/JU
Sample : PB157755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK755

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018899.D
Acq On : 18 Dec 2023 10:40
Operator : MA/JU
Sample : PB157755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK755

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc