

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018909.D
 Acq On : 18 Dec 2023 16:26
 Operator : MA/JU
 Sample : 05794-22 20X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGRG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.775	115	117	122	rBV6	3398	5964	0.15%	0.026%
2	4.005	152	156	160	rVB	18196	22736	0.58%	0.099%
3	5.834	460	467	471	rBV10	4650	11265	0.29%	0.049%
4	6.369	555	558	563	rBV7	2442	4500	0.12%	0.020%
5	6.493	574	579	581	rBV6	4890	6640	0.17%	0.029%
6	6.563	588	591	596	rBV7	3405	5854	0.15%	0.026%
7	6.746	620	622	627	rBV6	2750	4602	0.12%	0.020%
8	6.916	647	651	655	rBV7	2721	4241	0.11%	0.018%
9	6.957	655	658	659	rVV3	5449	5089	0.13%	0.022%
10	7.005	662	666	671	rVB2	20021	29344	0.75%	0.128%
11	7.169	689	694	699	rBV	22925	35619	0.91%	0.155%
12	7.363	719	727	733	rVB	24205	41990	1.08%	0.183%
13	7.828	799	806	813	rBV	1006172	1552475	39.75%	6.766%
14	8.010	834	837	842	rVB7	2992	3969	0.10%	0.017%
15	8.181	862	866	869	rBV6	3405	6223	0.16%	0.027%
16	8.269	877	881	883	rBV5	3068	3990	0.10%	0.017%
17	8.375	892	899	903	rVB10	5916	12113	0.31%	0.053%
18	8.546	923	928	934	rBV2	27710	50206	1.29%	0.219%
19	8.657	942	947	953	rBV	24338	42460	1.09%	0.185%
20	8.910	984	990	991	rBV6	4496	6552	0.17%	0.029%
21	8.922	991	992	998	rVB6	4376	5793	0.15%	0.025%
22	8.993	998	1004	1011	rBV	21535	38101	0.98%	0.166%
23	9.399	1070	1073	1077	rVB6	4090	6249	0.16%	0.027%
24	9.540	1096	1097	1102	rVB5	4772	3927	0.10%	0.017%
25	9.710	1119	1126	1130	rBV5	14860	26579	0.68%	0.116%
26	9.799	1137	1141	1146	rVB8	5642	9649	0.25%	0.042%
27	10.251	1210	1218	1226	rBV3	22628	48331	1.24%	0.211%
28	10.622	1272	1281	1288	rBV	1211629	2031370	52.01%	8.854%
29	10.669	1288	1289	1298	rVB	20634	26473	0.68%	0.115%
30	10.775	1303	1307	1308	rBV4	5368	5766	0.15%	0.025%
31	11.110	1359	1364	1369	rVV8	4258	8048	0.21%	0.035%
32	11.175	1372	1375	1381	rVB8	5174	7330	0.19%	0.032%
33	11.422	1414	1417	1421	rBV6	3055	4983	0.13%	0.022%
34	11.651	1453	1456	1457	rBV3	4537	4947	0.13%	0.022%
35	11.816	1477	1484	1486	rBV7	4420	8147	0.21%	0.036%
36	11.904	1492	1499	1502	rBV9	5380	8754	0.22%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018909.D
 Acq On : 18 Dec 2023 16:26
 Operator : MA/JU
 Sample : 05794-22 20X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGRG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	12.134	1533	1538	1540	rBV6	3211	4345	0.11%	0.019%
38	12.287	1556	1564	1569	rVB3	15063	29384	0.75%	0.128%
39	12.504	1596	1601	1609	rBV2	13082	23272	0.60%	0.101%
40	12.669	1624	1629	1633	rVV8	5099	10134	0.26%	0.044%
41	12.951	1675	1677	1681	rBV5	3379	4094	0.10%	0.018%
42	13.004	1682	1686	1689	rVB6	5461	7386	0.19%	0.032%
43	13.263	1726	1730	1731	rBV4	4704	5362	0.14%	0.023%
44	13.298	1733	1736	1741	rVB6	6994	11668	0.30%	0.051%
45	13.363	1745	1747	1753	rVB7	6145	11146	0.29%	0.049%
46	13.522	1771	1774	1778	rVB6	4700	6264	0.16%	0.027%
47	13.622	1786	1791	1792	rBV4	7776	9354	0.24%	0.041%
48	13.639	1792	1794	1799	rVB6	8166	11048	0.28%	0.048%
49	13.781	1812	1818	1824	rBV2	16415	31238	0.80%	0.136%
50	13.839	1824	1828	1830	rVV3	8314	12488	0.32%	0.054%
51	13.875	1830	1834	1840	rVB	50684	71359	1.83%	0.311%
52	14.151	1877	1881	1884	rBV	59800	86413	2.21%	0.377%
53	14.181	1884	1886	1892	rVB	30973	42494	1.09%	0.185%
54	14.287	1901	1904	1909	rBV7	7062	10509	0.27%	0.046%
55	14.357	1912	1916	1923	rBV9	5367	10953	0.28%	0.048%
56	14.463	1923	1934	1940	rBV	1657506	2486220	63.65%	10.836%
57	14.522	1940	1944	1953	rVB	38505	71583	1.83%	0.312%
58	14.669	1965	1969	1971	rBV5	6796	11007	0.28%	0.048%
59	14.863	1997	2002	2009	rVV	30814	49143	1.26%	0.214%
60	14.934	2012	2014	2019	rVB4	11560	13123	0.34%	0.057%
61	14.986	2021	2023	2027	rBV5	5597	6407	0.16%	0.028%
62	15.086	2036	2040	2042	rVB5	8798	11049	0.28%	0.048%
63	15.128	2046	2047	2052	rVB5	6374	6361	0.16%	0.028%
64	15.245	2061	2067	2071	rBV8	11981	28536	0.73%	0.124%
65	15.281	2071	2073	2076	rVV4	5285	5185	0.13%	0.023%
66	15.451	2098	2102	2107	rBV	73616	102029	2.61%	0.445%
67	15.510	2107	2112	2123	rVB	55350	103480	2.65%	0.451%
68	15.669	2137	2139	2144	rBV5	6436	7707	0.20%	0.034%
69	15.728	2145	2149	2153	rVV6	10042	12670	0.32%	0.055%
70	15.804	2159	2162	2169	rVB	14815	20466	0.52%	0.089%
71	15.957	2184	2188	2195	rVB4	12303	24648	0.63%	0.107%
72	16.192	2223	2228	2232	rVB8	15340	30712	0.79%	0.134%
73	16.516	2277	2283	2287	rVV5	23973	41602	1.07%	0.181%
74	16.563	2288	2291	2297	rVB5	16980	23795	0.61%	0.104%
75	16.663	2306	2308	2313	rVB5	12727	16949	0.43%	0.074%
76	16.863	2340	2342	2346	rVB3	14520	19331	0.49%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018909.D
 Acq On : 18 Dec 2023 16:26
 Operator : MA/JU
 Sample : 05794-22 20X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGRG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	17.028	2367	2370	2378	rVB	35228	54277	1.39%	0.237%
78	17.210	2395	2401	2405	rBV	1917595	2723900	69.74%	11.872%
79	17.251	2405	2408	2414	rVV	516133	774850	19.84%	3.377%
80	17.310	2414	2418	2421	rVV	95198	157693	4.04%	0.687%
81	17.345	2421	2424	2430	rVB	125651	180456	4.62%	0.787%
82	17.622	2467	2471	2480	rVB	56200	91745	2.35%	0.400%
83	18.080	2545	2549	2554	rBV	75050	139457	3.57%	0.608%
84	18.127	2554	2557	2562	rVB	105241	140017	3.58%	0.610%
85	18.204	2568	2570	2576	rVB	30579	33209	0.85%	0.145%
86	18.269	2576	2581	2585	rVV2	123173	230902	5.91%	1.006%
87	18.304	2585	2587	2593	rVB	71128	79569	2.04%	0.347%
88	18.569	2628	2632	2635	rBV	56093	76429	1.96%	0.333%
89	18.969	2697	2700	2705	rBV	67435	100504	2.57%	0.438%
90	19.227	2739	2744	2751	rBV	881156	1280374	32.78%	5.580%
91	19.486	2785	2788	2793	rVB	118439	136790	3.50%	0.596%
92	19.551	2795	2799	2800	rVV2	221708	282483	7.23%	1.231%
93	19.580	2800	2804	2812	rVB	754523	1114031	28.52%	4.855%
94	19.686	2819	2822	2827	rVB	116286	140820	3.61%	0.614%
95	21.304	3091	3097	3101	rBV2	2649432	3906001	100.00%	17.024%
96	21.339	3101	3103	3110	rVB	397338	480826	12.31%	2.096%
97	23.674	3494	3500	3508	rBV	1711181	3228279	82.65%	14.070%




Sum of corrected areas: 22943805

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018909.D
Acq On : 18 Dec 2023 16:26
Operator : MA/JU
Sample : 05794-22 20X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGRG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

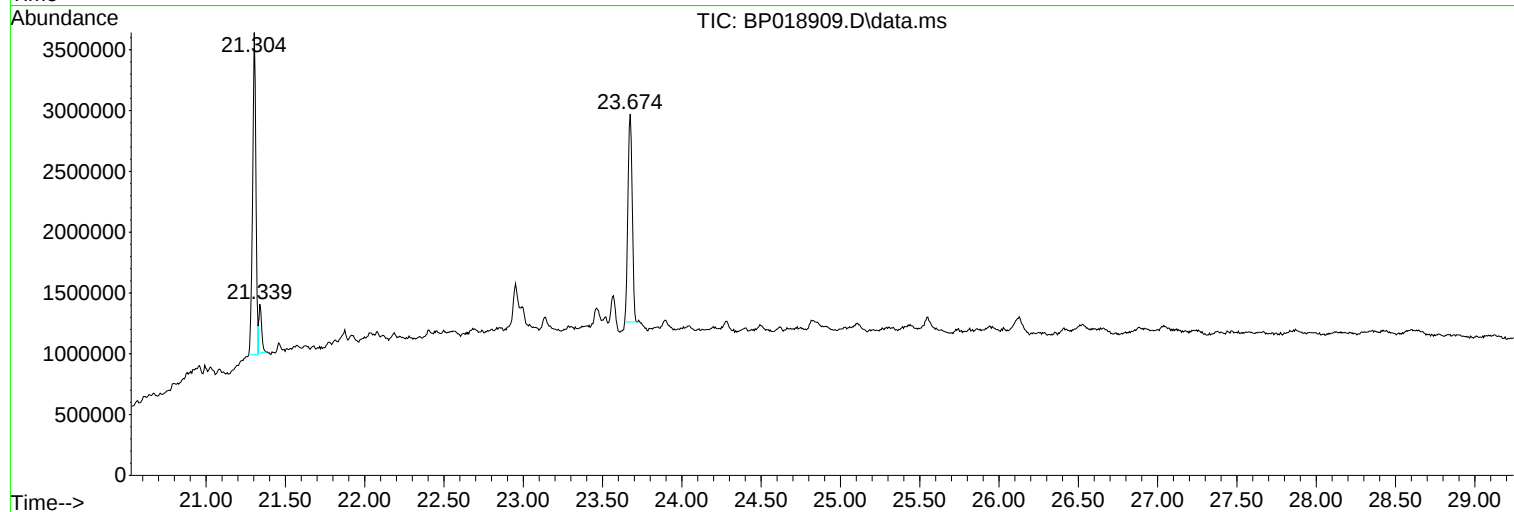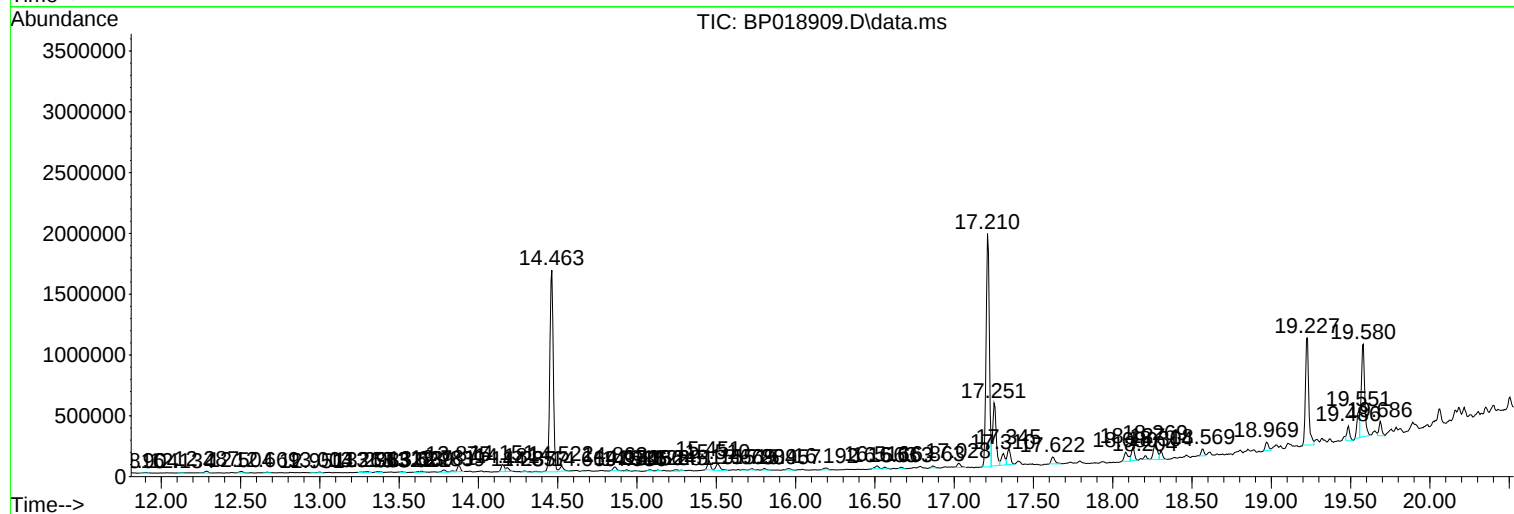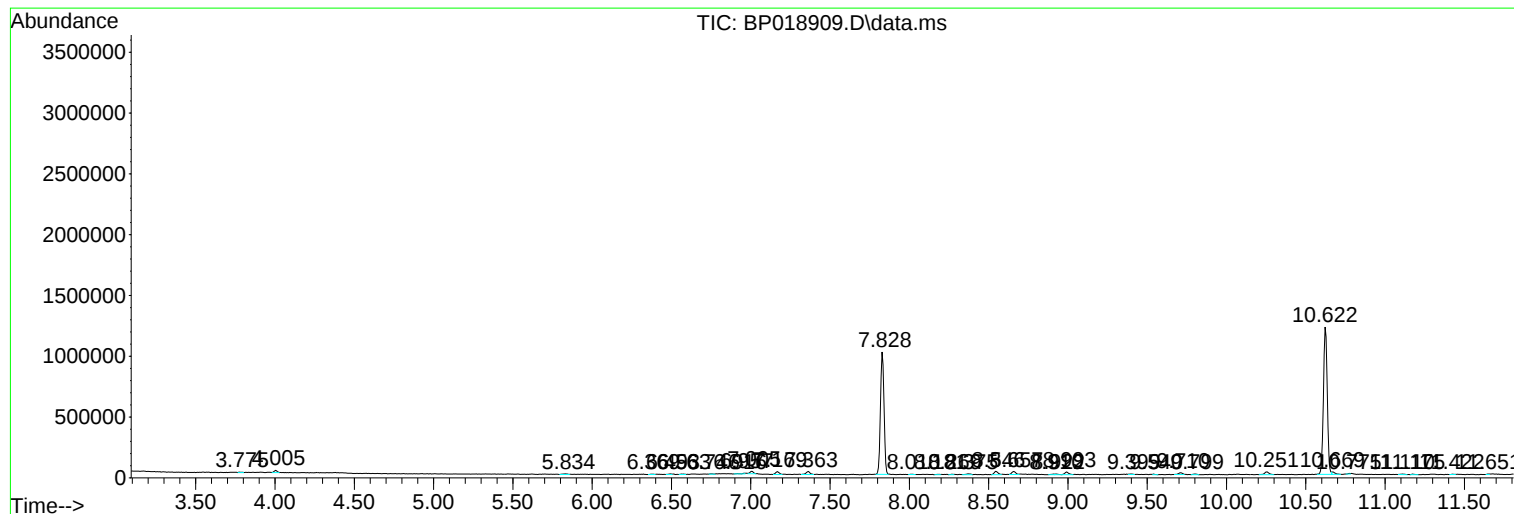

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018909.D
Acq On : 18 Dec 2023 16:26
Operator : MA/JU
Sample : 05794-22 20X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGRG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018909.D
Acq On : 18 Dec 2023 16:26
Operator : MA/JU
Sample : 05794-22 20X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGRG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------