

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018911.D
 Acq On : 18 Dec 2023 17:35
 Operator : MA/JU
 Sample : PB157838BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK838

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rVB	72922	97726	1.72%	0.174%
2	3.675	96	100	117	rBV	782148	1258860	22.13%	2.243%
3	4.005	151	156	162	rVB	56553	84389	1.48%	0.150%
4	7.005	657	666	676	rBV	928638	1469313	25.82%	2.618%
5	7.169	687	694	704	rVB	787763	1234752	21.70%	2.200%
6	7.357	719	726	735	rBV	956431	1544974	27.15%	2.753%
7	7.828	799	806	814	rVB	1015008	1551273	27.26%	2.765%
8	8.546	920	928	937	rBV	1080287	1778640	31.26%	3.170%
9	8.987	995	1003	1013	rBV	831515	1370466	24.09%	2.442%
10	9.710	1118	1126	1133	rBV	675302	1103943	19.40%	1.967%
11	10.246	1210	1217	1231	rBV	1089758	1816344	31.92%	3.237%
12	10.622	1273	1281	1291	rVB	1204450	1968396	34.60%	3.508%
13	10.763	1297	1305	1322	rBV	984443	1757962	30.90%	3.133%
14	10.869	1322	1323	1330	rVB7	3990	6235	0.11%	0.011%
15	11.598	1440	1447	1449	rBV8	3254	6065	0.11%	0.011%
16	12.210	1545	1551	1559	rBV	19417	35727	0.63%	0.064%
17	13.357	1741	1746	1752	rVB4	10324	16949	0.30%	0.030%
18	13.875	1828	1834	1845	rBV	1752158	2360379	41.49%	4.206%
19	14.151	1872	1881	1895	rBV	2053255	3048981	53.59%	5.434%
20	14.463	1926	1934	1941	rBV	1622430	2442321	42.93%	4.352%
21	14.522	1941	1944	1953	rVB6	9928	21978	0.39%	0.039%
22	14.669	1963	1969	1987	rBV	557857	1047871	18.42%	1.867%
23	14.863	1998	2002	2010	rVB2	10832	23460	0.41%	0.042%
24	15.451	2095	2102	2109	rBV	2522989	3665714	64.43%	6.533%
25	15.510	2109	2112	2117	rVV2	19972	33684	0.59%	0.060%
26	15.575	2118	2123	2132	rVV	409053	569480	10.01%	1.015%
27	15.692	2139	2143	2148	rVB4	10467	16753	0.29%	0.030%
28	16.233	2232	2235	2243	rVB7	9182	16116	0.28%	0.029%
29	16.869	2338	2343	2344	rBV5	8997	10539	0.19%	0.019%
30	16.992	2362	2364	2367	rBV3	5781	7043	0.12%	0.013%
31	17.210	2394	2401	2406	rBV	2046030	2900275	50.97%	5.169%
32	17.257	2406	2409	2412	rVV	127938	183945	3.23%	0.328%
33	17.310	2412	2418	2430	rVB	2840290	4087026	71.83%	7.284%
34	17.475	2442	2446	2455	rBV8	12354	28075	0.49%	0.050%
35	17.622	2467	2471	2477	rVB	19451	30149	0.53%	0.054%
36	18.275	2578	2582	2585	rBV7	10872	17946	0.32%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018911.D
Acq On : 18 Dec 2023 17:35
Operator : MA/JU
Sample : PB157838BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK838

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.122	2724	2726	2731	rVB2	39713	45534	0.80%	0.081%
38	19.192	2736	2738	2740	rVV	36774	44669	0.79%	0.080%
39	19.227	2740	2744	2752	rVB	210045	319450	5.61%	0.569%
40	19.551	2793	2799	2810	rBV	3889203	5294792	93.06%	9.436%
41	21.304	3092	3097	3102	rBV	2828795	3490040	61.34%	6.220%
42	23.515	3466	3473	3488	rVB2	2856217	5689621	100.00%	10.139%
43	23.668	3493	3499	3508	rVB	1889209	3615574	63.55%	6.443%




Sum of corrected areas: 56113429

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018911.D
Acq On : 18 Dec 2023 17:35
Operator : MA/JU
Sample : PB157838BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

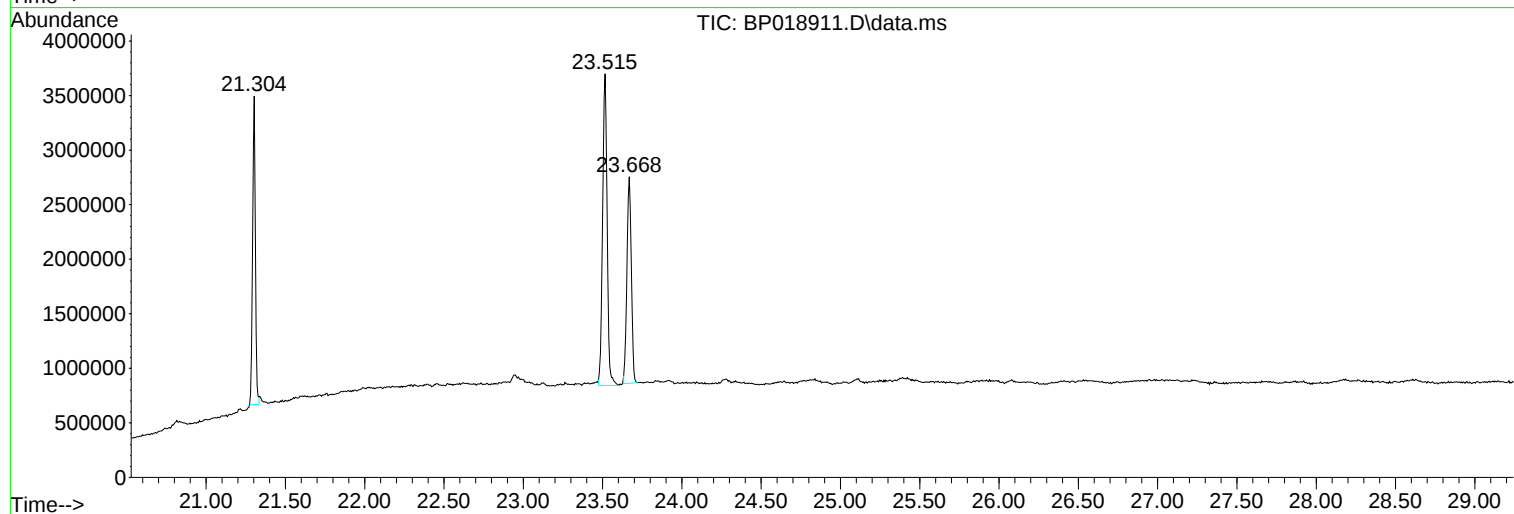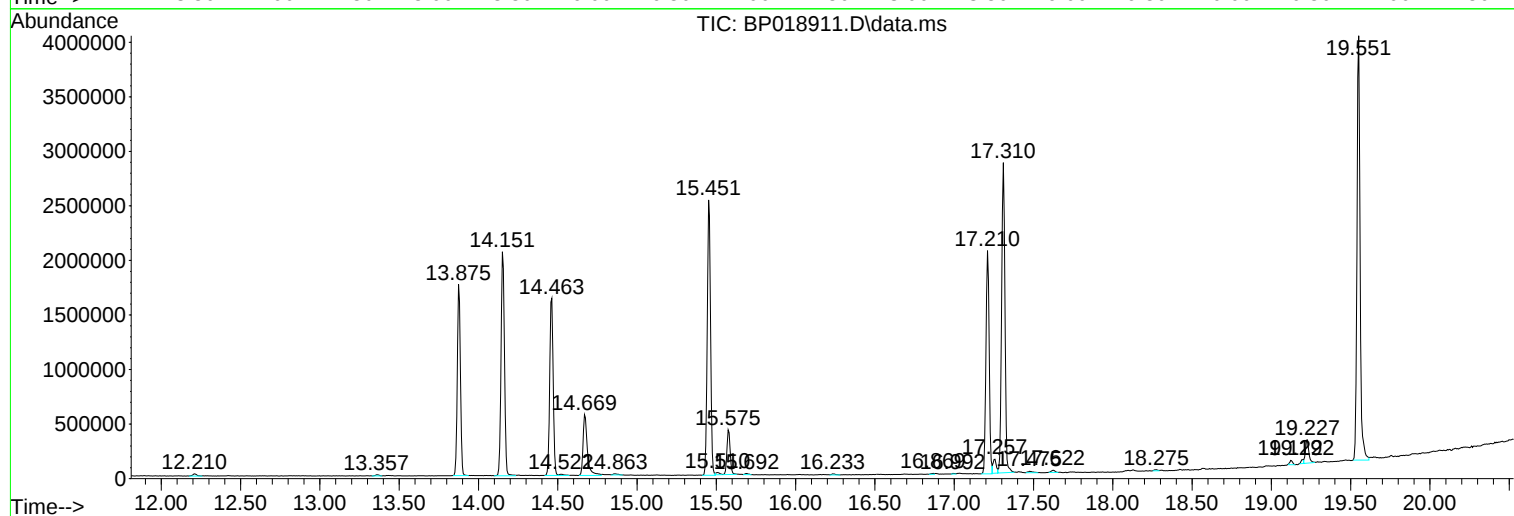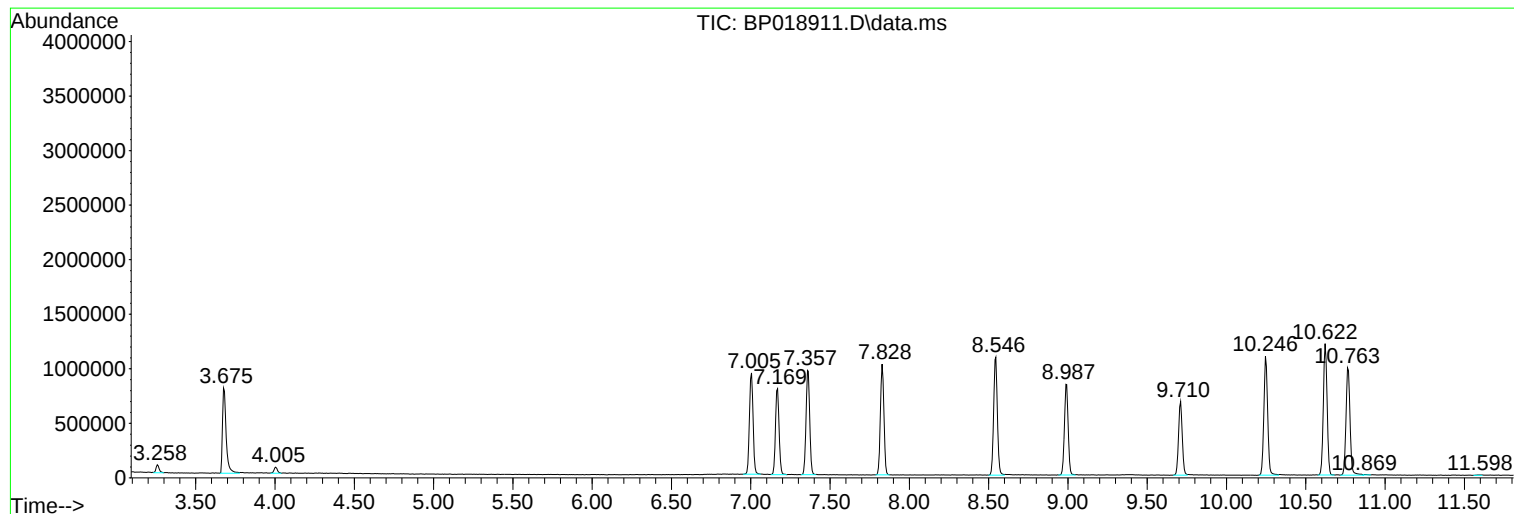

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018911.D
Acq On : 18 Dec 2023 17:35
Operator : MA/JU
Sample : PB157838BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018911.D
Acq On : 18 Dec 2023 17:35
Operator : MA/JU
Sample : PB157838BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK838

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------