

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018912.D
 Acq On : 18 Dec 2023 18:09
 Operator : MA/JU
 Sample : PB157781BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK781

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	38	rVB	79146	105373	1.83%	0.195%
2	3.675	96	100	119	rBV	810291	1269132	22.09%	2.354%
3	4.005	151	156	166	rVB	50419	76289	1.33%	0.142%
4	7.005	658	666	677	rVB	939364	1481967	25.80%	2.749%
5	7.163	687	693	701	rVB	788790	1220975	21.25%	2.265%
6	7.358	719	726	738	rBV	988563	1554286	27.06%	2.883%
7	7.828	797	806	816	rBV	866981	1359045	23.66%	2.521%
8	8.540	920	927	941	rBV	1093794	1773503	30.87%	3.290%
9	8.987	996	1003	1015	rBV	835155	1364670	23.75%	2.532%
10	9.710	1117	1126	1135	rBV	662593	1098002	19.11%	2.037%
11	10.246	1209	1217	1230	rBV	1087088	1811810	31.54%	3.361%
12	10.622	1272	1281	1289	rBV	1036282	1724762	30.02%	3.200%
13	10.763	1297	1305	1321	rBV	999641	1741069	30.31%	3.230%
14	11.004	1342	1346	1352	rVB8	3352	6307	0.11%	0.012%
15	12.210	1546	1551	1559	rVB	20672	34150	0.59%	0.063%
16	13.363	1740	1747	1751	rBV7	8567	14950	0.26%	0.028%
17	13.875	1828	1834	1849	rBV	1708313	2329132	40.54%	4.321%
18	14.151	1875	1881	1893	rBV	1989043	2993386	52.11%	5.553%
19	14.457	1927	1933	1940	rBV	1410563	2090786	36.39%	3.879%
20	14.669	1963	1969	1985	rBV	543505	1010623	17.59%	1.875%
21	14.857	1998	2001	2010	rVB2	11809	24712	0.43%	0.046%
22	15.122	2043	2046	2051	rBV6	3758	6496	0.11%	0.012%
23	15.451	2094	2102	2109	rBV	2542103	3639996	63.36%	6.753%
24	15.510	2109	2112	2118	rVV3	19524	35617	0.62%	0.066%
25	15.575	2118	2123	2133	rVV	421240	574083	9.99%	1.065%
26	15.692	2139	2143	2150	rVB7	12615	23091	0.40%	0.043%
27	16.239	2233	2236	2241	rVB4	10458	14185	0.25%	0.026%
28	17.210	2394	2401	2406	rBV	1716131	2493013	43.40%	4.625%
29	17.251	2406	2408	2412	rVV	113052	154786	2.69%	0.287%
30	17.310	2412	2418	2432	rVB	2842067	4052269	70.54%	7.518%
31	17.475	2444	2446	2454	rVB7	10454	16778	0.29%	0.031%
32	17.622	2468	2471	2478	rVB2	15940	26623	0.46%	0.049%
33	19.122	2723	2726	2732	rVB2	41443	57513	1.00%	0.107%
34	19.192	2735	2738	2740	rBV	40586	52909	0.92%	0.098%
35	19.222	2740	2743	2754	rVB	190445	280323	4.88%	0.520%
36	19.545	2793	2798	2810	rBV	3736183	5283103	91.96%	9.801%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018912.D
Acq On : 18 Dec 2023 18:09
Operator : MA/JU
Sample : PB157781BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK781

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	21.304	3092	3097	3101	rBV	2321395	3070074	53.44%	5.695%
38	23.515	3466	3473	3485	rVB2	2937382	5744772	100.00%	10.657%
39	23.668	3492	3499	3507	rVB	1645504	3293479	57.33%	6.110%




Sum of corrected areas: 53904039

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018912.D
Acq On : 18 Dec 2023 18:09
Operator : MA/JU
Sample : PB157781BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

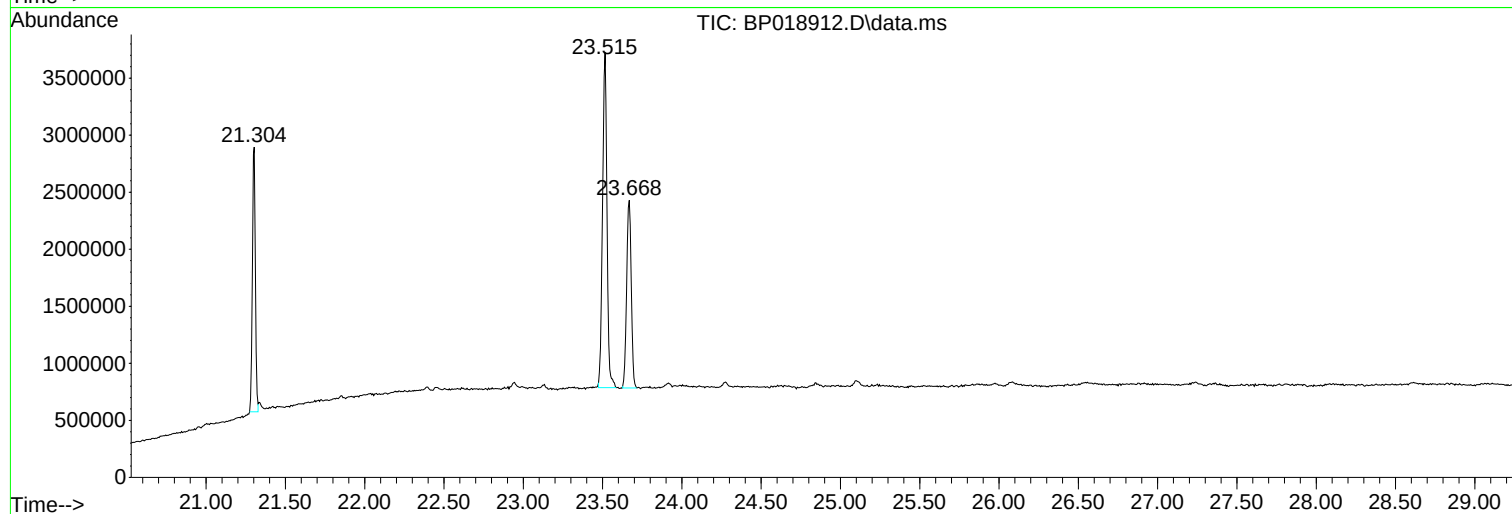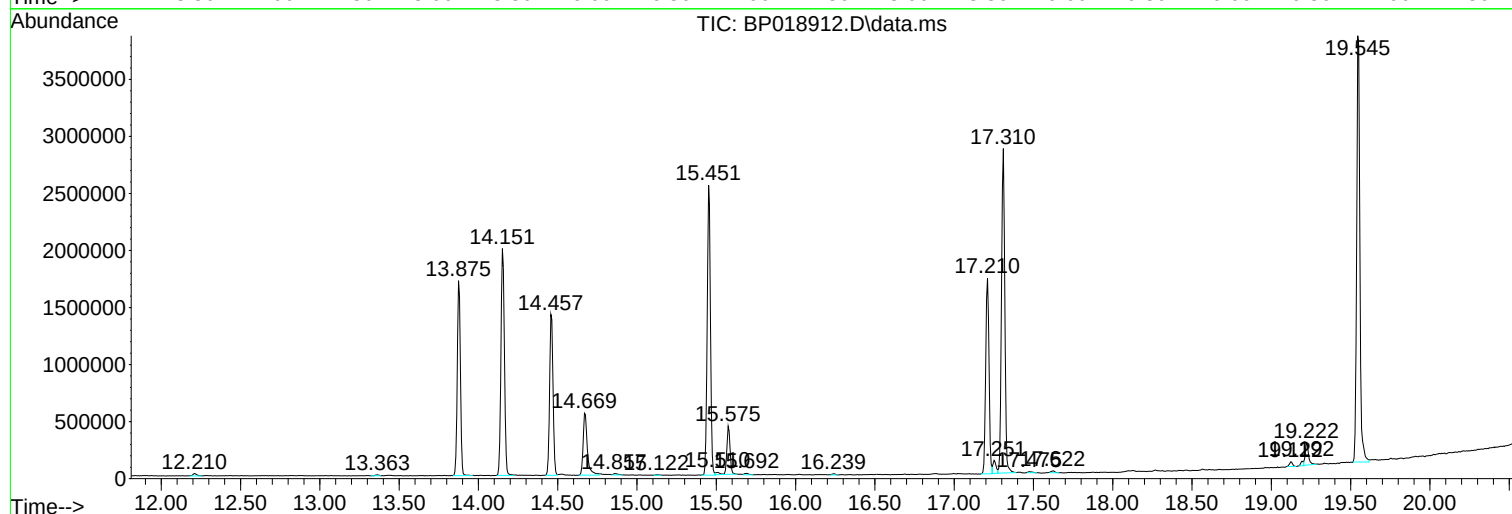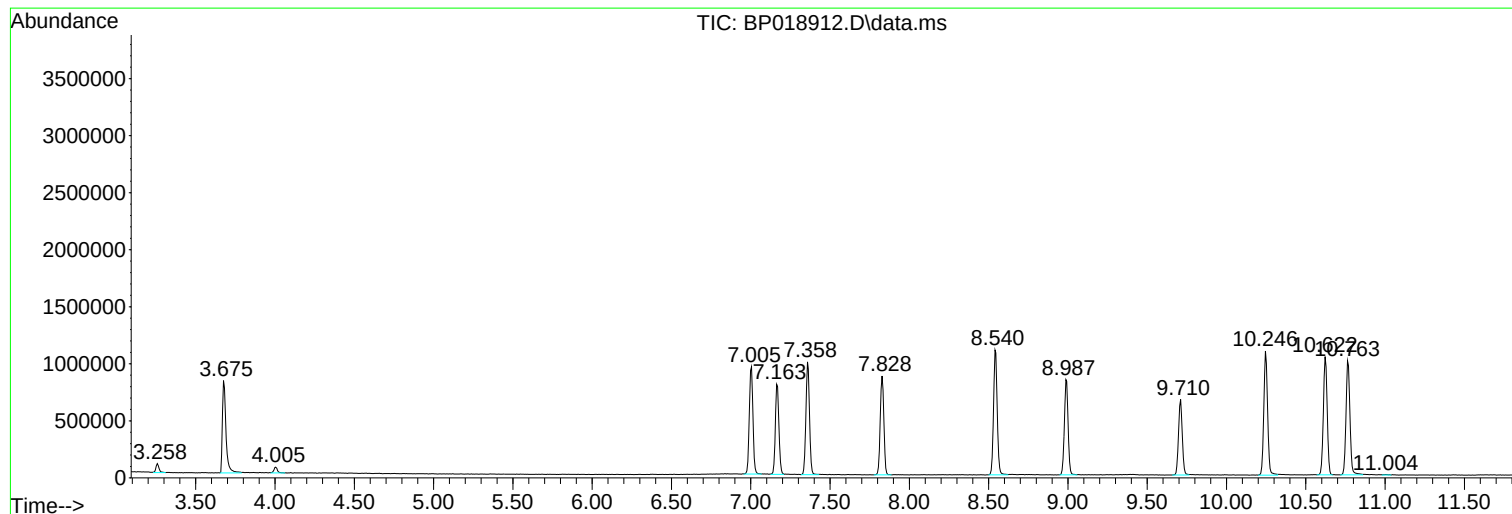

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018912.D
Acq On : 18 Dec 2023 18:09
Operator : MA/JU
Sample : PB157781BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018912.D
Acq On : 18 Dec 2023 18:09
Operator : MA/JU
Sample : PB157781BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc