

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018931.D
 Acq On : 19 Dec 2023 05:29
 Operator : MA/JU
 Sample : PB157879BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK879

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	38	rVB	82793	119008	1.83%	0.203%
2	3.681	97	101	120	rBV	876631	1332391	20.45%	2.276%
3	4.005	153	156	161	rVB	18203	22465	0.34%	0.038%
4	5.105	339	343	346	rBV6	4529	7595	0.12%	0.013%
5	7.010	661	667	679	rVB	991629	1590547	24.41%	2.716%
6	7.169	688	694	703	rVB	831813	1255419	19.27%	2.144%
7	7.363	720	727	738	rBV	1030859	1635560	25.10%	2.793%
8	7.834	800	807	815	rVB	932088	1467000	22.51%	2.505%
9	8.551	922	929	944	rBV	1186462	1925931	29.55%	3.289%
10	8.993	997	1004	1014	rBV	882991	1473928	22.62%	2.517%
11	9.398	1070	1073	1080	rVB8	3847	7044	0.11%	0.012%
12	9.716	1119	1127	1136	rBV	700137	1176374	18.05%	2.009%
13	10.257	1209	1219	1228	rBV	1165540	1958981	30.06%	3.346%
14	10.628	1274	1282	1290	rBV	1176061	1893509	29.06%	3.234%
15	10.775	1297	1307	1321	rBV	1069412	1908260	29.28%	3.259%
16	12.216	1545	1552	1556	rBV2	21868	35156	0.54%	0.060%
17	13.363	1742	1747	1753	rVB	18094	31563	0.48%	0.054%
18	13.434	1755	1759	1762	rBV4	5269	7245	0.11%	0.012%
19	13.881	1829	1835	1847	rBV	1830911	2479137	38.04%	4.234%
20	14.157	1875	1882	1896	rBV	2166329	3260868	50.04%	5.569%
21	14.463	1928	1934	1943	rBV	1586047	2343779	35.97%	4.003%
22	14.686	1965	1972	1987	rBV	686354	1177784	18.07%	2.012%
23	14.875	2000	2004	2010	rVB8	7410	15625	0.24%	0.027%
24	15.022	2025	2029	2034	rVB8	6118	9907	0.15%	0.017%
25	15.381	2086	2090	2096	rBV5	10468	22862	0.35%	0.039%
26	15.457	2096	2103	2110	rBV	2706120	3908173	59.97%	6.675%
27	15.586	2120	2125	2132	rBV	220418	314523	4.83%	0.537%
28	15.698	2141	2144	2148	rVB3	11615	17690	0.27%	0.030%
29	16.239	2233	2236	2241	rBV7	9966	15010	0.23%	0.026%
30	17.216	2396	2402	2408	rBV	2009655	2837050	43.54%	4.845%
31	17.263	2408	2410	2413	rVV	39789	46395	0.71%	0.079%
32	17.316	2413	2419	2431	rVB2	3090009	4442846	68.18%	7.588%
33	17.480	2442	2447	2457	rBV2	60768	128877	1.98%	0.220%
34	19.127	2725	2727	2732	rVB	49114	54077	0.83%	0.092%
35	19.557	2794	2800	2811	rBV	4293837	5740520	88.09%	9.804%
36	21.310	3093	3098	3103	rBV	2749009	3523354	54.07%	6.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018931.D
Acq On : 19 Dec 2023 05:29
Operator : MA/JU
Sample : PB157879BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK879

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.527	3469	3475	3490	rVB2	3100858	6516500	100.00%	11.129%
38	23.680	3496	3501	3514	rVB	1928083	3848685	59.06%	6.573%




Sum of corrected areas: 58551638

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018931.D
Acq On : 19 Dec 2023 05:29
Operator : MA/JU
Sample : PB157879BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK879

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

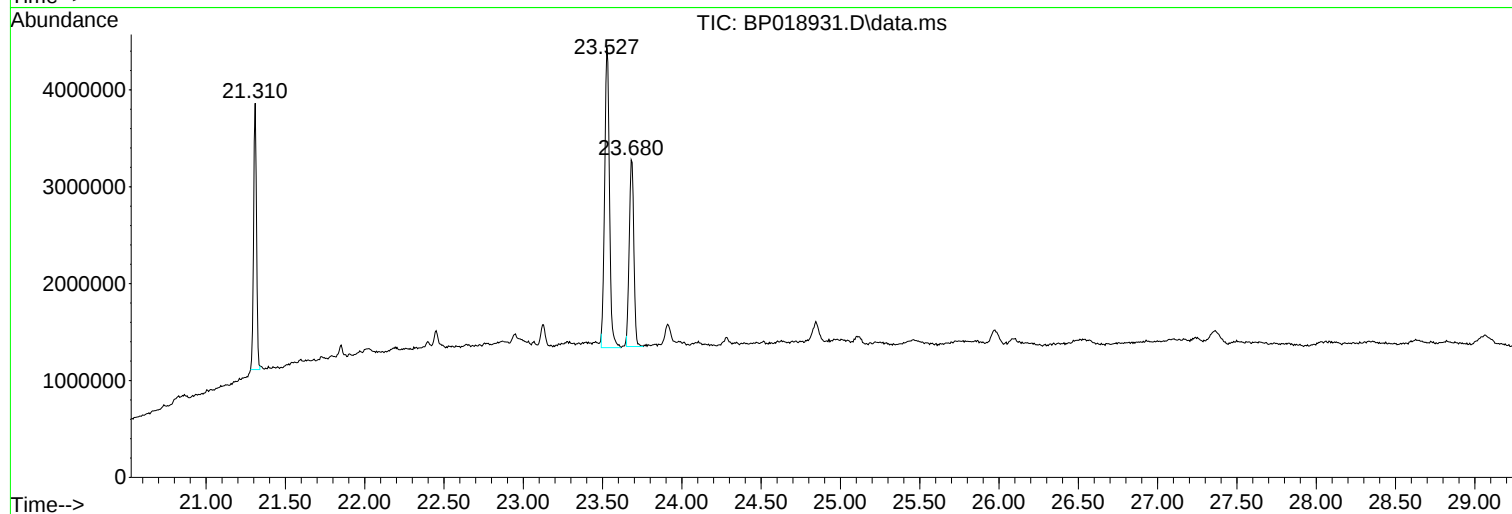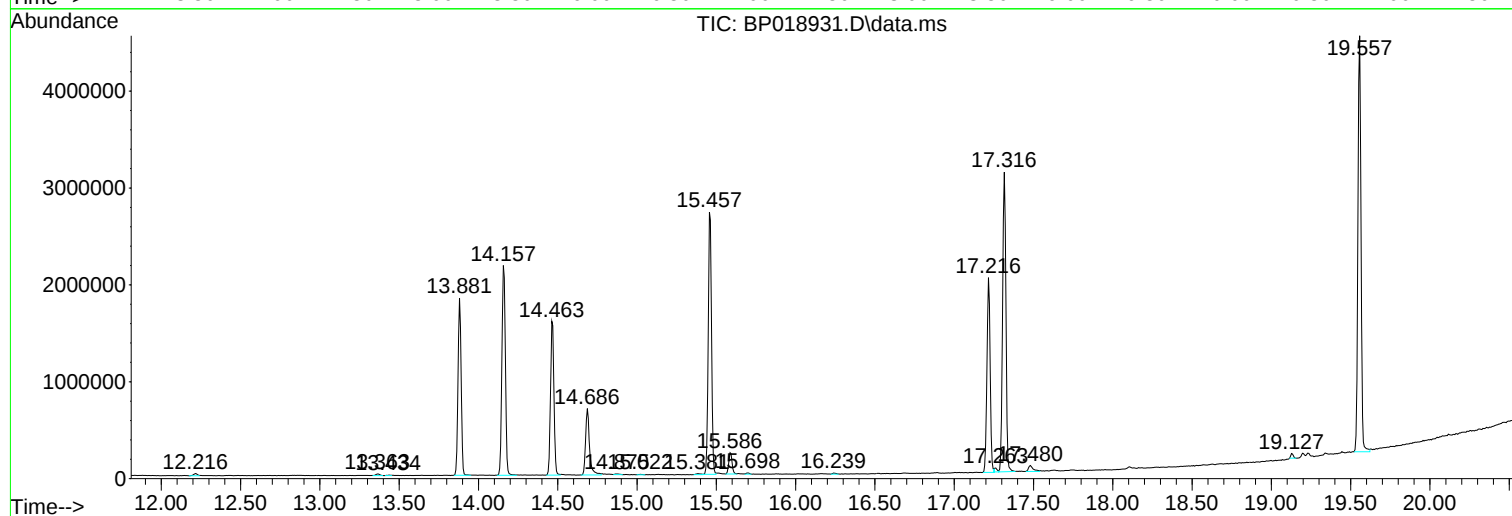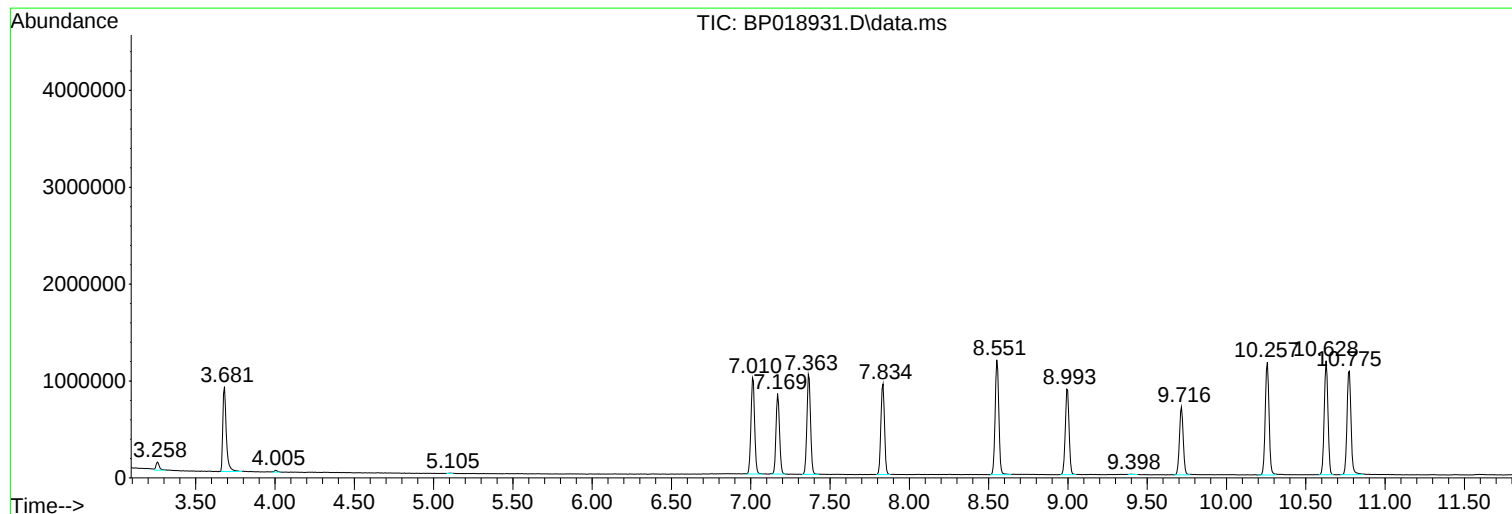

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018931.D
Acq On : 19 Dec 2023 05:29
Operator : MA/JU
Sample : PB157879BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK879

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018931.D
Acq On : 19 Dec 2023 05:29
Operator : MA/JU
Sample : PB157879BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK879

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc