

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
 Data File : BP018932.D
 Acq On : 19 Dec 2023 06:03
 Operator : MA/JU
 Sample : PB157772TB 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB772

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	35	rVB	77876	98548	1.58%	0.180%
2	3.681	96	101	114	rBV	825312	1278214	20.49%	2.339%
3	3.999	152	155	160	rVB2	13629	20367	0.33%	0.037%
4	7.011	660	667	676	rVB	974062	1519194	24.36%	2.780%
5	7.169	688	694	705	rVB	798307	1219338	19.55%	2.231%
6	7.363	720	727	739	rBV	1005301	1575671	25.26%	2.883%
7	7.834	799	807	817	rBV	751294	1195812	19.17%	2.188%
8	8.552	922	929	944	rBV	1161438	1857271	29.78%	3.398%
9	8.993	997	1004	1014	rBV	865549	1413814	22.67%	2.587%
10	9.716	1117	1127	1135	rBV	678630	1131939	18.15%	2.071%
11	10.257	1211	1219	1230	rBV	1123198	1876674	30.09%	3.434%
12	10.628	1274	1282	1290	rBV	923116	1517280	24.33%	2.776%
13	10.769	1298	1306	1319	rBV	1059697	1816283	29.12%	3.323%
14	11.587	1439	1445	1450	rBV9	7405	18986	0.30%	0.035%
15	12.216	1547	1552	1559	rBV	21707	37527	0.60%	0.069%
16	12.822	1649	1655	1661	rBV10	3770	11475	0.18%	0.021%
17	13.363	1740	1747	1752	rBV8	7762	13789	0.22%	0.025%
18	13.434	1755	1759	1763	rBV7	3925	7082	0.11%	0.013%
19	13.881	1828	1835	1848	rBV	1752116	2414471	38.71%	4.418%
20	14.157	1875	1882	1890	rBV	2072173	3161921	50.69%	5.785%
21	14.463	1927	1934	1943	rBV	1284342	1921752	30.81%	3.516%
22	14.687	1965	1972	1983	rBV	649807	1152615	18.48%	2.109%
23	15.387	2085	2091	2094	rBV7	9702	17699	0.28%	0.032%
24	15.457	2094	2103	2111	rBV	2749788	3862676	61.93%	7.067%
25	15.587	2120	2125	2137	rVV	247655	344170	5.52%	0.630%
26	15.698	2140	2144	2149	rVB4	13511	23024	0.37%	0.042%
27	16.245	2233	2237	2243	rVB7	9852	16130	0.26%	0.030%
28	17.216	2395	2402	2407	rBV	1657447	2358190	37.81%	4.315%
29	17.257	2407	2409	2413	rVV	38153	50713	0.81%	0.093%
30	17.316	2413	2419	2430	rVB	3136140	4445753	71.28%	8.134%
31	17.475	2442	2446	2456	rBV2	49050	110377	1.77%	0.202%
32	19.128	2725	2727	2731	rVB	47450	49075	0.79%	0.090%
33	19.198	2736	2739	2742	rBV	43554	63933	1.02%	0.117%
34	19.557	2794	2800	2811	rBV	4258031	5751984	92.22%	10.524%
35	21.310	3093	3098	3103	rBV	2222037	2906124	46.59%	5.317%
36	23.527	3469	3475	3487	rVB2	3080494	6237422	100.00%	11.412%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018932.D
Acq On : 19 Dec 2023 06:03
Operator : MA/JU
Sample : PB157772TB 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB772

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37 23.680 3495 3501 3510 rVB 1587444 3159447 50.65% 5.781%




Sum of corrected areas: 54656740

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018932.D
Acq On : 19 Dec 2023 06:03
Operator : MA/JU
Sample : PB157772TB 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB772

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

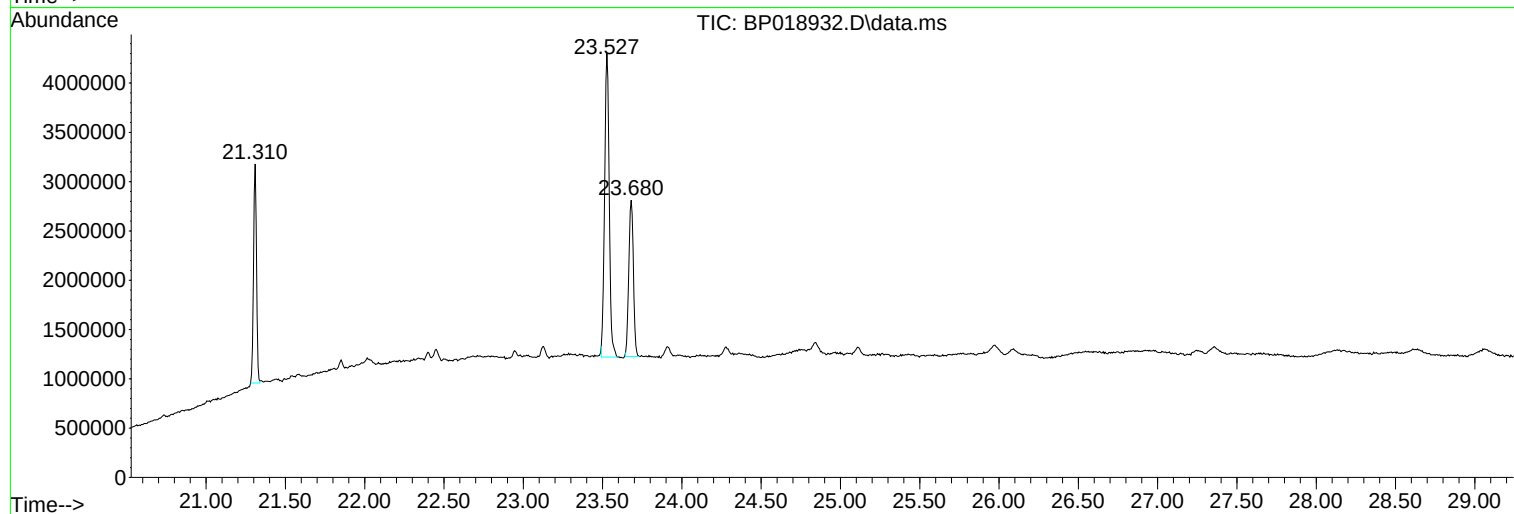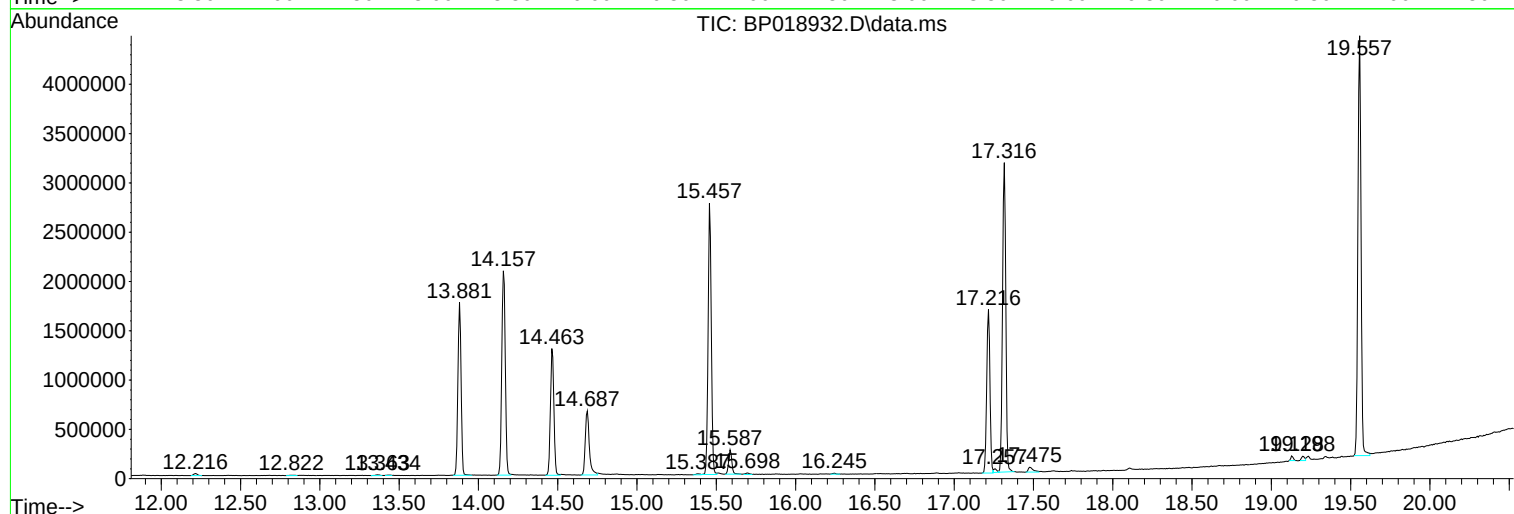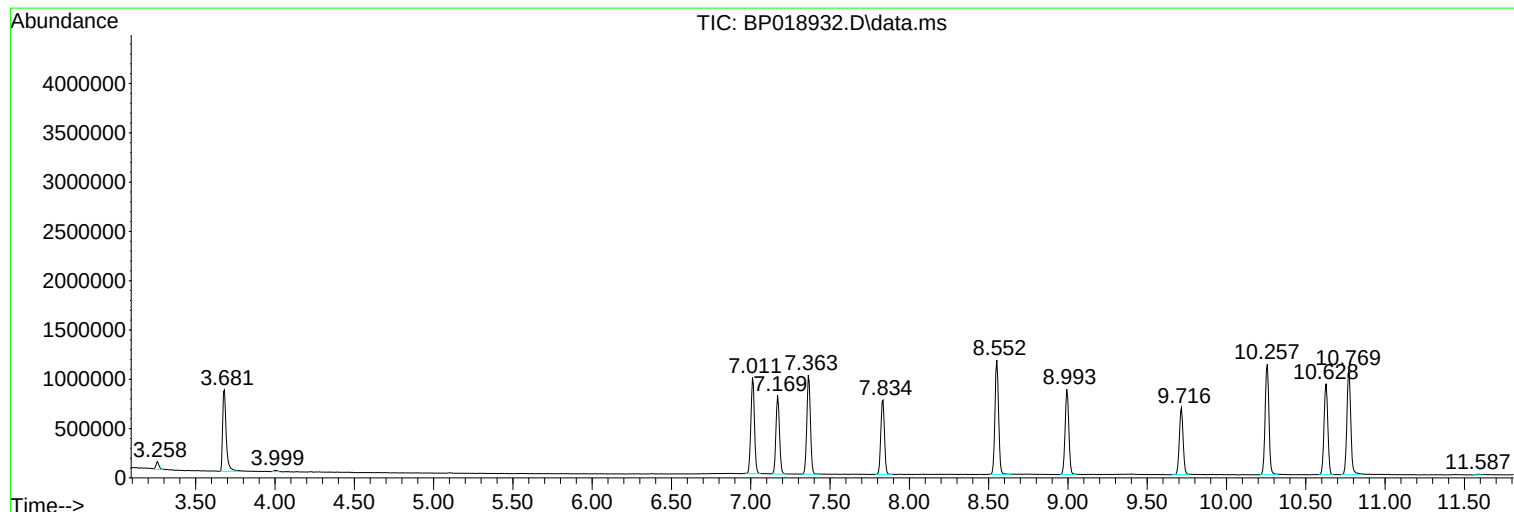

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018932.D
Acq On : 19 Dec 2023 06:03
Operator : MA/JU
Sample : PB157772TB 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB772

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121823\
Data File : BP018932.D
Acq On : 19 Dec 2023 06:03
Operator : MA/JU
Sample : PB157772TB 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB772

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------