

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121824\
 Data File : BP023501.D
 Acq On : 18 Dec 2024 17:01
 Operator : RC/JU
 Sample : P5235-02 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023501.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	15	19	21	rBV2	51026	69953	0.90%	0.098%
2	3.128	21	24	34	rVB	388542	482528	6.22%	0.677%
3	3.428	73	75	80	rVB2	31281	38585	0.50%	0.054%
4	3.522	88	91	93	rBV	115506	149081	1.92%	0.209%
5	3.793	133	137	144	rVB2	71198	112330	1.45%	0.158%
6	4.064	179	183	190	rVV	83081	109789	1.42%	0.154%
7	4.134	192	195	201	rVB5	16196	23445	0.30%	0.033%
8	4.246	209	214	220	rBV	115241	162287	2.09%	0.228%
9	4.311	221	225	234	rVB	76119	117584	1.52%	0.165%
10	4.681	283	288	294	rBV	166567	231987	2.99%	0.325%
11	5.269	385	388	399	rVB2	19337	42750	0.55%	0.060%
12	5.528	428	432	435	rBV3	12855	17831	0.23%	0.025%
13	6.434	581	586	596	rBV5	26101	47276	0.61%	0.066%
14	6.675	619	627	631	rBV5	7729	21714	0.28%	0.030%
15	6.752	634	640	656	rVV	191118	457755	5.90%	0.642%
16	6.881	656	662	679	rVV	783501	1220588	15.74%	1.712%
17	6.999	679	682	689	rVB4	8870	13271	0.17%	0.019%
18	7.081	689	696	711	rBV	780523	1327246	17.12%	1.862%
19	7.299	730	733	738	rVB5	8312	14256	0.18%	0.020%
20	7.528	765	772	781	rBV	834741	1414782	18.25%	1.985%
21	7.599	783	784	796	rVB7	16990	31909	0.41%	0.045%
22	7.863	825	829	835	rVB7	10113	18729	0.24%	0.026%
23	8.252	889	895	908	rBV	646279	1281179	16.53%	1.797%
24	8.357	910	913	920	rVV3	23688	44863	0.58%	0.063%
25	8.428	920	925	932	rVB6	12157	27377	0.35%	0.038%
26	8.669	956	966	988	rBV	792960	1454518	18.76%	2.040%
27	8.887	999	1003	1006	rBV2	16285	28825	0.37%	0.040%
28	8.916	1006	1008	1014	rVV3	14321	22809	0.29%	0.032%
29	9.040	1026	1029	1034	rVB7	6149	8400	0.11%	0.012%
30	9.104	1036	1040	1045	rBV7	9830	16078	0.21%	0.023%
31	9.240	1055	1063	1067	rBV10	8771	20811	0.27%	0.029%
32	9.381	1080	1087	1102	rBV	655606	1261351	16.27%	1.769%
33	9.687	1136	1139	1146	rBV9	6198	9807	0.13%	0.014%
34	9.822	1160	1162	1170	rVB9	5293	9703	0.13%	0.014%
35	9.934	1170	1181	1208	rBV2	1166292	2849691	36.76%	3.998%
36	10.222	1225	1230	1233	rBV2	60161	97680	1.26%	0.137%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121824\
 Data File : BP023501.D
 Acq On : 18 Dec 2024 17:01
 Operator : RC/JU
 Sample : P5235-02 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

37	10.269	1233	1238	1252	rVB	1191453	1978303	25.52%	2.775%
38	10.428	1258	1265	1282	rBV	766257	1625840	20.97%	2.281%
39	10.798	1322	1328	1334	rBV	174929	307840	3.97%	0.432%
40	10.863	1334	1339	1353	rVV	230301	478894	6.18%	0.672%
41	10.951	1353	1354	1361	rVB7	6916	10024	0.13%	0.014%
42	11.104	1374	1380	1392	rVB2	145220	237057	3.06%	0.333%
43	11.481	1436	1444	1452	rBV8	17597	28906	0.37%	0.041%
44	11.604	1459	1465	1471	rBV8	5789	13043	0.17%	0.018%
45	11.710	1481	1483	1494	rVB8	6435	13576	0.18%	0.019%
46	11.810	1494	1500	1503	rBV7	6716	13274	0.17%	0.019%
47	11.875	1506	1511	1518	rVB5	10527	22049	0.28%	0.031%
48	11.987	1522	1530	1539	rBV3	37232	114410	1.48%	0.160%
49	12.428	1600	1605	1610	rBV8	10897	16556	0.21%	0.023%
50	12.687	1638	1649	1663	rBV10	47163	140721	1.82%	0.197%
51	12.969	1692	1697	1701	rVV2	30979	61247	0.79%	0.086%
52	13.028	1701	1707	1718	rVB3	112411	249370	3.22%	0.350%
53	13.145	1722	1727	1736	rBV	58480	114677	1.48%	0.161%
54	13.245	1741	1744	1747	rVV4	22410	29810	0.38%	0.042%
55	13.275	1747	1749	1753	rVV5	12101	18165	0.23%	0.025%
56	13.310	1753	1755	1761	rVB7	5883	8655	0.11%	0.012%
57	13.398	1767	1770	1775	rVB6	7930	12406	0.16%	0.017%
58	13.504	1779	1788	1790	rBV8	7626	13208	0.17%	0.019%
59	13.551	1790	1796	1814	rVV	2678612	3407197	43.95%	4.780%
60	13.839	1832	1845	1862	rBV	2200759	3306768	42.65%	4.639%
61	13.992	1864	1871	1883	rBV2	55603	165359	2.13%	0.232%
62	14.145	1890	1897	1907	rBV	2010331	2973978	38.36%	4.172%
63	14.275	1917	1919	1924	rVB6	5651	7847	0.10%	0.011%
64	14.475	1946	1953	1957	rBV	106384	222060	2.86%	0.312%
65	14.957	2031	2035	2038	rVB4	12103	14289	0.18%	0.020%
66	15.034	2045	2048	2053	rVB5	6389	7806	0.10%	0.011%
67	15.157	2061	2069	2085	rBV	2458721	4818744	62.15%	6.760%
68	15.316	2090	2096	2107	rBV	1093578	1854947	23.93%	2.602%
69	15.539	2129	2134	2139	rBV	98567	136993	1.77%	0.192%
70	16.275	2252	2259	2260	rBV7	5649	10627	0.14%	0.015%
71	16.469	2289	2292	2299	rBV	18783	31986	0.41%	0.045%
72	16.739	2334	2338	2345	rVB2	12717	23986	0.31%	0.034%
73	16.951	2367	2374	2384	rBV2	2562223	3853409	49.70%	5.406%
74	17.051	2385	2391	2406	rVB2	4063135	6182464	79.74%	8.673%
75	17.198	2414	2416	2421	rVB3	9557	15254	0.20%	0.021%
76	17.386	2443	2448	2450	rBV5	8647	15519	0.20%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121824\
 Data File : BP023501.D
 Acq On : 18 Dec 2024 17:01
 Operator : RC/JU
 Sample : P5235-02 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

77	17.622	2484	2488	2496	rVB5	15670	36621	0.47%	0.051%
78	17.710	2500	2503	2508	rVV3	12131	20062	0.26%	0.028%
79	17.810	2517	2520	2526	rBV3	14242	25735	0.33%	0.036%
80	17.886	2528	2533	2541	rBV	230120	354370	4.57%	0.497%
81	18.169	2579	2581	2585	rBV5	9753	15688	0.20%	0.022%
82	18.280	2597	2600	2606	rBV	19106	30609	0.39%	0.043%
83	18.980	2715	2719	2724	rVB2	60014	78428	1.01%	0.110%
84	19.063	2728	2733	2737	rBV3	48783	87114	1.12%	0.122%
85	19.098	2737	2739	2748	rVB10	21559	41144	0.53%	0.058%
86	19.227	2757	2761	2770	rBV	89563	177918	2.29%	0.250%
87	19.433	2790	2796	2808	rBV	5313233	7752959	100.00%	10.876%
88	21.374	3121	3126	3137	rBV2	2522359	4464546	57.59%	6.263%
89	24.345	3621	3631	3644	rVB	2852417	7639843	98.54%	10.717%
90	24.551	3657	3666	3685	rVB	1796361	4743350	61.18%	6.654%




Sum of corrected areas: 71284419

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121824\
Data File : BP023501.D
Acq On : 18 Dec 2024 17:01
Operator : RC/JU
Sample : P5235-02 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COAT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

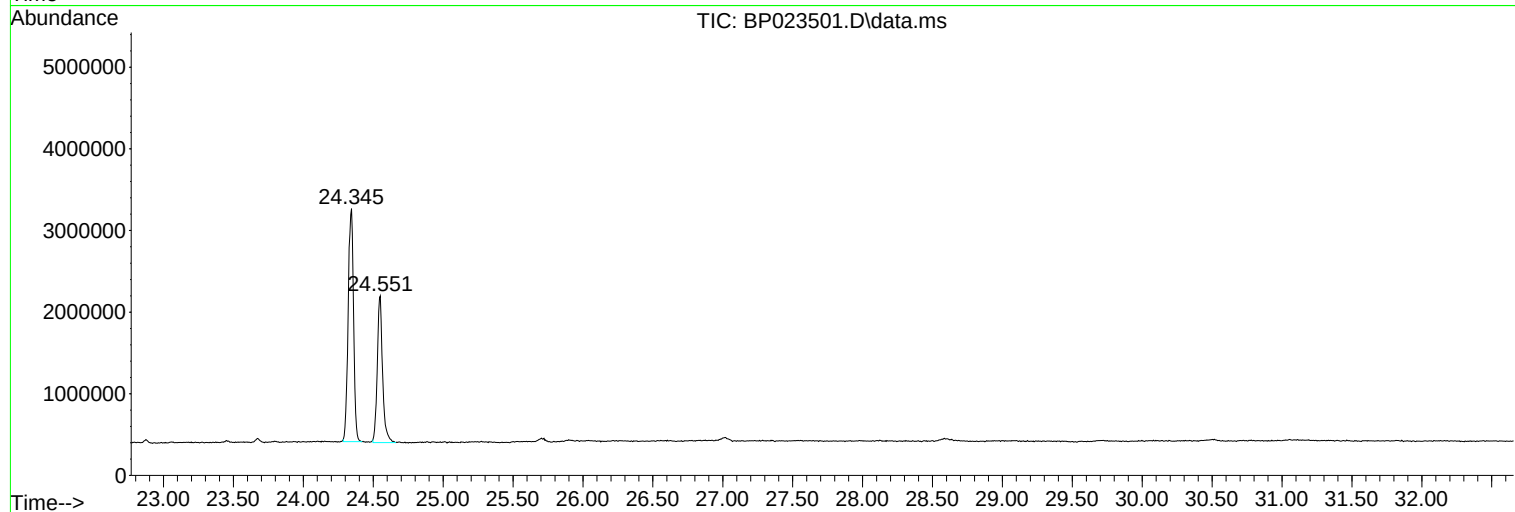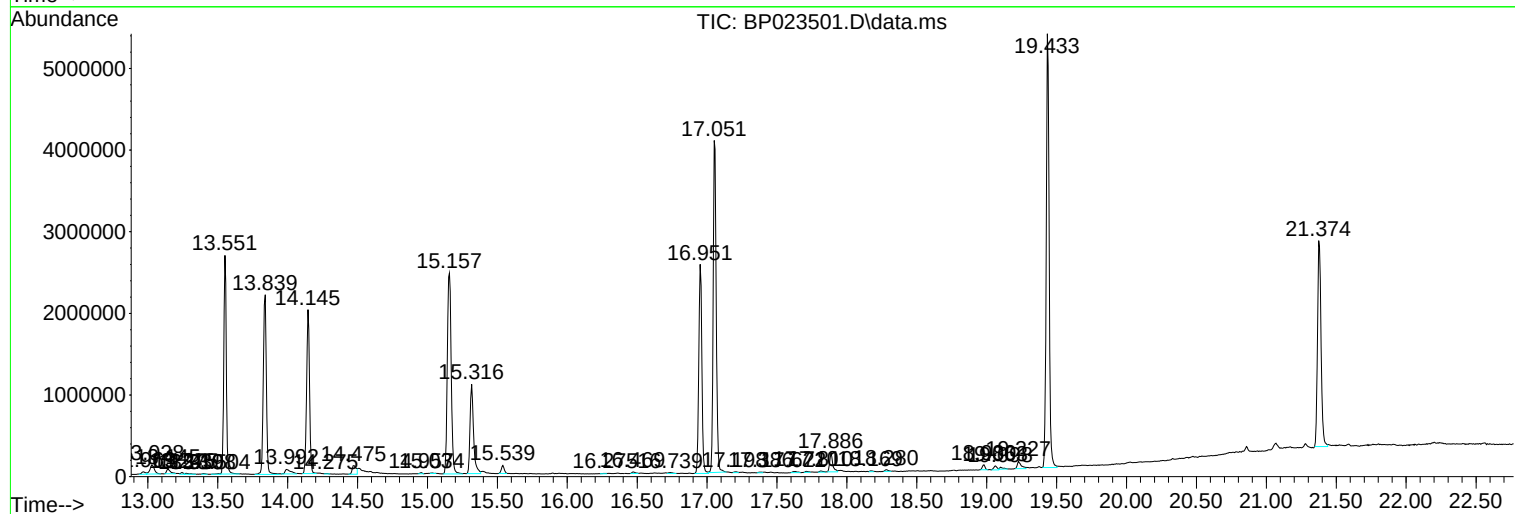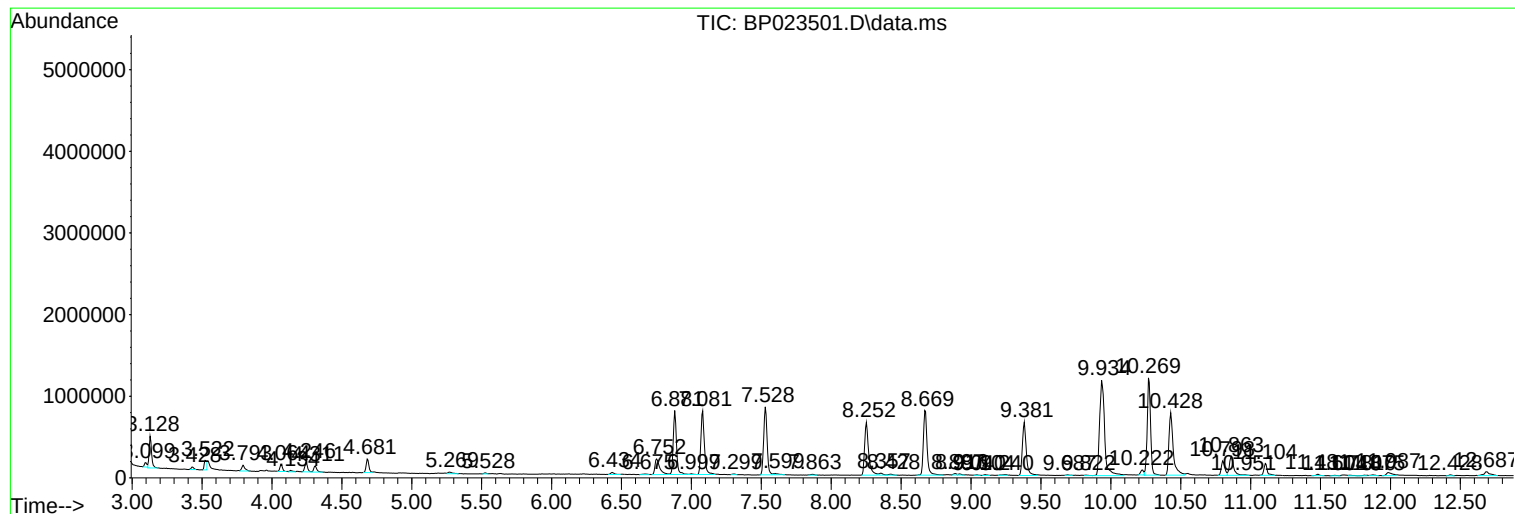

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121824\
Data File : BP023501.D
Acq On : 18 Dec 2024 17:01
Operator : RC/JU
Sample : P5235-02 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl butyrate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.681	3.28 ng/ul	231987	1,4-Dichlorobenzene-d4	7.528

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl butyrate	130	C7H14O2	000638-11-9	90
2			Isopropyl butyrate	130	C7H14O2	000638-11-9	86
3			Isopropyl butyrate	130	C7H14O2	000638-11-9	83
4			Propanoic acid, 2-methyl-, propy...	130	C7H14O2	000644-49-5	72
5			Propanoic acid, 2-methyl-, propy...	130	C7H14O2	000644-49-5	64

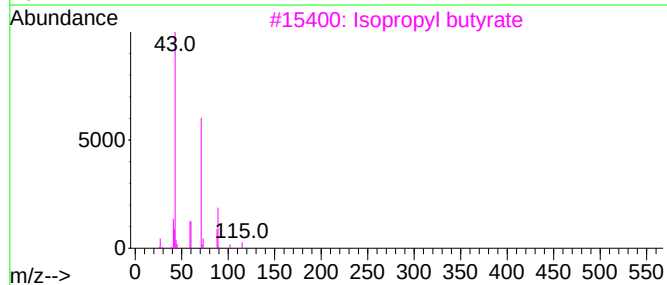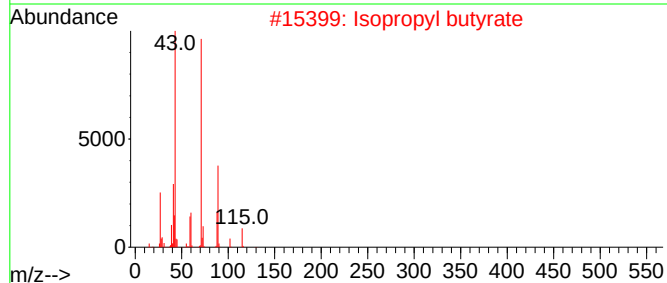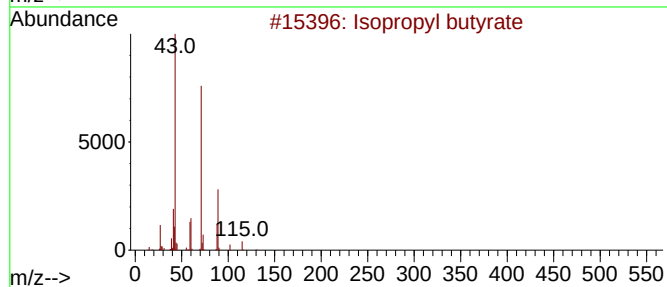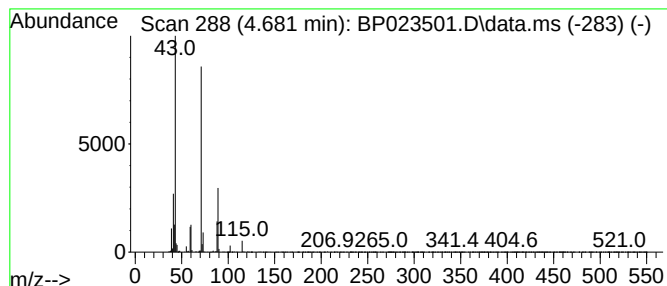

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121824\
Data File : BP023501.D
Acq On : 18 Dec 2024 17:01
Operator : RC/JU
Sample : P5235-02 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl butyrate	4.681	3.3	ng/u1	231987	1	7.528	1414780	20.0