

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
 Data File : BP018952.D
 Acq On : 20 Dec 2023 09:49
 Operator : MA/JU
 Sample : PB157879BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK879

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	38	rVB	52779	70606	1.43%	0.168%
2	3.669	95	99	113	rBV	637744	895503	18.14%	2.136%
3	3.999	151	155	159	rVB2	10820	15545	0.31%	0.037%
4	6.957	654	658	659	rBV3	5314	5504	0.11%	0.013%
5	6.999	659	665	678	rVB	679918	1076348	21.80%	2.567%
6	7.163	686	693	701	rVB	550649	832057	16.85%	1.984%
7	7.357	719	726	740	rBV	695668	1090365	22.09%	2.601%
8	7.822	799	805	815	rVB	601925	960723	19.46%	2.291%
9	8.540	920	927	940	rBV	793455	1297609	26.29%	3.095%
10	8.987	996	1003	1014	rBV	604872	983689	19.93%	2.346%
11	9.710	1117	1126	1133	rBV	480050	793169	16.07%	1.892%
12	10.246	1210	1217	1235	rBV	740755	1297018	26.27%	3.093%
13	10.622	1274	1281	1291	rVB	756037	1234882	25.02%	2.945%
14	10.763	1298	1305	1327	rBV	706185	1278439	25.90%	3.049%
15	12.210	1547	1551	1561	rVB2	13942	26357	0.53%	0.063%
16	13.363	1742	1747	1753	rBV4	10413	19985	0.40%	0.048%
17	13.434	1753	1759	1765	rVV10	2424	5558	0.11%	0.013%
18	13.881	1827	1835	1848	rBV	1263147	1770483	35.86%	4.223%
19	14.157	1875	1882	1893	rBV	1518904	2217431	44.92%	5.289%
20	14.463	1927	1934	1943	rBV	1069051	1617256	32.76%	3.857%
21	14.681	1964	1971	1991	rBV	479779	915258	18.54%	2.183%
22	15.457	2095	2103	2117	rBV	1952042	2820079	57.13%	6.726%
23	15.581	2118	2124	2139	rVV	546757	769541	15.59%	1.835%
24	15.692	2139	2143	2148	rVB4	9249	15139	0.31%	0.036%
25	16.239	2232	2236	2240	rBV5	6773	9564	0.19%	0.023%
26	17.004	2359	2366	2368	rBV4	5545	10902	0.22%	0.026%
27	17.210	2394	2401	2412	rBV	1382939	2037374	41.27%	4.859%
28	17.310	2412	2418	2435	rVV	2143353	3141803	63.64%	7.493%
29	18.104	2549	2553	2558	rBV8	14223	22452	0.45%	0.054%
30	19.127	2723	2727	2731	rBV3	32034	43334	0.88%	0.103%
31	19.198	2735	2739	2746	rVV	29217	47132	0.95%	0.112%
32	19.551	2793	2799	2810	rBV	3020700	4036481	81.77%	9.627%
33	21.304	3092	3097	3106	rBV	2144050	2663507	53.95%	6.353%
34	23.515	3466	3473	3486	rVB2	2475999	4936560	100.00%	11.774%
35	23.668	3493	3499	3507	rVB	1509824	2970547	60.17%	7.085%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018952.D
Acq On : 20 Dec 2023 09:49
Operator : MA/JU
Sample : PB157879BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK879

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 41928200

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018952.D
Acq On : 20 Dec 2023 09:49
Operator : MA/JU
Sample : PB157879BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK879

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

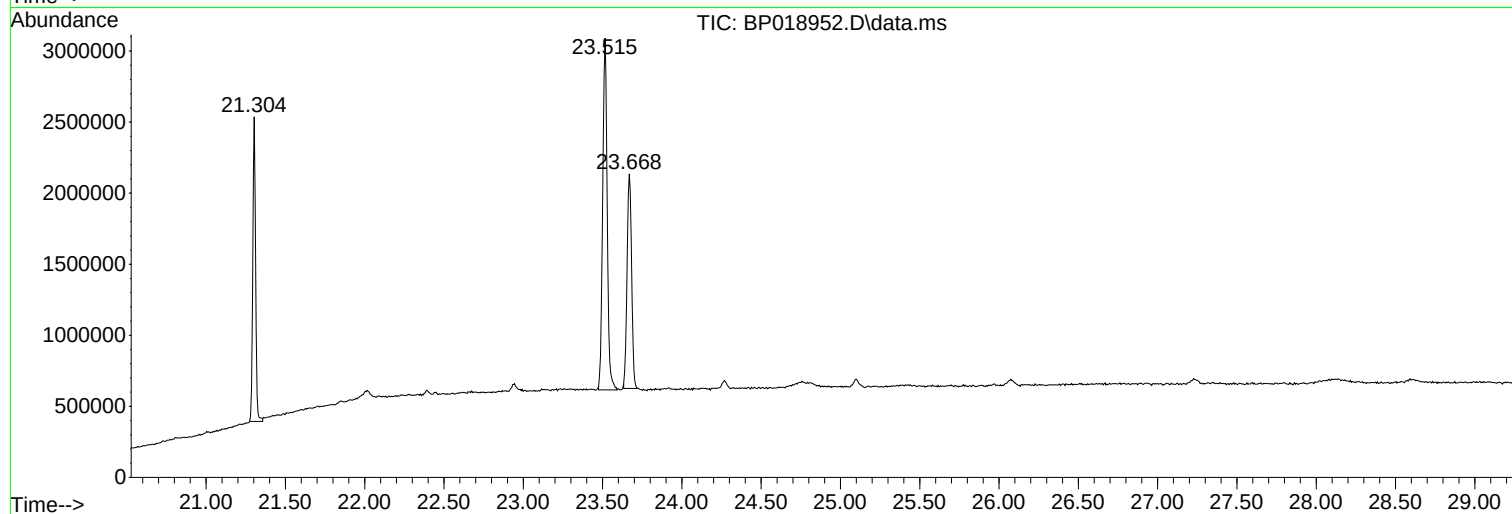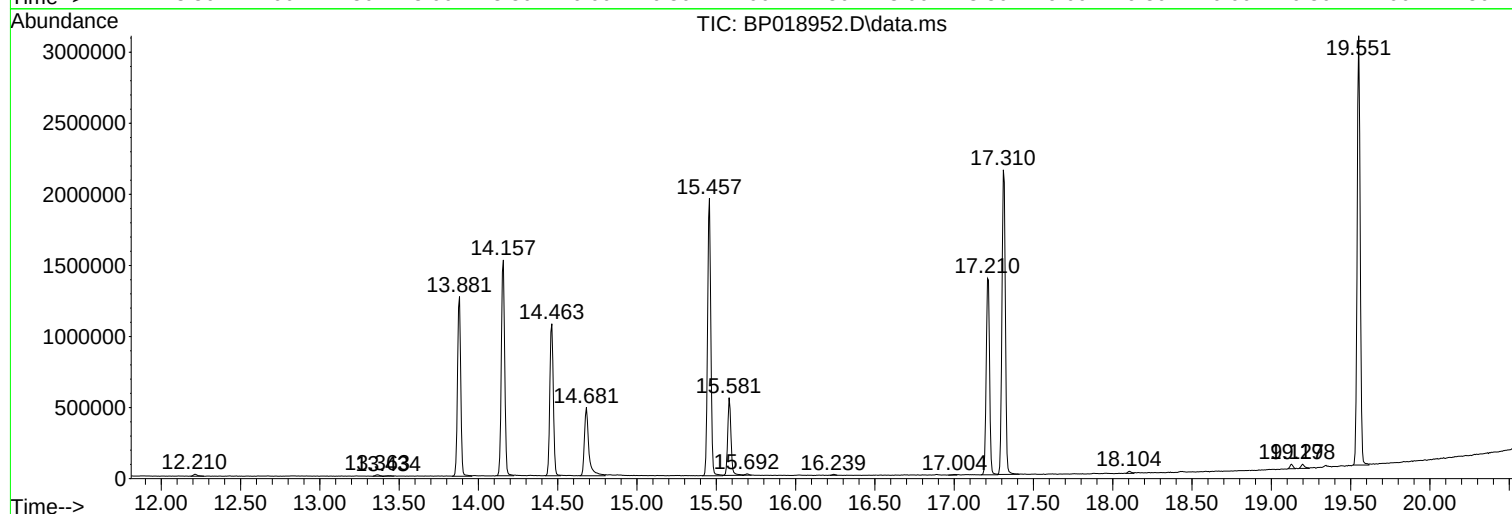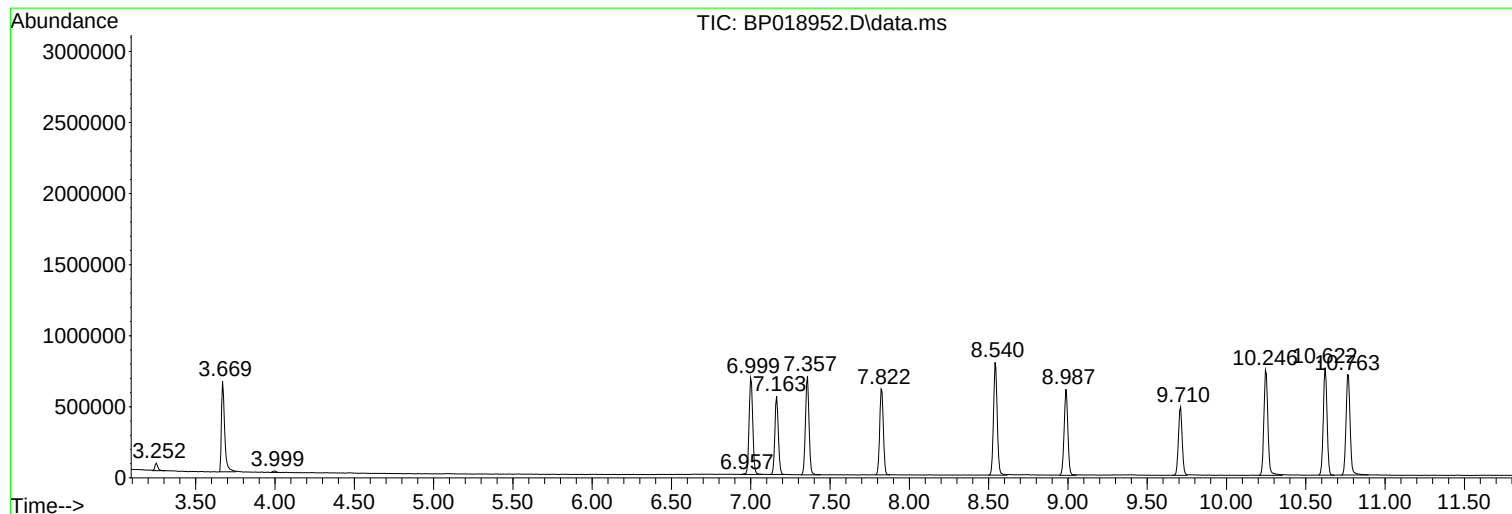

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018952.D
Acq On : 20 Dec 2023 09:49
Operator : MA/JU
Sample : PB157879BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK879

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018952.D
Acq On : 20 Dec 2023 09:49
Operator : MA/JU
Sample : PB157879BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK879

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc