

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
 Data File : BP018961.D
 Acq On : 20 Dec 2023 15:07
 Operator : MA/JU
 Sample : 05850-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	35	rBV	23918	31109	0.80%	0.110%
2	3.675	96	100	109	rBV	150286	211814	5.46%	0.752%
3	3.904	135	139	145	rVB3	10195	16698	0.43%	0.059%
4	3.999	152	155	159	rVB3	8043	10822	0.28%	0.038%
5	4.940	307	315	317	rBV6	5941	12528	0.32%	0.044%
6	5.134	343	348	356	rVB	58182	83840	2.16%	0.298%
7	6.998	660	665	677	rVB	88453	144509	3.73%	0.513%
8	7.163	687	693	706	rVB	375571	581399	14.99%	2.064%
9	7.357	719	726	736	rBV	359237	561296	14.47%	1.992%
10	7.710	783	786	792	rVB5	4578	7547	0.19%	0.027%
11	7.828	798	806	817	rBV	399174	674832	17.40%	2.395%
12	8.175	859	865	870	rBV	25831	40097	1.03%	0.142%
13	8.540	921	927	939	rBV	247880	415381	10.71%	1.474%
14	8.987	994	1003	1014	rBV	423041	689603	17.78%	2.448%
15	9.398	1067	1073	1076	rVV6	8493	15564	0.40%	0.055%
16	9.440	1076	1080	1086	rVB8	5169	10672	0.28%	0.038%
17	9.710	1117	1126	1133	rBV	310685	531136	13.70%	1.885%
18	10.245	1209	1217	1235	rBV	469658	818680	21.11%	2.906%
19	10.487	1253	1258	1263	rVB5	5983	9025	0.23%	0.032%
20	10.622	1272	1281	1288	rBV	500589	834846	21.53%	2.963%
21	10.763	1298	1305	1322	rBV	385088	689624	17.78%	2.448%
22	11.892	1491	1497	1504	rVB6	7532	13063	0.34%	0.046%
23	12.210	1546	1551	1558	rVV2	9177	16632	0.43%	0.059%
24	13.280	1727	1733	1742	rVB7	16426	28849	0.74%	0.102%
25	13.363	1742	1747	1753	rBV3	11229	19933	0.51%	0.071%
26	13.475	1763	1766	1772	rVB3	6632	9331	0.24%	0.033%
27	13.875	1827	1834	1846	rBV	922184	1289434	33.25%	4.577%
28	14.151	1875	1881	1900	rBV	1100158	1625757	41.92%	5.770%
29	14.333	1908	1912	1916	rBV7	2586	4519	0.12%	0.016%
30	14.463	1925	1934	1946	rBV	739252	1115763	28.77%	3.960%
31	14.692	1966	1973	1985	rBV2	37721	98691	2.54%	0.350%
32	14.880	2000	2005	2013	rVB2	3718	10261	0.26%	0.036%
33	15.451	2095	2102	2117	rBV	1407790	2088868	53.86%	7.414%
34	15.580	2118	2124	2135	rVV	260820	392466	10.12%	1.393%
35	15.692	2139	2143	2148	rVB5	7427	12512	0.32%	0.044%
36	16.239	2233	2236	2240	rBV6	5347	6652	0.17%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
 Data File : BP018961.D
 Acq On : 20 Dec 2023 15:07
 Operator : MA/JU
 Sample : 05850-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.610	2296	2299	2301	rBV4	3290	4031	0.10%	0.014%
38	16.892	2343	2347	2350	rBV5	3146	4209	0.11%	0.015%
39	17.210	2394	2401	2411	rBV	1003468	1425016	36.75%	5.058%
40	17.310	2411	2418	2431	rVV	1729615	2423247	62.49%	8.601%
41	18.098	2548	2552	2560	rBV3	41147	63336	1.63%	0.225%
42	19.127	2723	2727	2732	rBV3	25587	35520	0.92%	0.126%
43	19.198	2735	2739	2742	rVV	19751	26234	0.68%	0.093%
44	19.339	2759	2763	2768	rBV3	27171	39099	1.01%	0.139%
45	19.545	2793	2798	2806	rBV	2260983	3116850	80.37%	11.063%
46	21.304	3092	3097	3106	rBV	1404720	1867873	48.17%	6.630%
47	23.509	3465	3472	3487	rVB2	1875716	3878000	100.00%	13.764%
48	23.662	3492	3498	3510	rVB	1100545	2167229	55.89%	7.692%




Sum of corrected areas: 28174397

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018961.D
Acq On : 20 Dec 2023 15:07
Operator : MA/JU
Sample : 05850-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

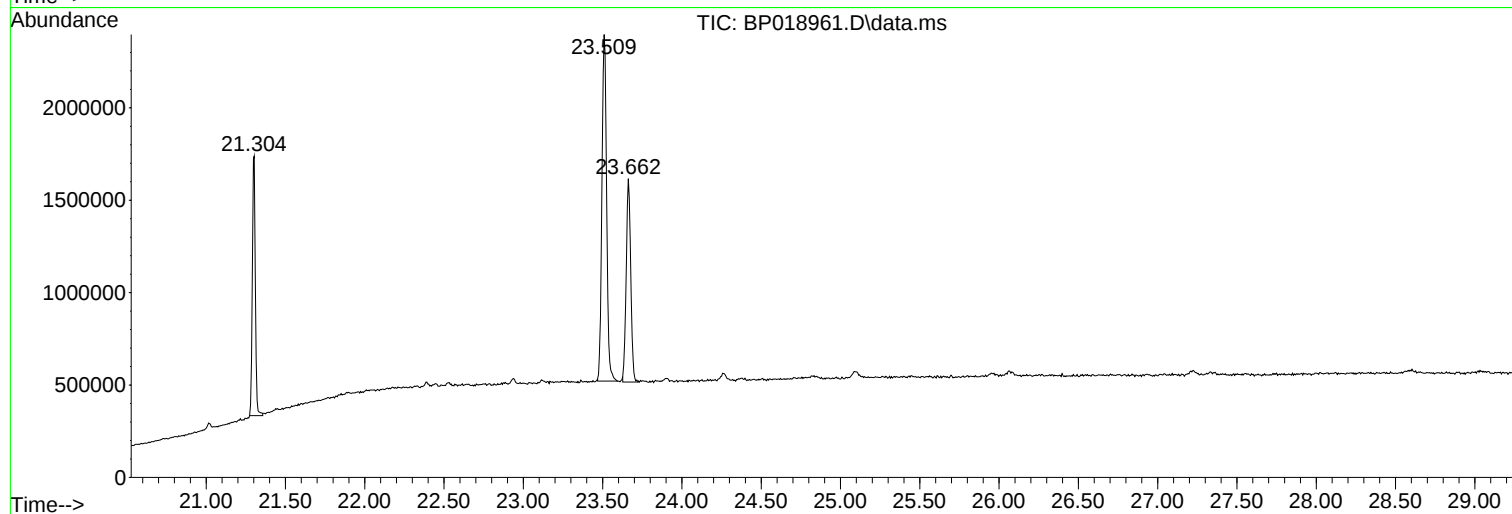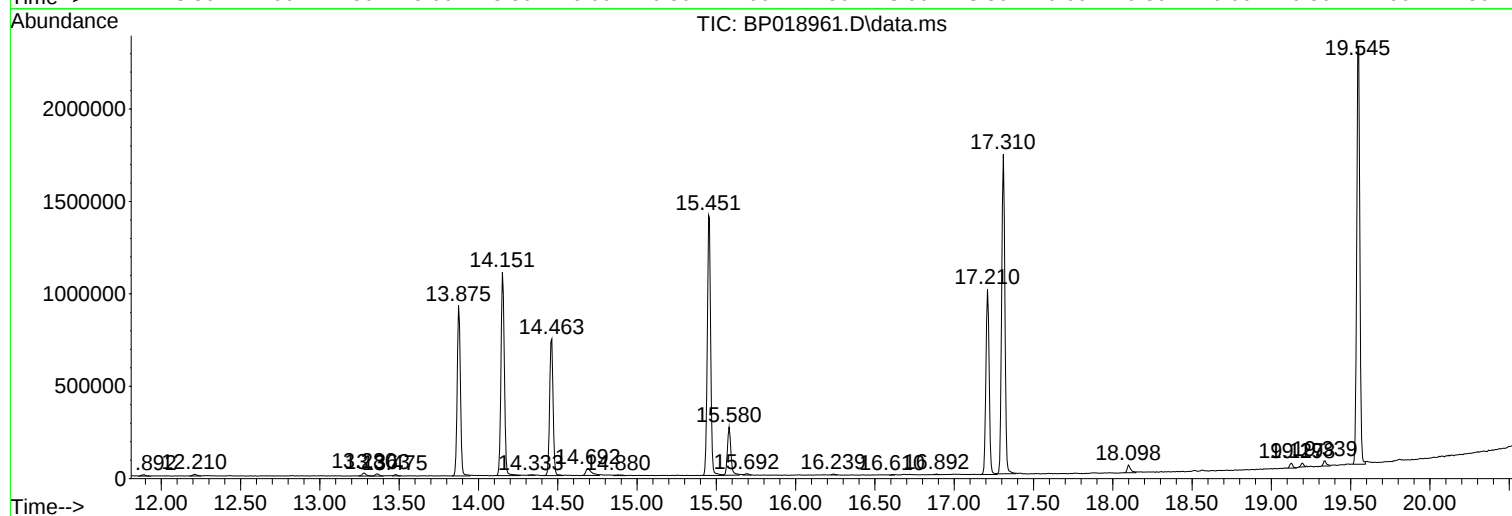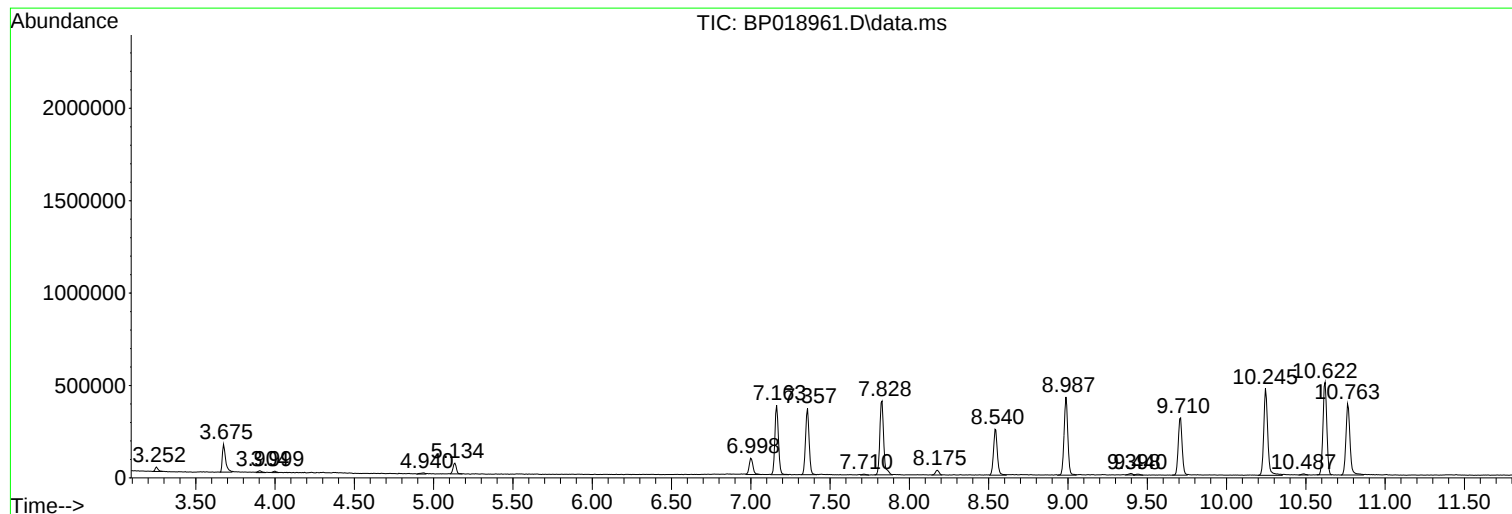

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018961.D
Acq On : 20 Dec 2023 15:07
Operator : MA/JU
Sample : 05850-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018961.D
Acq On : 20 Dec 2023 15:07
Operator : MA/JU
Sample : 05850-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QM1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc