

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
 Data File : BP018964.D
 Acq On : 20 Dec 2023 17:11
 Operator : MA/JU
 Sample : PB157887BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK887

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	36	rVB	40377	51174	1.30%	0.147%
2	3.669	95	99	115	rBV	462743	670340	17.04%	1.932%
3	3.999	152	155	159	rVB	9149	11870	0.30%	0.034%
4	5.134	344	348	352	rVB3	5395	8927	0.23%	0.026%
5	6.999	655	665	675	rVB	500463	784964	19.95%	2.262%
6	7.163	687	693	701	rVB	406932	616678	15.68%	1.777%
7	7.358	719	726	736	rBV	515651	807440	20.52%	2.327%
8	7.822	797	805	814	rBV	432807	692220	17.60%	1.995%
9	8.540	920	927	938	rBV	595898	967592	24.59%	2.789%
10	8.987	994	1003	1014	rBV	452616	750796	19.08%	2.164%
11	9.399	1069	1073	1082	rVB	2708	6644	0.17%	0.019%
12	9.710	1118	1126	1135	rBV	370514	622236	15.82%	1.793%
13	10.246	1209	1217	1235	rBV	586623	1013554	25.76%	2.921%
14	10.622	1274	1281	1294	rVB	551592	920288	23.39%	2.652%
15	10.763	1295	1305	1321	rBV	587812	1011480	25.71%	2.915%
16	12.210	1545	1551	1559	rVB2	11232	21587	0.55%	0.062%
17	13.363	1742	1747	1752	rVB4	11979	18580	0.47%	0.054%
18	13.875	1826	1834	1846	rBV	1151898	1604622	40.79%	4.625%
19	14.151	1874	1881	1890	rBV	1310443	1891681	48.08%	5.452%
20	14.457	1926	1933	1943	rBV	905876	1326858	33.73%	3.824%
21	14.681	1964	1971	1988	rBV	362635	742485	18.87%	2.140%
22	15.451	2095	2102	2115	rBV	1747044	2467118	62.71%	7.111%
23	15.581	2118	2124	2133	rBV	474358	669817	17.03%	1.931%
24	15.692	2140	2143	2148	rVB4	9371	12311	0.31%	0.035%
25	16.239	2232	2236	2241	rVB6	6810	10625	0.27%	0.031%
26	16.686	2309	2312	2316	rBV6	2345	4540	0.12%	0.013%
27	16.886	2341	2346	2349	rBV7	4269	5951	0.15%	0.017%
28	17.210	2394	2401	2411	rBV	1314591	1783961	45.35%	5.142%
29	17.310	2412	2418	2433	rVB	1988551	2810356	71.44%	8.100%
30	18.104	2550	2553	2556	rBV5	7430	8704	0.22%	0.025%
31	19.128	2723	2727	2731	rBV3	29307	38580	0.98%	0.111%
32	19.192	2735	2738	2743	rBV	25425	32054	0.81%	0.092%
33	19.551	2793	2799	2806	rBV	2818334	3619813	92.01%	10.433%
34	21.304	3092	3097	3106	rBV	1824913	2309175	58.70%	6.655%
35	23.515	3466	3473	3485	rVB2	1933398	3934101	100.00%	11.339%
36	23.668	3492	3499	3511	rVB	1182522	2446962	62.20%	7.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018964.D
Acq On : 20 Dec 2023 17:11
Operator : MA/JU
Sample : PB157887BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK887

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 34696084

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018964.D
Acq On : 20 Dec 2023 17:11
Operator : MA/JU
Sample : PB157887BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK887

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

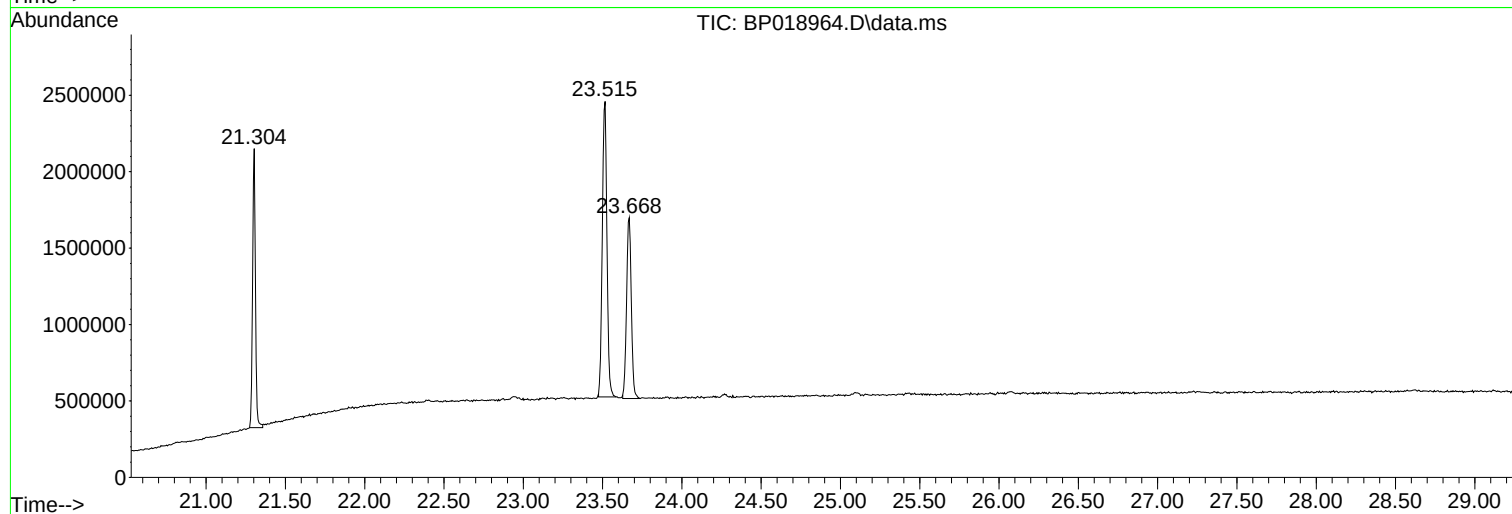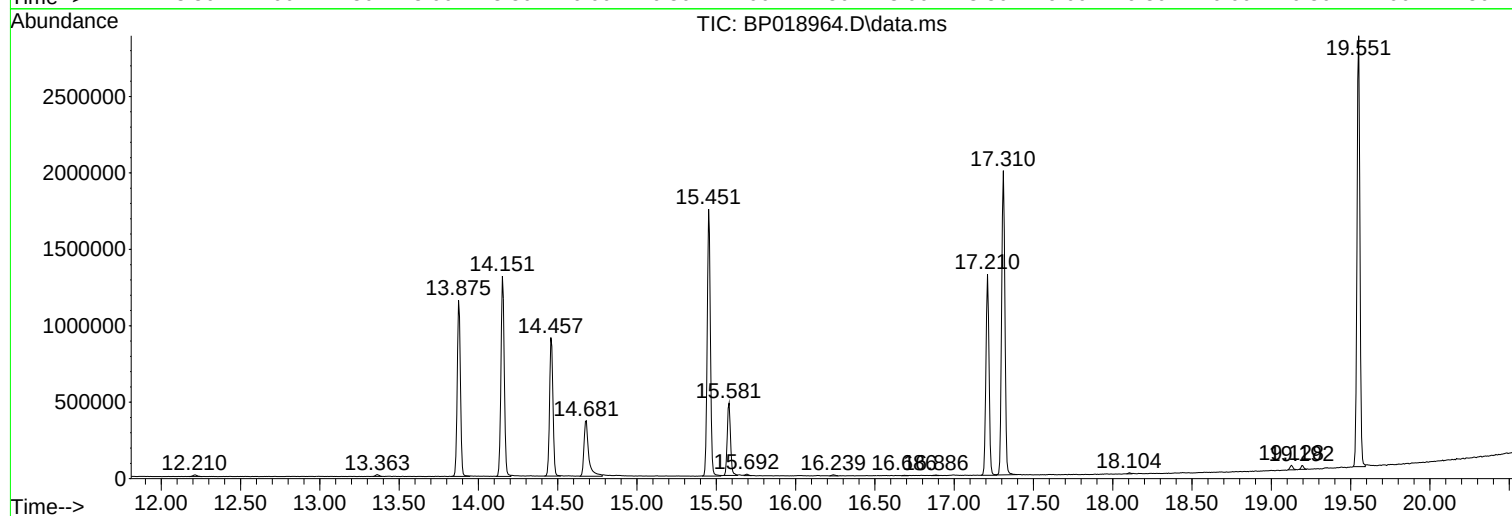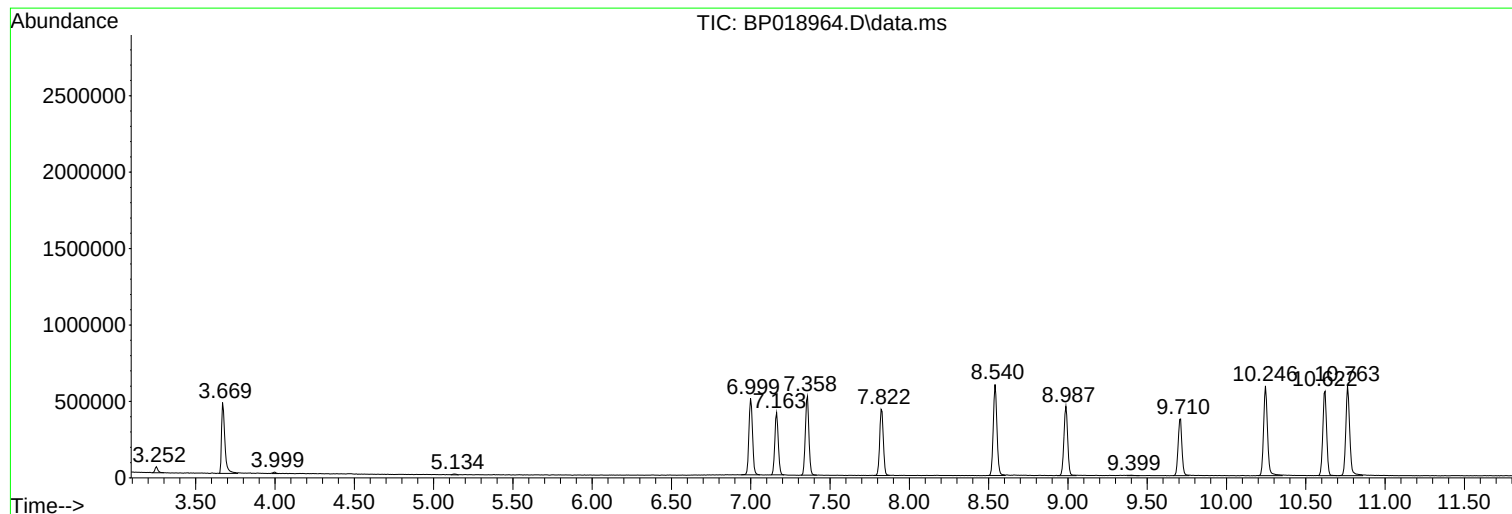

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018964.D
Acq On : 20 Dec 2023 17:11
Operator : MA/JU
Sample : PB157887BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK887

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018964.D
Acq On : 20 Dec 2023 17:11
Operator : MA/JU
Sample : PB157887BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK887

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------