

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
 Data File : BP018984.D
 Acq On : 21 Dec 2023 05:03
 Operator : MA/JU
 Sample : PB157897BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK897

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	33	rVB	43452	50150	1.06%	0.132%
2	3.670	95	99	112	rBV	519595	715436	15.17%	1.883%
3	3.999	151	155	158	rVB2	9602	12630	0.27%	0.033%
4	6.999	653	665	677	rVB	551818	864724	18.34%	2.276%
5	7.164	686	693	702	rVB	432662	674209	14.30%	1.774%
6	7.352	718	725	734	rBV	569563	882554	18.72%	2.323%
7	7.822	796	805	813	rBV	580656	897366	19.03%	2.362%
8	8.540	919	927	941	rBV	643141	1043395	22.13%	2.746%
9	8.987	994	1003	1010	rBV	480349	800796	16.98%	2.107%
10	9.705	1116	1125	1138	rBV	411744	671799	14.25%	1.768%
11	10.240	1209	1216	1236	rBV	618756	1081759	22.94%	2.847%
12	10.616	1270	1280	1292	rVB	712975	1162309	24.65%	3.059%
13	10.763	1296	1305	1323	rBV	585802	1053494	22.34%	2.772%
14	12.210	1546	1551	1559	rVB2	10809	18193	0.39%	0.048%
15	13.357	1742	1746	1752	rBV7	4373	6738	0.14%	0.018%
16	13.875	1827	1834	1843	rBV	1083109	1502427	31.87%	3.954%
17	14.151	1873	1881	1890	rBV	1247829	1824814	38.70%	4.802%
18	14.457	1926	1933	1947	rBV	1051783	1532359	32.50%	4.033%
19	14.675	1963	1970	1986	rBV	373167	765502	16.24%	2.015%
20	15.451	2093	2102	2117	rBV	1619217	2359039	50.03%	6.208%
21	15.575	2117	2123	2136	rVV	492665	698518	14.82%	1.838%
22	15.693	2139	2143	2150	rVB4	8153	14023	0.30%	0.037%
23	16.234	2231	2235	2243	rVB8	5860	9599	0.20%	0.025%
24	16.887	2342	2346	2351	rVB8	3982	6150	0.13%	0.016%
25	16.998	2360	2365	2366	rBV5	3529	5251	0.11%	0.014%
26	17.204	2394	2400	2410	rBV	1358301	2000251	42.42%	5.264%
27	17.304	2411	2417	2433	rVB2	1940364	2728932	57.88%	7.182%
28	19.122	2722	2726	2732	rVB3	27609	37819	0.80%	0.100%
29	19.192	2734	2738	2745	rVV	26092	37156	0.79%	0.098%
30	19.545	2792	2798	2810	rBV	2867168	3682922	78.11%	9.692%
31	21.298	3091	3096	3103	rBV	2363796	2913582	61.80%	7.667%
32	23.510	3464	3472	3486	rVB	2329753	4714903	100.00%	12.408%
33	23.663	3491	3498	3508	rVB	1591773	3230357	68.51%	8.501%




Sum of corrected areas: 37999156

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018984.D
Acq On : 21 Dec 2023 05:03
Operator : MA/JU
Sample : PB157897BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

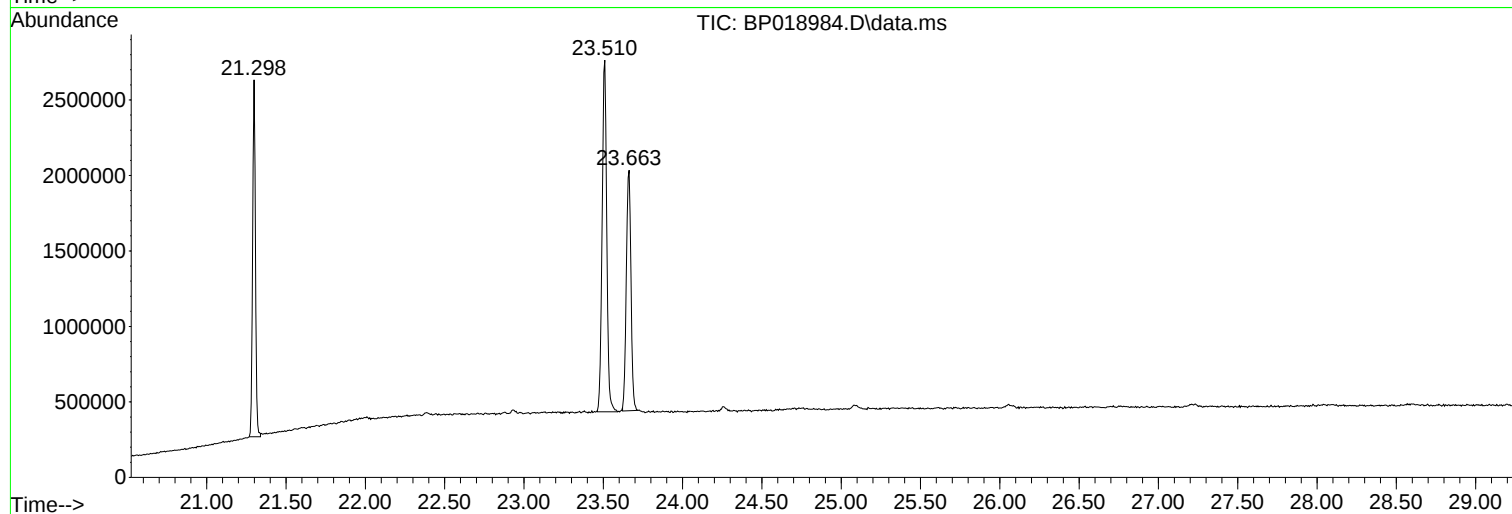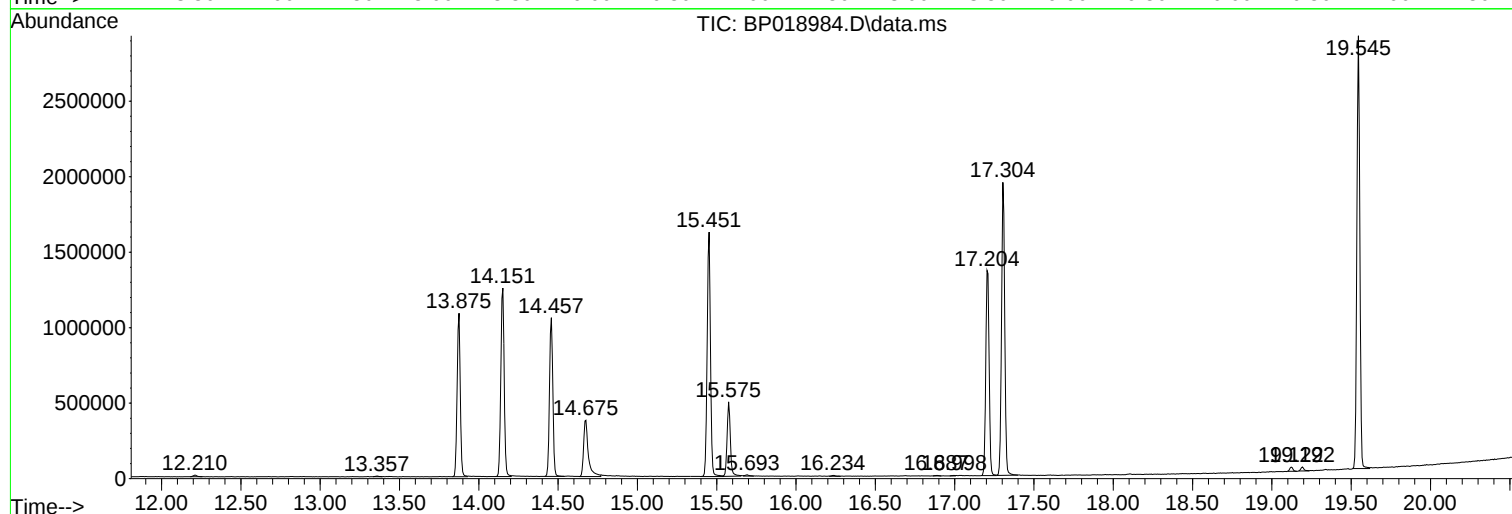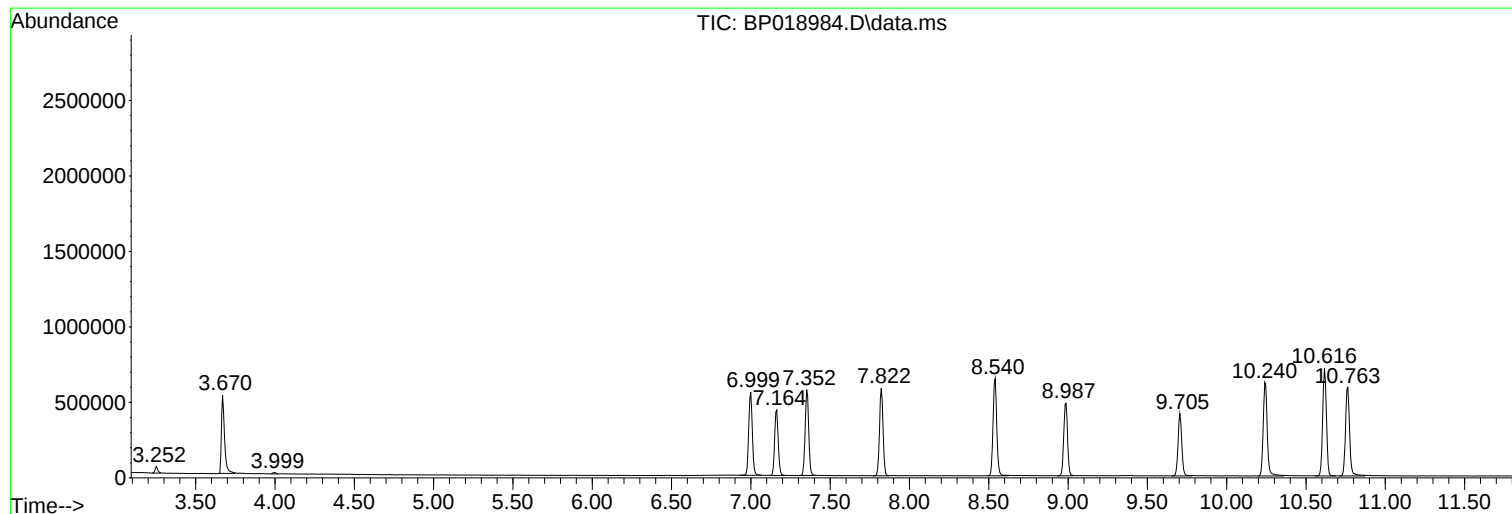

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018984.D
Acq On : 21 Dec 2023 05:03
Operator : MA/JU
Sample : PB157897BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018984.D
Acq On : 21 Dec 2023 05:03
Operator : MA/JU
Sample : PB157897BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK897

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc