

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
 Data File : BP018995.D
 Acq On : 21 Dec 2023 11:15
 Operator : MA/JU
 Sample : PB157780BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK780

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	5	7	10	rVB	25344	24964	1.07%	0.210%
2	3.169	10	14	22	rVB	442948	443302	18.97%	3.725%
3	3.511	68	72	78	rVB3	16224	19357	0.83%	0.163%
4	3.993	150	154	158	rVB2	13431	17420	0.75%	0.146%
5	4.187	185	187	192	rVB5	2894	3912	0.17%	0.033%
6	4.934	310	314	319	rVB6	3290	6852	0.29%	0.058%
7	5.034	327	331	335	rVB7	2186	3417	0.15%	0.029%
8	5.522	412	414	418	rVB5	2215	2650	0.11%	0.022%
9	6.822	630	635	637	rBV6	1629	2919	0.12%	0.025%
10	7.816	796	804	815	rBV	741827	1186498	50.77%	9.969%
11	8.722	953	958	961	rBV7	1246	2554	0.11%	0.021%
12	9.393	1070	1072	1078	rVB7	2465	3597	0.15%	0.030%
13	10.616	1272	1280	1296	rBV	897694	1491080	63.80%	12.528%
14	13.087	1697	1700	1705	rBV5	1565	2817	0.12%	0.024%
15	14.163	1880	1883	1886	rBV4	1943	2549	0.11%	0.021%
16	14.457	1925	1933	1946	rBV	1276793	1895094	81.09%	15.923%
17	14.651	1963	1966	1971	rBV6	1774	3579	0.15%	0.030%
18	15.434	2094	2099	2101	rBV6	2248	3016	0.13%	0.025%
19	15.722	2143	2148	2154	rBV10	2258	5022	0.21%	0.042%
20	16.998	2361	2365	2366	rBV4	4187	4949	0.21%	0.042%
21	17.210	2394	2401	2417	rBV	1387716	2215482	94.80%	18.615%
22	17.710	2482	2486	2490	rBV7	2956	5219	0.22%	0.044%
23	17.757	2492	2494	2497	rVB4	2862	2661	0.11%	0.022%
24	21.298	3091	3096	3105	rBV	1678296	2215724	94.81%	18.617%
25	23.657	3491	3497	3508	rVB	1154192	2337121	100.00%	19.637%




Sum of corrected areas: 11901755

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018995.D
Acq On : 21 Dec 2023 11:15
Operator : MA/JU
Sample : PB157780BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

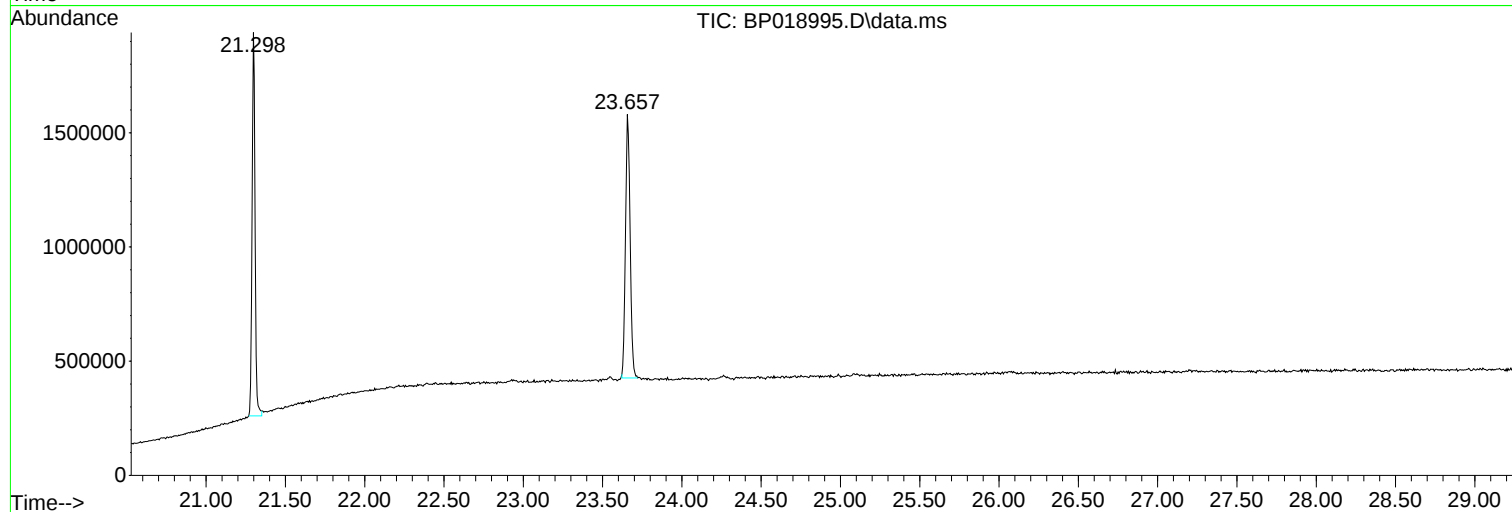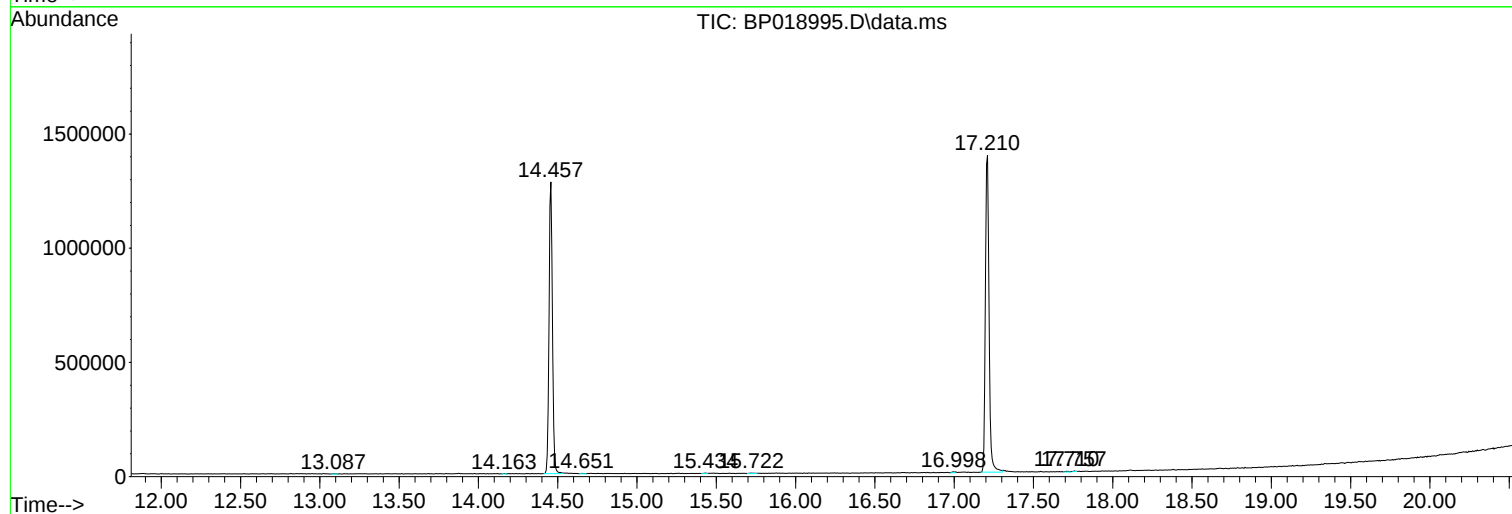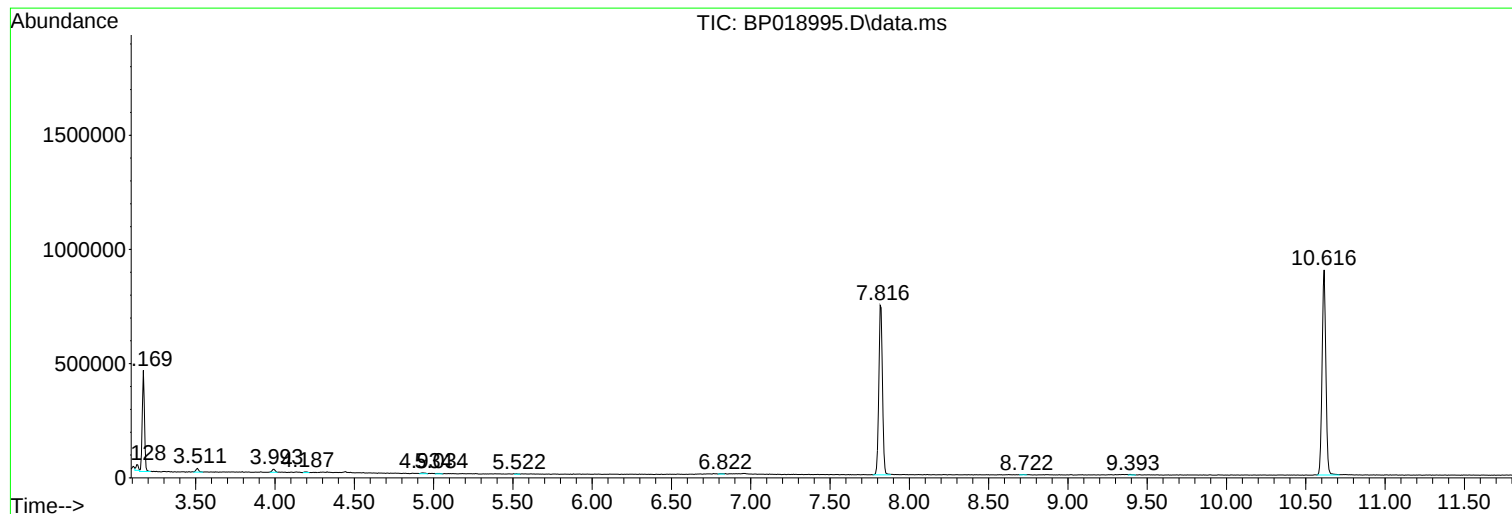

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018995.D
Acq On : 21 Dec 2023 11:15
Operator : MA/JU
Sample : PB157780BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.169	7.47 ng/ul	443302	1,4-Dichlorobenzene-d4	7.822

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	91
2	Heptane			100	C7H16	000142-82-5	91
3	Heptane			100	C7H16	000142-82-5	90
4	Heptane			100	C7H16	000142-82-5	86
5	Octane, 3,3-dimethyl-			142	C10H22	004110-44-5	47

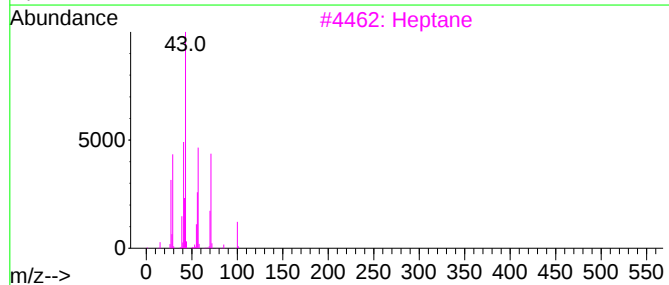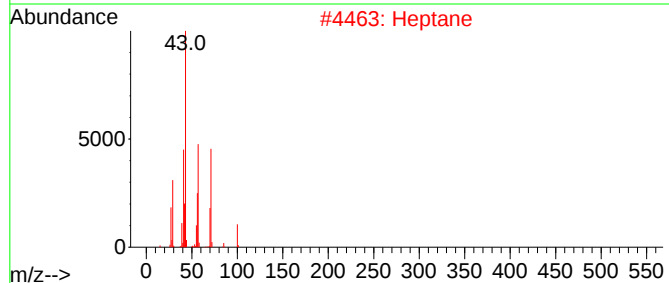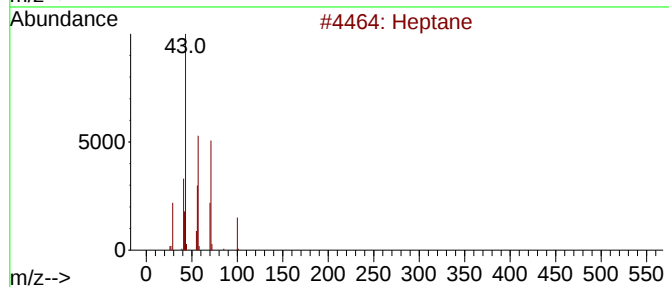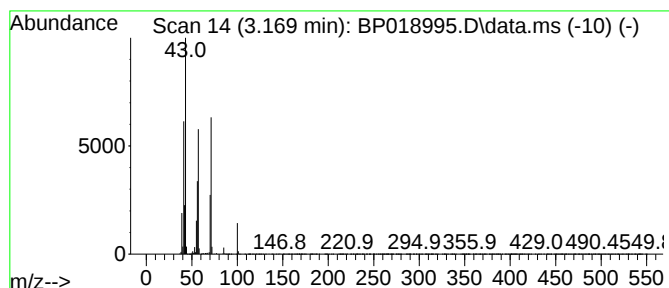

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018995.D
Acq On : 21 Dec 2023 11:15
Operator : MA/JU
Sample : PB157780BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.169	7.5	ng/u1	443302	1	7.822	1186500	20.0