

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
 Data File : BP018998.D
 Acq On : 21 Dec 2023 12:57
 Operator : MA/JU
 Sample : PB157782BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK782

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	5	7	10	rVB	24637	22557	0.98%	0.216%
2	3.169	10	14	18	rVB	367847	371608	16.20%	3.566%
3	3.505	69	71	75	rVB2	12135	14085	0.61%	0.135%
4	3.993	150	154	159	rBV	11329	15428	0.67%	0.148%
5	4.340	209	213	215	rBV5	2736	3460	0.15%	0.033%
6	6.952	655	657	661	rBV5	2058	2734	0.12%	0.026%
7	7.816	797	804	813	rBV	623494	984962	42.95%	9.453%
8	10.381	1237	1240	1244	rBV5	1844	2434	0.11%	0.023%
9	10.616	1272	1280	1294	rBV	724497	1248598	54.44%	11.983%
10	13.016	1685	1688	1696	rVB10	1879	3066	0.13%	0.029%
11	13.869	1829	1833	1836	rBV6	1539	2602	0.11%	0.025%
12	14.322	1907	1910	1914	rBV6	1683	2317	0.10%	0.022%
13	14.369	1914	1918	1920	rBV4	1815	2331	0.10%	0.022%
14	14.457	1926	1933	1943	rBV	988561	1567807	68.36%	15.047%
15	15.251	2062	2068	2070	rVB6	1711	3370	0.15%	0.032%
16	15.681	2136	2141	2145	rVB8	1880	2918	0.13%	0.028%
17	17.210	2394	2401	2418	rBV	1145979	1819130	79.32%	17.459%
18	21.298	3091	3096	3104	rBV	1609470	2056867	89.69%	19.740%
19	23.662	3491	3498	3510	rVB	1099088	2293430	100.00%	22.011%




Sum of corrected areas: 10419704

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018998.D
Acq On : 21 Dec 2023 12:57
Operator : MA/JU
Sample : PB157782BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK782

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

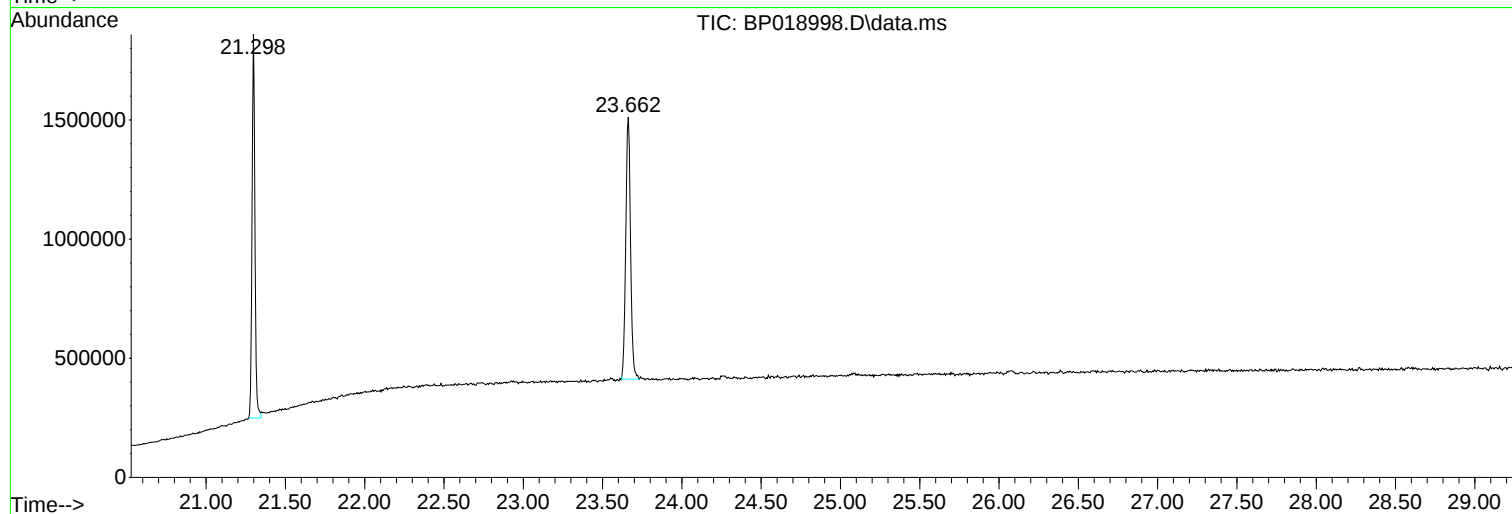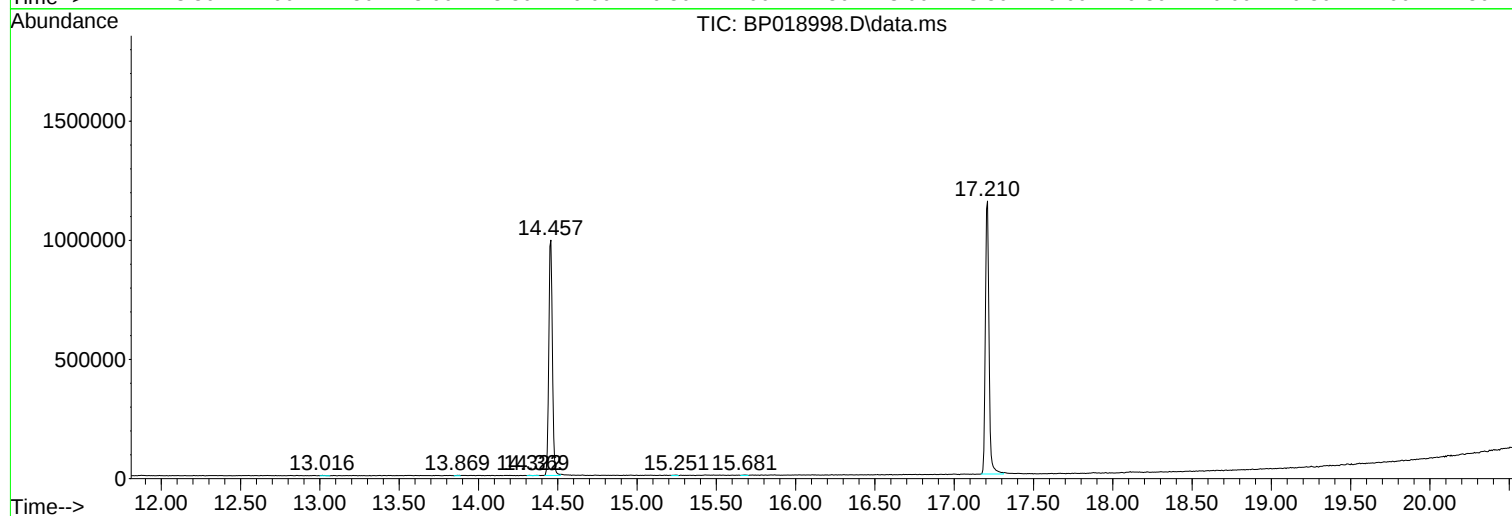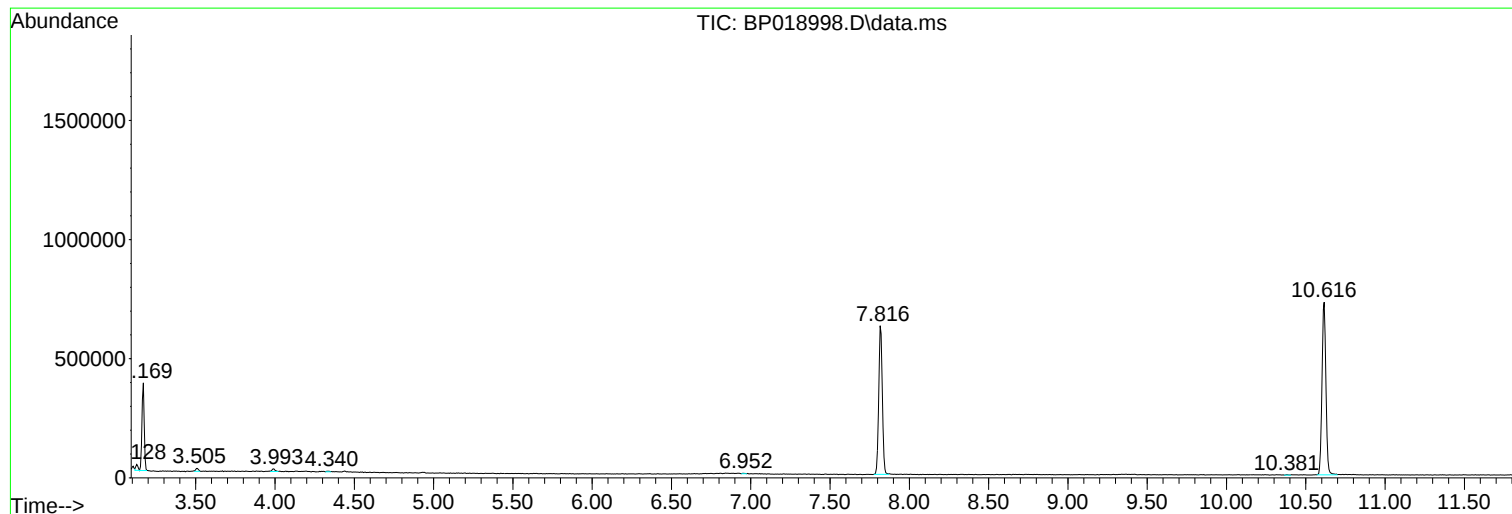

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018998.D
Acq On : 21 Dec 2023 12:57
Operator : MA/JU
Sample : PB157782BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK782










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.169	7.55 ng/ul	371608	1,4-Dichlorobenzene-d4	7.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	91
2			Heptane	100	C7H16	000142-82-5	90
3			Heptane	100	C7H16	000142-82-5	90
4			Heptane	100	C7H16	000142-82-5	87
5			Oxalic acid, isobutyl pentyl ester	216	C11H20O4	1000309-37-0	53

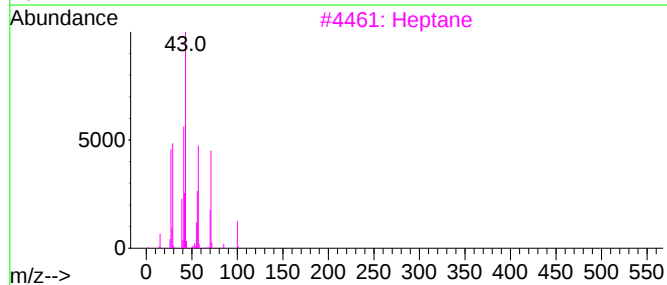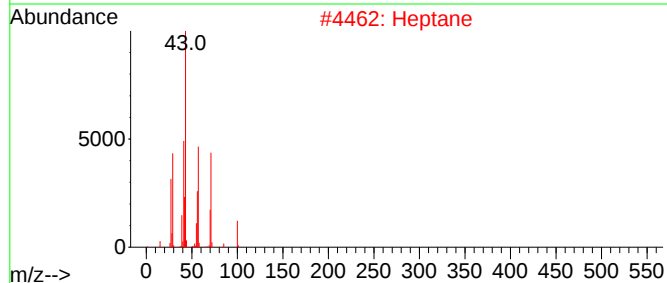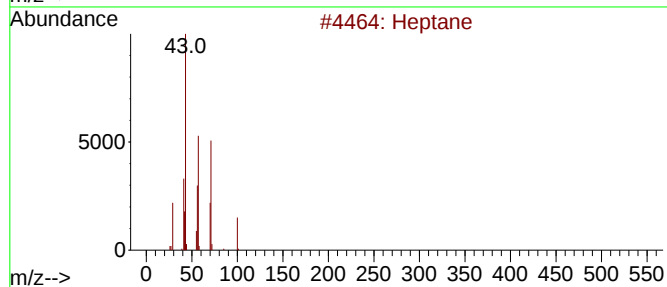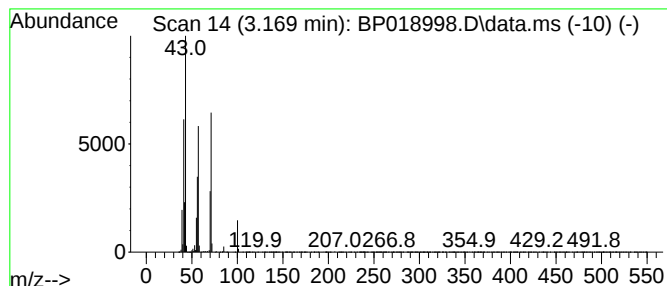

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122023\
Data File : BP018998.D
Acq On : 21 Dec 2023 12:57
Operator : MA/JU
Sample : PB157782BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK782

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.169	7.5	ng/u1	371608	1	7.816	984962	20.0