
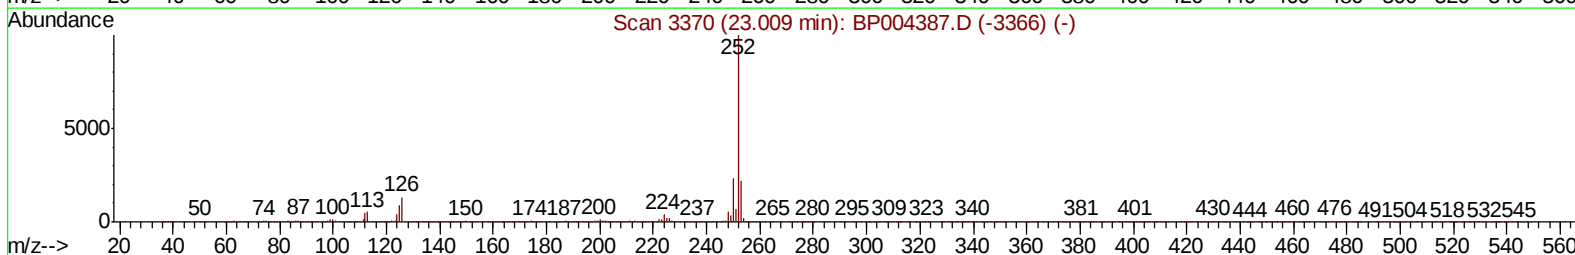
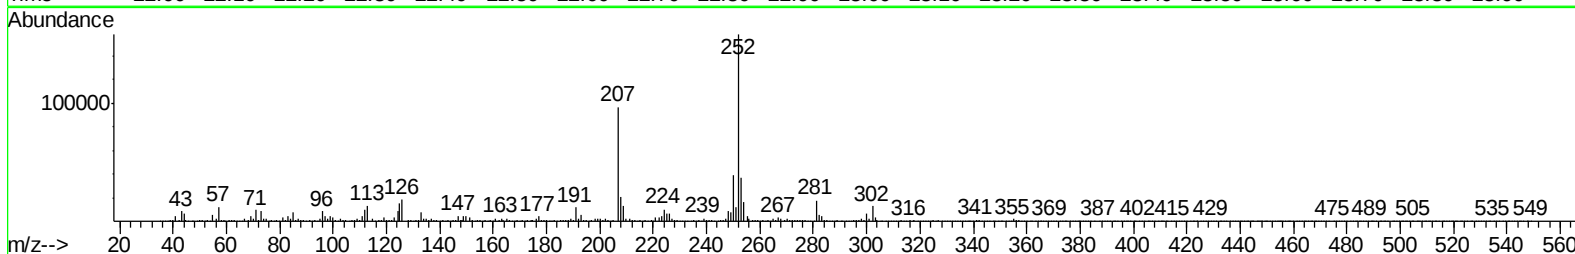


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122120\
Data File : BP004408.D
Acq On : 21 Dec 2020 15:03
Operator : CG/JU
Sample : L5114-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Dec 21 15:58:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 18 17:12:07 2020
Response via : Initial Calibration

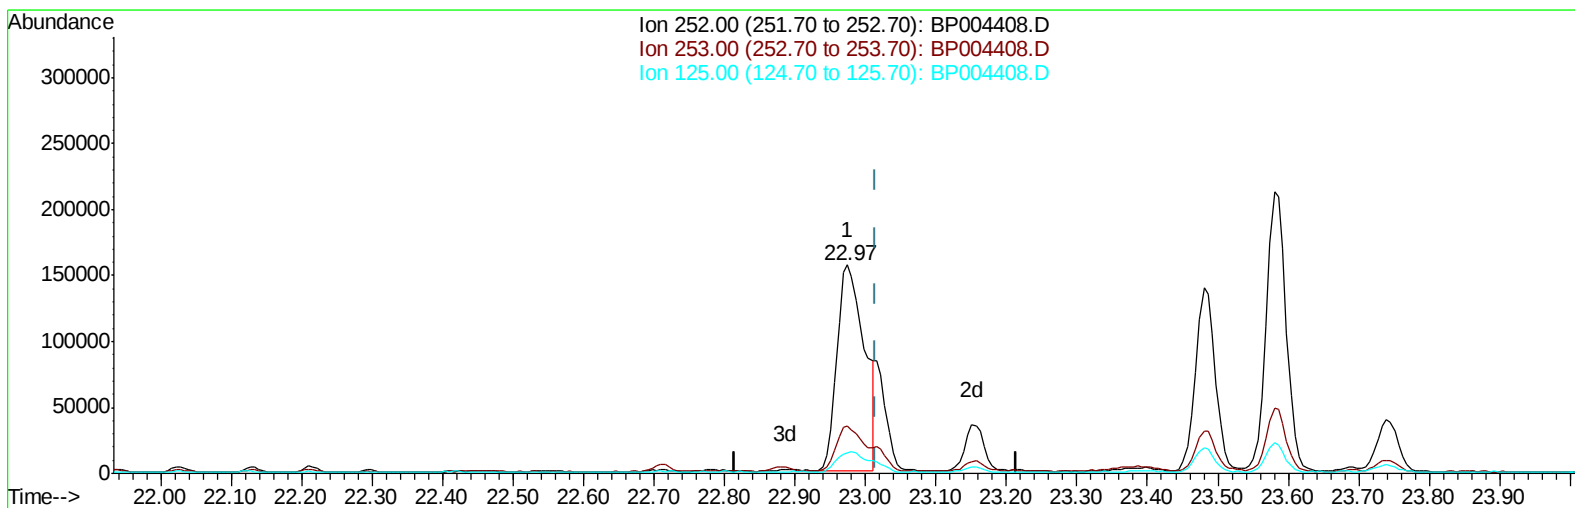

TIC: BP004408.D

(89) Benzo(k)fluoranthene




22.974min (-0.041) 3.63ng/ul

response 416172

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	23.03
125.00	9.00	9.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122120\
 Data File : BG047779.D
 Acq On : 21 Dec 2020 14:59
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 21 16:55:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 21 16:48:34 2020
 Response via : Initial Calibration

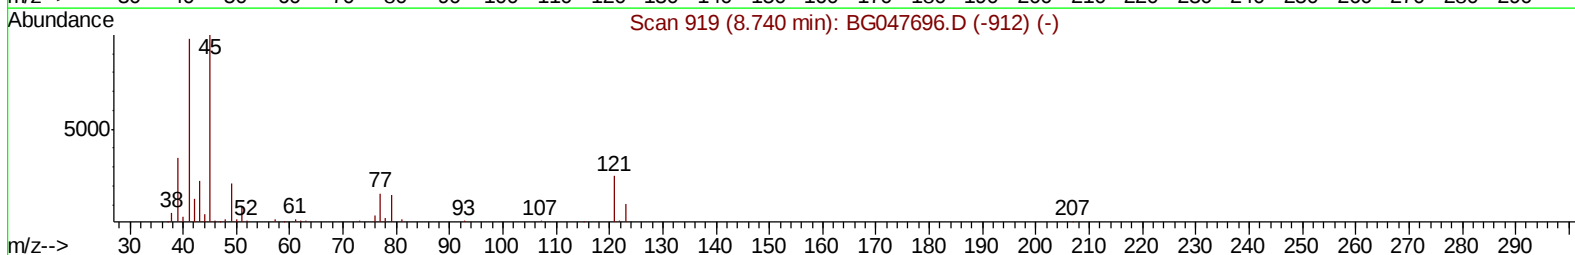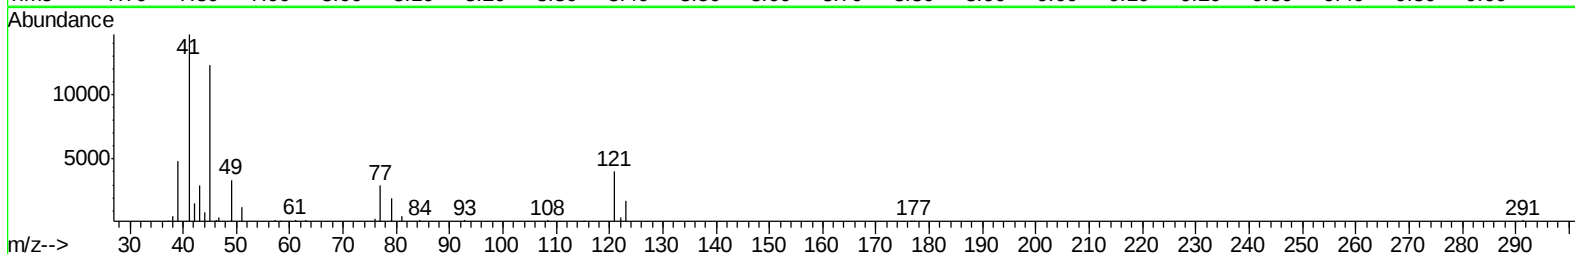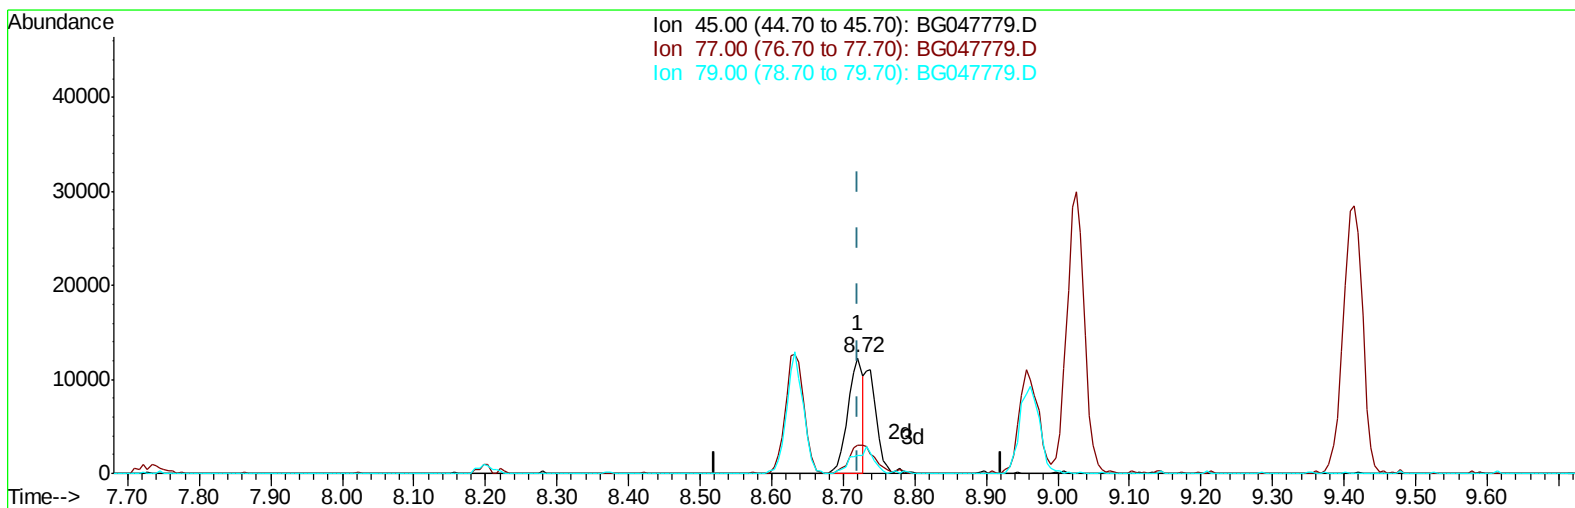

TIC: BG047779.D

(12) 2,2'-oxybis(1-Chloropropane)

8.720min (0.000) 11.54ng/ul

response 17742

Ion	Exp%	Act%
45.00	100	100
77.00	24.00	23.99
79.00	15.50	15.53
0.00	0.00	0.00