

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122120\
 Data File : BP004414.D
 Acq On : 21 Dec 2020 18:27
 Operator : CG/JU
 Sample : L5154-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC2

Quant Time: Dec 22 00:33:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 22 00:25:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	281462	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	1048040	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	547020	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	1062733	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	1155643	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	1365320	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	8478	1.25	ng/uL	0.00
5) Phenol-d5	6.99	99	147924	6.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	360412	26.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	434309	21.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	255301	13.12	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	256798	28.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	277724	28.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	456814	24.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	42350	2.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.87	166	1257669	28.72	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	1706439	31.38	ng/ul	0.00
52) 4-Nitrophenol-d4	14.67	143	35691	4.51	ng/ul	0.00
58) Fluorene-d10	15.47	176	1136807	29.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.60	200	169258	24.69	ng/ul	0.00
71) Anthracene-d10	17.33	188	1858543	35.40	ng/ul	0.00
79) Pyrene-d10	19.57	212	2126456	34.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	2686516	35.72	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.92	163	71642	1.633	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
Data File : BP004414.D
Acq On : 21 Dec 2020 18:27
Operator : CG/JU
Sample : L5154-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC2

Quant Time: Dec 22 00:33:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 22 00:25:51 2020
Response via : Initial Calibration

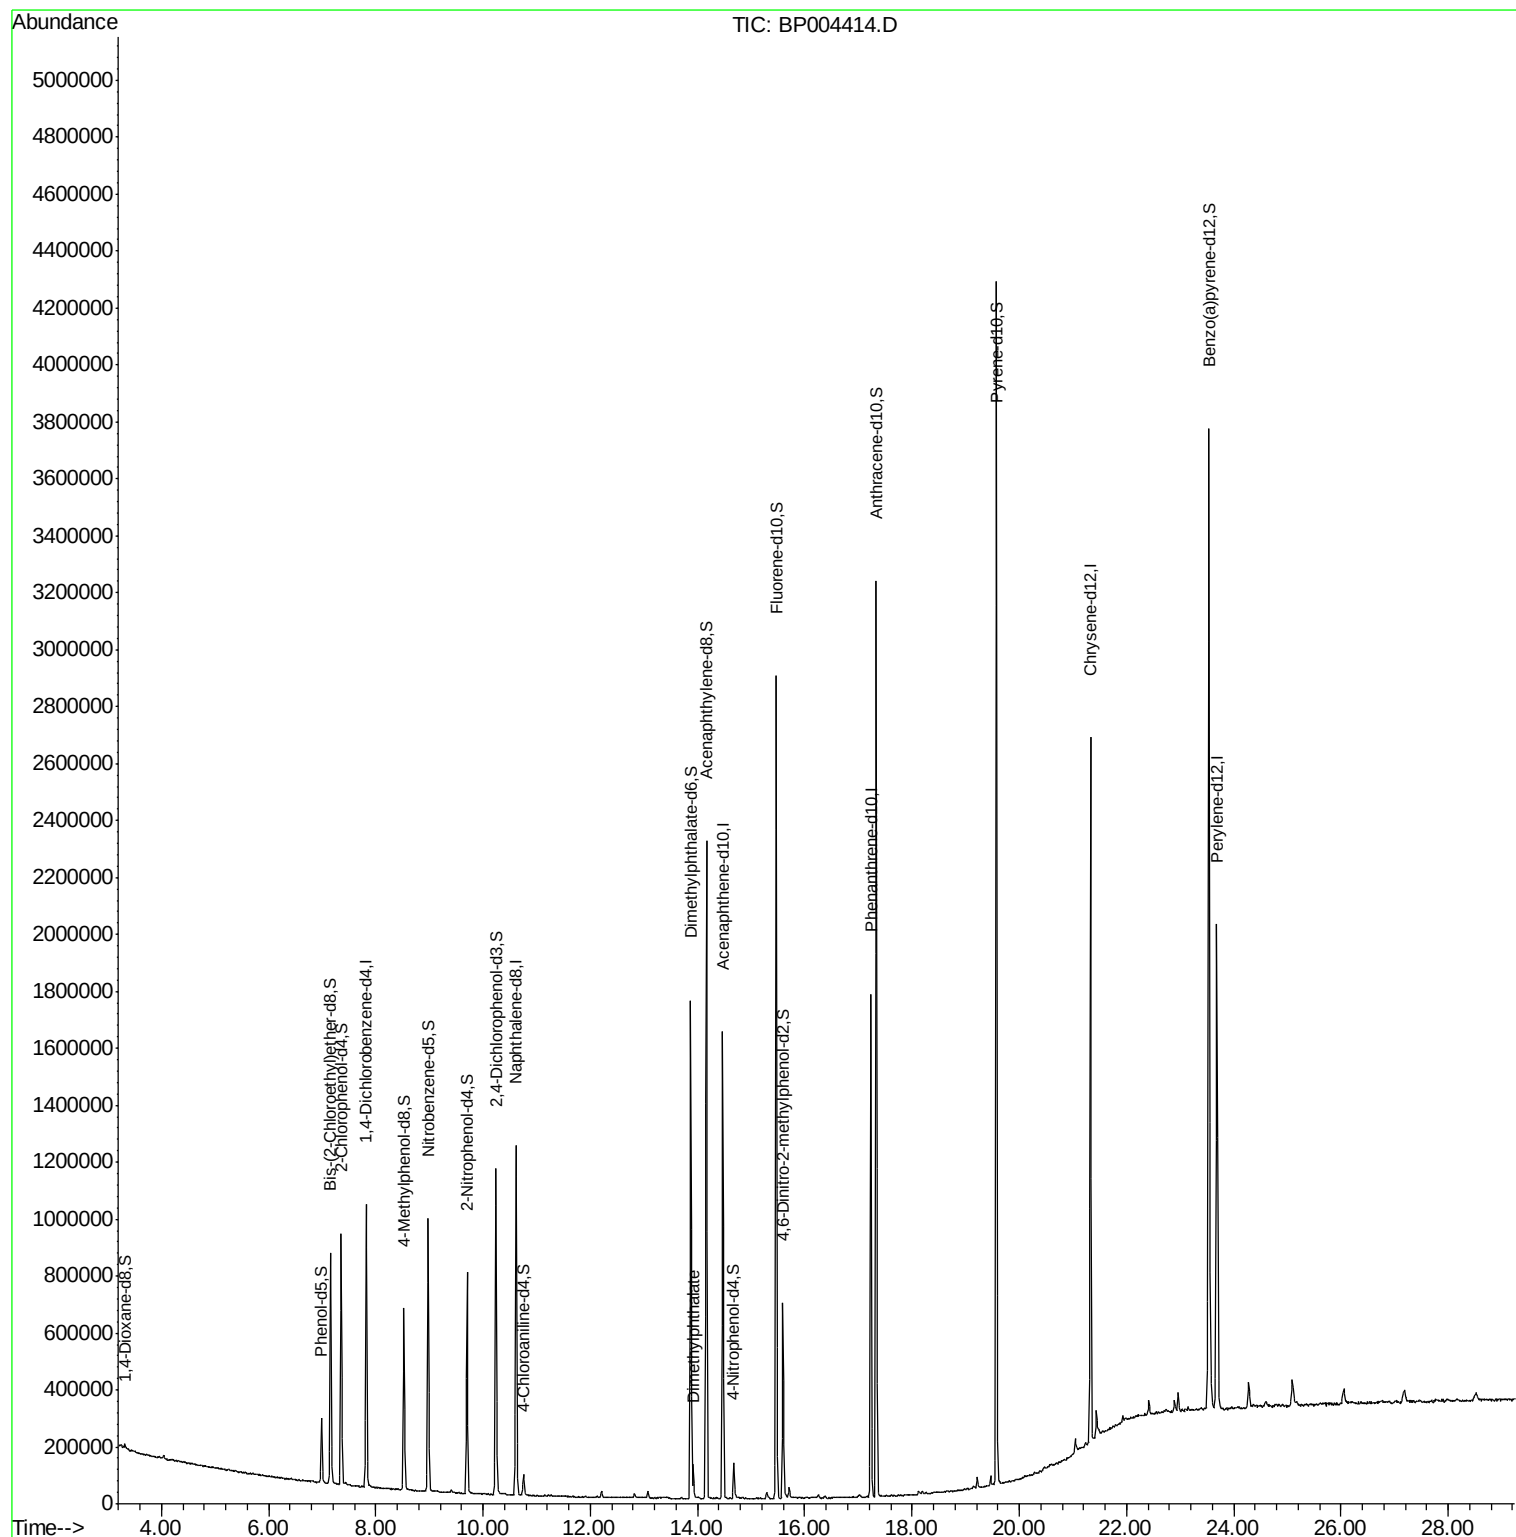

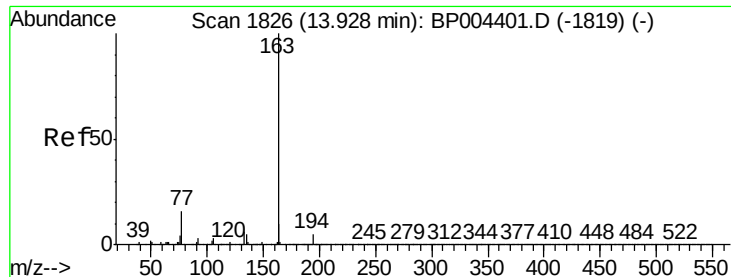

#45

Dimethylphthalate

Concen: 1.633 ng/ul

RT: 13.92 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BP004414.D

Acq: 21 Dec 2020 18:27

Instrument :

BNA_P

ClientSampleId :

C0AC2


Tot Ion:163 Resp: 71642

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 10.7 7.8 11.8

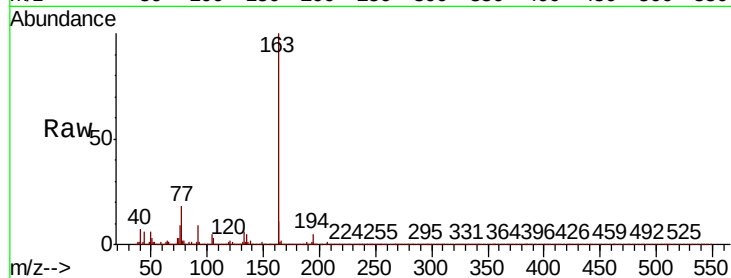

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

