

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122120\
 Data File : BP004415.D
 Acq On : 21 Dec 2020 19:01
 Operator : CG/JU
 Sample : L5154-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC3

Quant Time: Dec 22 00:36:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 22 00:25:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	264754	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	990410	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	524370	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	1042930	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	1168466	20.00	ng/ul	0.00
86) Perylene-d12	23.69	264	1349519	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	8767	1.38	ng/uL	0.00
5) Phenol-d5	6.99	99	148631	6.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	373173	28.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	443636	23.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	258238	14.11	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	261295	30.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	285068	30.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	466698	26.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	41501	2.11	ng/ul	0.00
44) Dimethylphthalate-d6	13.87	166	1316429	31.37	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	1771678	33.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.67	143	36793	4.85	ng/ul	0.00
58) Fluorene-d10	15.47	176	1183946	32.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.59	200	177017	26.31	ng/ul	0.00
71) Anthracene-d10	17.33	188	1922964	37.32	ng/ul	0.00
79) Pyrene-d10	19.57	212	2236131	35.82	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.54	264	2795351	37.61	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.92	163	76980	1.831	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
Data File : BP004415.D
Acq On : 21 Dec 2020 19:01
Operator : CG/JU
Sample : L5154-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC3

Quant Time: Dec 22 00:36:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 22 00:25:51 2020
Response via : Initial Calibration

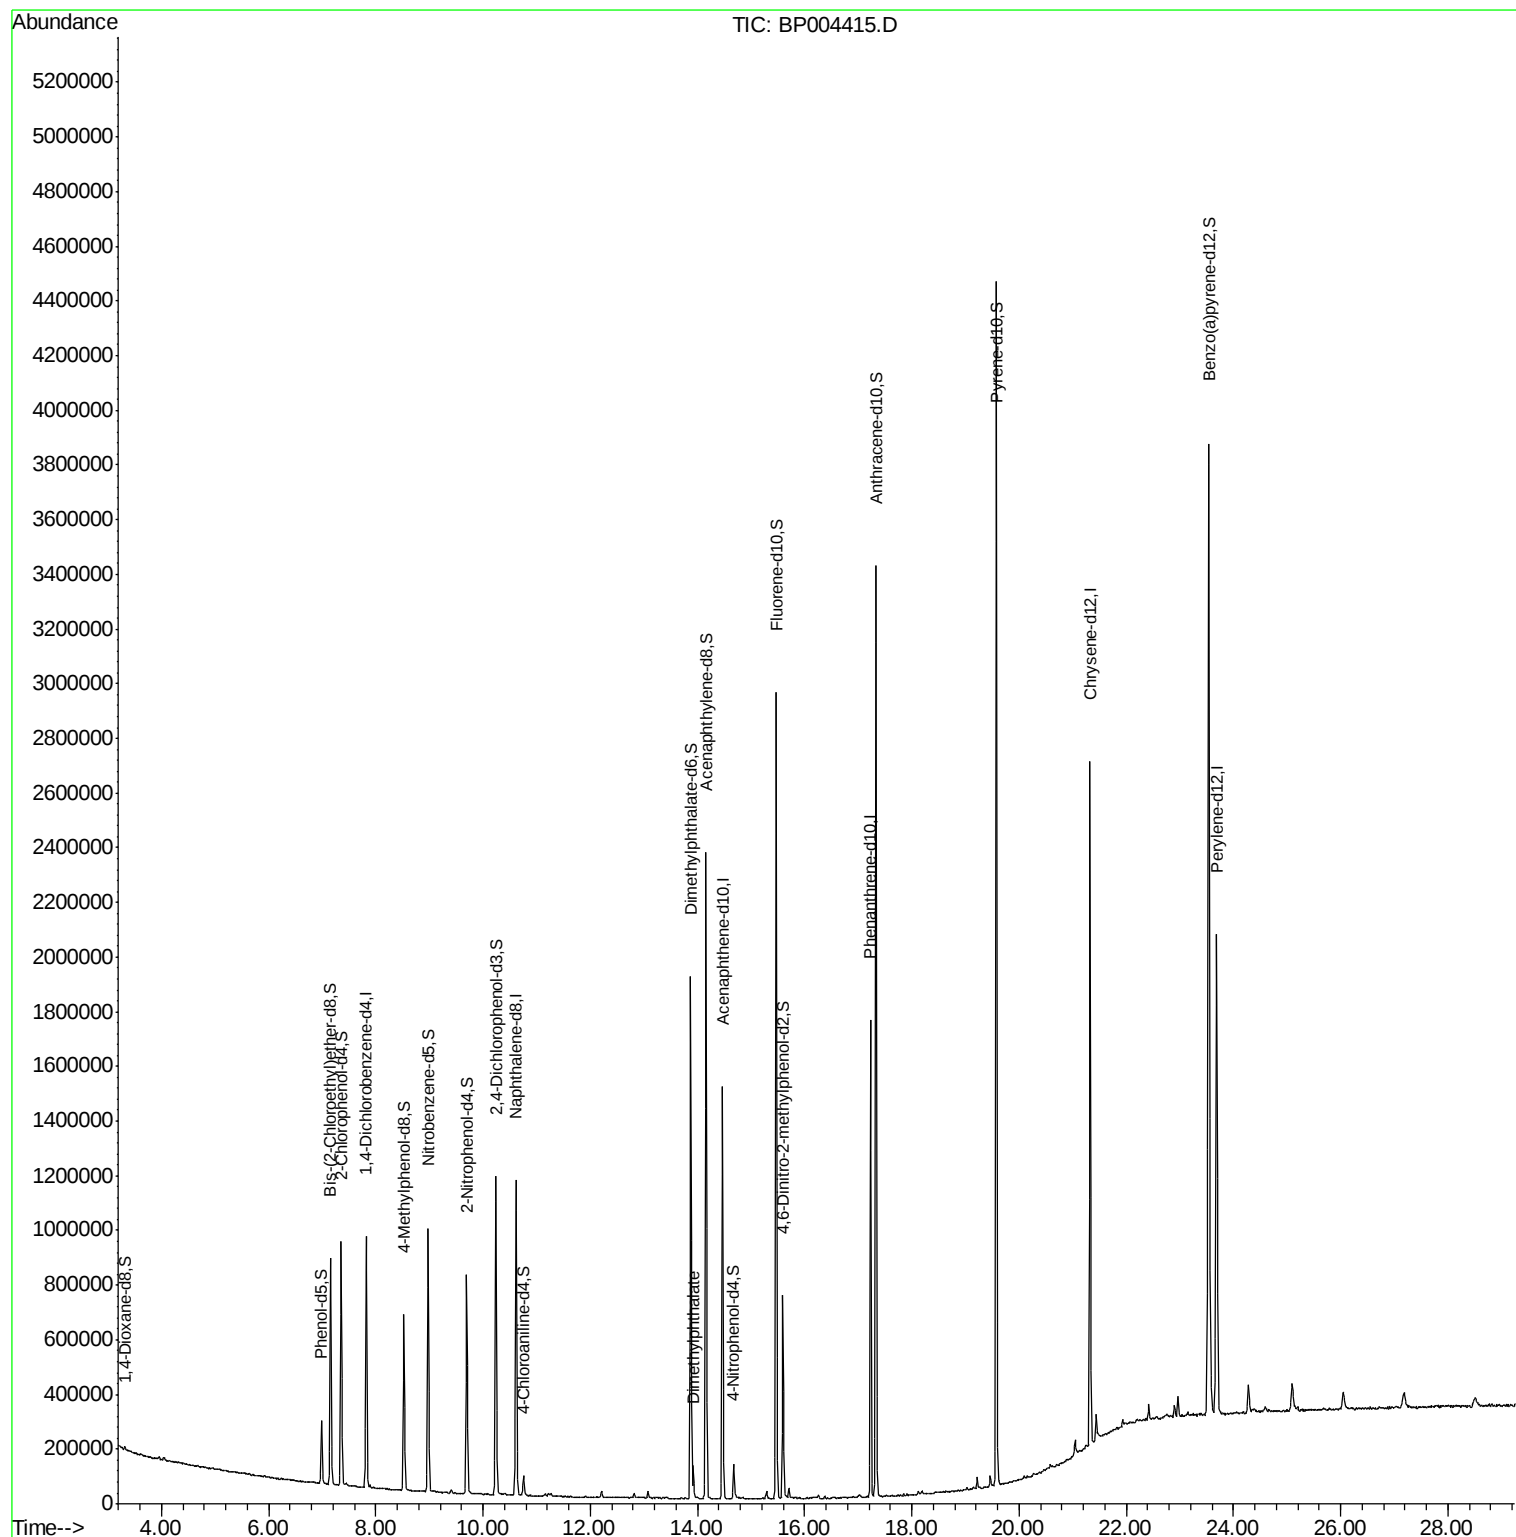

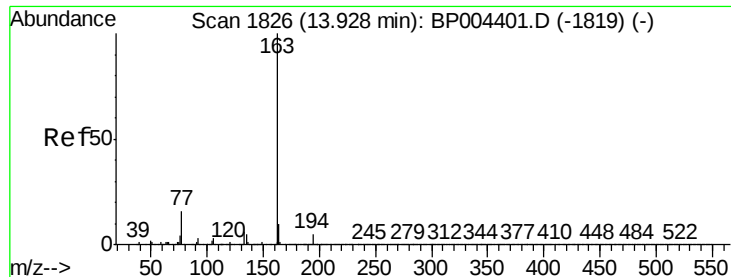

#45

Dimethylphthalate

Concen: 1.831 ng/ul

RT: 13.92 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BP004415.D

Acq: 21 Dec 2020 19:01

Instrument :

BNA_P

ClientSampleId :

C0AC3


Tot Ion:163 Resp: 76980

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 8.8 7.8 11.8

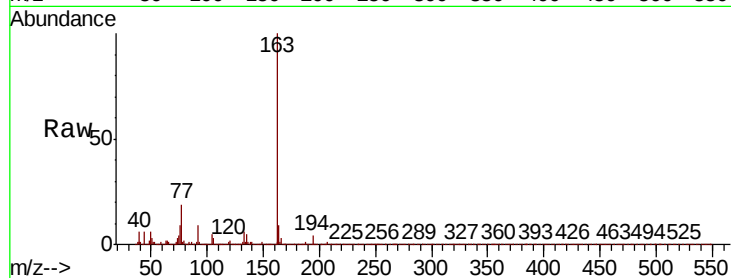

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

