

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
 Data File : BP004405.D
 Acq On : 21 Dec 2020 12:32
 Operator : CG/JU
 Sample : L5128-02DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8C0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	37	rVB	197938	278648	6.50%	1.193%
2	4.481	216	220	225	rVB	49867	74731	1.74%	0.320%
3	6.993	644	647	656	rVB2	25743	57459	1.34%	0.246%
4	7.158	670	675	684	rVB	69094	117609	2.74%	0.504%
5	7.358	703	709	717	rVB	88870	147934	3.45%	0.633%
6	7.822	781	788	796	rVB	1066573	1675171	39.07%	7.173%
7	8.528	903	908	916	rVB	65853	110366	2.57%	0.473%
8	8.805	949	955	963	rBV	95911	160802	3.75%	0.689%
9	8.922	971	975	979	rBV3	10488	15241	0.36%	0.065%
10	8.981	979	985	993	rVB	77031	137359	3.20%	0.588%
11	9.181	1017	1019	1026	rVB6	8905	13570	0.32%	0.058%
12	9.334	1041	1045	1051	rVB7	10535	17368	0.41%	0.074%
13	9.416	1053	1059	1072	rVB7	23483	54740	1.28%	0.234%
14	9.516	1072	1076	1080	rBV6	5248	8418	0.20%	0.036%
15	9.622	1091	1094	1101	rVB6	4845	8941	0.21%	0.038%
16	9.705	1101	1108	1114	rVV	64151	115275	2.69%	0.494%
17	9.752	1114	1116	1121	rVB4	6580	7620	0.18%	0.033%
18	9.828	1121	1129	1134	rBV9	11958	24409	0.57%	0.105%
19	9.881	1134	1138	1143	rVV4	19310	35298	0.82%	0.151%
20	9.922	1143	1145	1150	rVB6	3296	5368	0.13%	0.023%
21	10.040	1158	1165	1171	rVB8	7609	18208	0.42%	0.078%
22	10.163	1180	1186	1193	rVB3	33779	66423	1.55%	0.284%
23	10.240	1193	1199	1207	rBV	106227	196840	4.59%	0.843%
24	10.399	1220	1226	1229	rBV8	5502	11571	0.27%	0.050%
25	10.552	1246	1252	1256	rBV5	6231	11794	0.28%	0.051%
26	10.616	1256	1263	1271	rBV	1290556	2211742	51.58%	9.471%
27	10.752	1276	1286	1300	rVB2	94372	216618	5.05%	0.928%
28	10.869	1300	1306	1314	rBV9	8272	21408	0.50%	0.092%
29	10.969	1320	1323	1327	rVB6	4226	6414	0.15%	0.027%
30	11.040	1331	1335	1340	rVB7	4417	5811	0.14%	0.025%
31	11.275	1372	1375	1381	rVB5	5453	7784	0.18%	0.033%
32	11.463	1402	1407	1412	rVB4	9491	19049	0.44%	0.082%
33	11.587	1423	1428	1433	rVB7	8305	15561	0.36%	0.067%
34	11.652	1435	1439	1444	rVV6	5178	10345	0.24%	0.044%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
 Data File : BP004405.D
 Acq On : 21 Dec 2020 12:32
 Operator : CG/JU
 Sample : L5128-02DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8C0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	11.693	1444	1446	1450	rVB5	4564	4979	0.12%	0.021%
36	11.775	1457	1460	1465	rVV7	4416	7099	0.17%	0.030%
37	11.828	1465	1469	1474	rVB3	9149	13761	0.32%	0.059%
38	11.969	1489	1493	1500	rVB5	7913	15672	0.37%	0.067%
39	12.069	1504	1510	1512	rBV6	6431	8992	0.21%	0.039%
40	12.146	1518	1523	1527	rBV	16115	28917	0.67%	0.124%
41	12.187	1529	1530	1537	rVB7	5255	7769	0.18%	0.033%
42	12.340	1551	1556	1568	rVB7	7500	19308	0.45%	0.083%
43	12.622	1598	1604	1608	rVB5	8313	13047	0.30%	0.056%
44	12.722	1616	1621	1624	rBV7	5438	7534	0.18%	0.032%
45	13.010	1667	1670	1673	rBV5	3939	4532	0.11%	0.019%
46	13.069	1678	1680	1686	rVB7	3341	4591	0.11%	0.020%
47	13.187	1695	1700	1704	rVB7	6443	10896	0.25%	0.047%
48	13.299	1716	1719	1724	rVB5	4817	7095	0.17%	0.030%
49	13.422	1736	1740	1743	rBV6	2955	5015	0.12%	0.021%
50	13.504	1746	1754	1762	rBV6	12660	32157	0.75%	0.138%
51	13.569	1762	1765	1773	rVV10	6751	12678	0.30%	0.054%
52	13.698	1782	1787	1792	rBV9	4951	8958	0.21%	0.038%
53	13.787	1798	1802	1806	rBV7	4198	7496	0.17%	0.032%
54	13.828	1806	1809	1811	rVV4	4702	5982	0.14%	0.026%
55	13.875	1811	1817	1822	rVV	186673	262251	6.12%	1.123%
56	13.922	1822	1825	1831	rVB	36055	49580	1.16%	0.212%
57	14.022	1835	1842	1847	rBV	5028	12868	0.30%	0.055%
58	14.163	1856	1866	1873	rBV	198646	318028	7.42%	1.362%
59	14.216	1873	1875	1882	rVB8	3562	4503	0.11%	0.019%
60	14.281	1882	1886	1891	rBV8	6017	11986	0.28%	0.051%
61	14.393	1897	1905	1910	rBV5	33907	53381	1.25%	0.229%
62	14.469	1910	1918	1927	rVV	1772895	2725171	63.56%	11.669%
63	14.551	1930	1932	1937	rVB6	4094	5615	0.13%	0.024%
64	14.687	1950	1955	1959	rBV6	8812	15470	0.36%	0.066%
65	14.828	1975	1979	1983	rBV7	4616	7297	0.17%	0.031%
66	15.069	2016	2020	2024	rBV7	5606	9671	0.23%	0.041%
67	15.210	2041	2044	2047	rBV2	8355	12226	0.29%	0.052%
68	15.275	2053	2055	2061	rVB7	6327	10355	0.24%	0.044%
69	15.334	2061	2065	2068	rBV6	4659	6661	0.16%	0.029%
70	15.469	2079	2088	2099	rBV	251608	375085	8.75%	1.606%
71	15.598	2103	2110	2114	rBV4	18662	34324	0.80%	0.147%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
 Data File : BP004405.D
 Acq On : 21 Dec 2020 12:32
 Operator : CG/JU
 Sample : L5128-02DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8C0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

72	15.728	2125	2132	2137	rBV4	9068	17756	0.41%	0.076%
73	15.928	2162	2166	2170	rBV6	6717	9213	0.21%	0.039%
74	15.981	2170	2175	2180	rBV2	33486	48618	1.13%	0.208%
75	16.134	2196	2201	2203	rBV5	7530	9677	0.23%	0.041%
76	16.198	2210	2212	2220	rVB9	4262	5438	0.13%	0.023%
77	16.363	2236	2240	2245	rBV6	9094	15369	0.36%	0.066%
78	16.498	2256	2263	2265	rBV4	9094	17060	0.40%	0.073%
79	16.763	2301	2308	2316	rBV2	11061	21942	0.51%	0.094%
80	17.016	2343	2351	2355	rBV2	13766	29161	0.68%	0.125%
81	17.163	2372	2376	2378	rBV5	4262	5232	0.12%	0.022%
82	17.234	2380	2388	2399	rVV	2168068	3092805	72.13%	13.243%
83	17.334	2399	2405	2414	rVB	264585	403223	9.40%	1.727%
84	17.845	2487	2492	2497	rBV7	9788	19270	0.45%	0.083%
85	18.128	2536	2540	2544	rBV6	12712	22878	0.53%	0.098%
86	18.192	2547	2551	2557	rVV3	23658	38766	0.90%	0.166%
87	18.875	2663	2667	2671	rBV3	37430	46195	1.08%	0.198%
88	19.145	2709	2713	2716	rBV2	27892	38841	0.91%	0.166%
89	19.575	2781	2786	2790	rBV	374039	494187	11.53%	2.116%
90	19.616	2791	2793	2799	rVB	26864	35495	0.83%	0.152%
91	20.280	2903	2906	2912	rVB3	35740	43927	1.02%	0.188%
92	21.327	3079	3084	3091	rBV	2986677	3839167	89.54%	16.439%
93	21.439	3100	3103	3107	rBV	124280	164468	3.84%	0.704%
94	22.557	3290	3293	3299	rVB	191453	260763	6.08%	1.117%
95	23.533	3455	3459	3463	rBV	217722	359838	8.39%	1.541%
96	23.686	3478	3485	3499	rVB	2166937	4287606	100.00%	18.359%


Sum of corrected areas: 23353740

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
Data File : BP004405.D
Acq On : 21 Dec 2020 12:32
Operator : CG/JU
Sample : L5128-02DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8C0DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

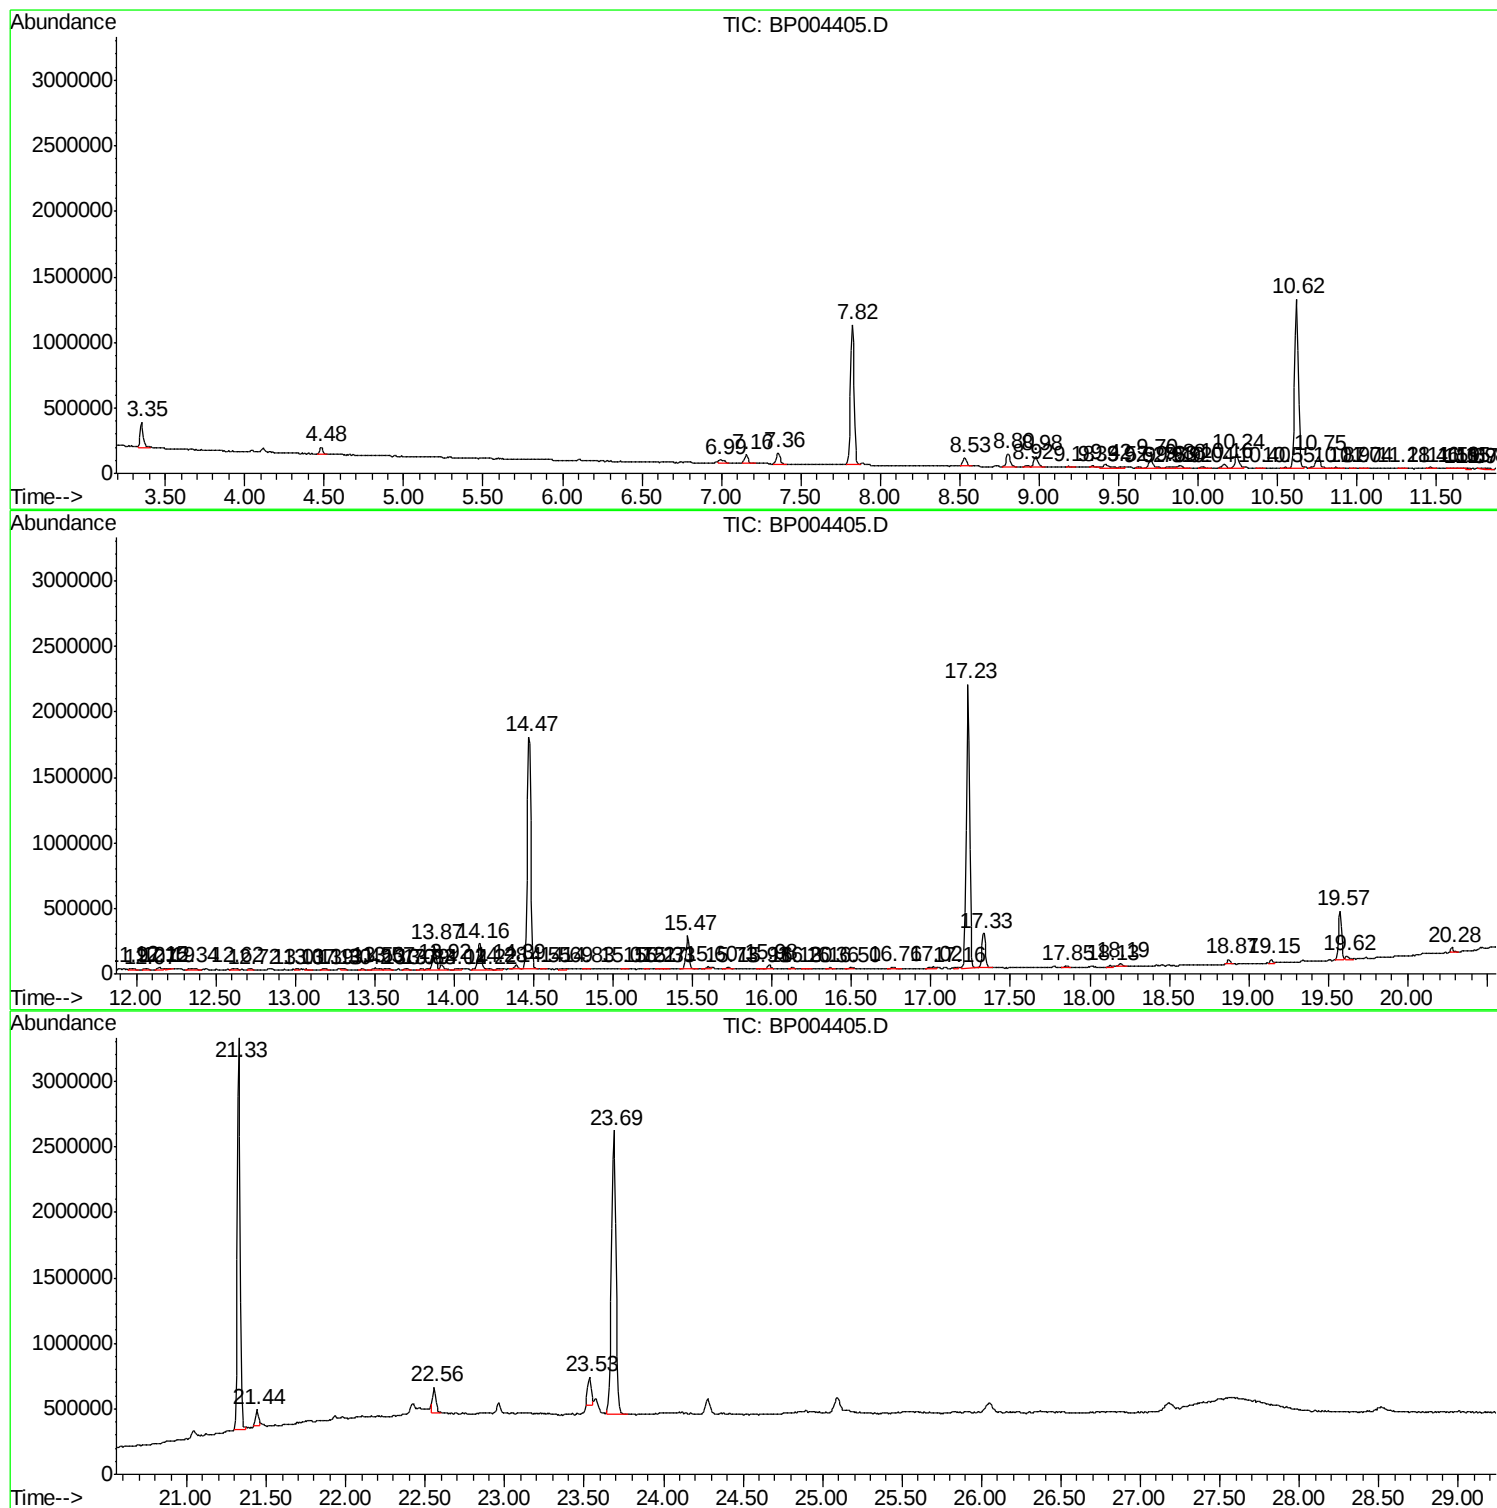

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122120\
Data File : BP004405.D
Acq On : 21 Dec 2020 12:32
Operator : CG/JU
Sample : L5128-02DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8C0DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122120\
Data File : BP004405.D
Acq On : 21 Dec 2020 12:32
Operator : CG/JU
Sample : L5128-02DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8C0DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc