

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
 Data File : BP004409.D
 Acq On : 21 Dec 2020 15:37
 Operator : CG/JU
 Sample : L5114-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54R4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	20	22	34	rVB	69791	107050	1.79%	0.167%
2	6.993	640	647	662	rVB	1127048	2009754	33.64%	3.127%
3	7.157	668	675	687	rVB	890745	1468239	24.58%	2.284%
4	7.357	702	709	719	rVB	1219136	1948893	32.62%	3.032%
5	7.822	781	788	796	rBV	1178354	1900643	31.81%	2.957%
6	7.887	796	799	807	rVB3	20861	36508	0.61%	0.057%
7	8.528	901	908	918	rBV	1377819	2203784	36.89%	3.428%
8	8.981	977	985	993	rBV	1003356	1757274	29.41%	2.734%
9	9.410	1054	1058	1064	rVB	33759	53205	0.89%	0.083%
10	9.698	1100	1107	1120	rBV	858161	1454166	24.34%	2.262%
11	10.239	1192	1199	1217	rBV	1318801	2271414	38.02%	3.534%
12	10.616	1255	1263	1272	rBV	1467409	2535582	42.44%	3.945%
13	10.751	1277	1286	1300	rBV	1205198	2100732	35.16%	3.268%
14	12.051	1502	1507	1512	rBV4	8048	11604	0.19%	0.018%
15	12.110	1512	1517	1522	rBV3	7196	11927	0.20%	0.019%
16	12.210	1528	1534	1542	rVB2	24538	41614	0.70%	0.065%
17	12.286	1542	1547	1552	rVB6	3093	6206	0.10%	0.010%
18	12.504	1579	1584	1590	rBV7	3437	6035	0.10%	0.009%
19	13.010	1666	1670	1676	rBV8	4336	7640	0.13%	0.012%
20	13.298	1714	1719	1725	rVV3	18663	30132	0.50%	0.047%
21	13.369	1727	1731	1737	rVV5	8083	14030	0.23%	0.022%
22	13.433	1737	1742	1750	rVB7	6280	13442	0.22%	0.021%
23	13.645	1770	1778	1780	rBV9	3630	7264	0.12%	0.011%
24	13.692	1781	1786	1792	rVB3	9491	17040	0.29%	0.027%
25	13.792	1797	1803	1807	rBV5	6238	11455	0.19%	0.018%
26	13.875	1809	1817	1822	rVV	1886585	2700494	45.20%	4.201%
27	13.922	1822	1825	1834	rVV	116935	167728	2.81%	0.261%
28	14.163	1857	1866	1877	rBV	2563138	3750662	62.78%	5.835%
29	14.380	1898	1903	1906	rVB2	11006	14505	0.24%	0.023%
30	14.469	1911	1918	1926	rBV	1875604	2896882	48.49%	4.507%
31	14.533	1926	1929	1936	rVB3	12617	21967	0.37%	0.034%
32	14.675	1946	1953	1966	rBV	675753	1063700	17.80%	1.655%
33	14.786	1970	1972	1975	rVV4	8194	10520	0.18%	0.016%
34	14.833	1975	1980	1982	rVV6	6816	13880	0.23%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
 Data File : BP004409.D
 Acq On : 21 Dec 2020 15:37
 Operator : CG/JU
 Sample : L5114-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54R4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	14.886	1984	1989	1995	rVV6	11858	26554	0.44%	0.041%
36	14.939	1995	1998	2004	rVB8	3516	6862	0.11%	0.011%
37	15.274	2047	2055	2058	rBV5	6804	15045	0.25%	0.023%
38	15.333	2061	2065	2070	rVB3	9433	13220	0.22%	0.021%
39	15.469	2081	2088	2095	rBV	2792539	4158521	69.61%	6.469%
40	15.522	2095	2097	2103	rVV	10193	14901	0.25%	0.023%
41	15.598	2103	2110	2122	rVV	570730	851753	14.26%	1.325%
42	15.710	2122	2129	2138	rVB	33975	67360	1.13%	0.105%
43	16.045	2181	2186	2189	rBV5	5397	10453	0.17%	0.016%
44	16.157	2200	2205	2208	rBV6	5937	10378	0.17%	0.016%
45	16.204	2208	2213	2218	rVV9	10761	19547	0.33%	0.030%
46	16.257	2218	2222	2228	rVB4	12212	18385	0.31%	0.029%
47	16.374	2234	2242	2246	rBV10	5278	11625	0.19%	0.018%
48	16.469	2252	2258	2263	rBV2	9377	11858	0.20%	0.018%
49	16.539	2267	2270	2274	rVB5	5033	7028	0.12%	0.011%
50	16.586	2274	2278	2283	rBV6	4426	7562	0.13%	0.012%
51	16.886	2325	2329	2331	rBV4	7394	11040	0.18%	0.017%
52	16.992	2340	2347	2349	rBV8	7167	15095	0.25%	0.023%
53	17.051	2353	2357	2366	rVB2	14655	23900	0.40%	0.037%
54	17.233	2381	2388	2393	rBV	2051928	2982022	49.91%	4.639%
55	17.274	2393	2395	2399	rVV	183790	212149	3.55%	0.330%
56	17.333	2399	2405	2417	rVV	2909969	4108841	68.78%	6.392%
57	17.427	2417	2421	2425	rVB7	5034	9843	0.16%	0.015%
58	17.610	2448	2452	2453	rBV3	5815	7939	0.13%	0.012%
59	17.757	2474	2477	2481	rBV6	5935	8171	0.14%	0.013%
60	17.816	2483	2487	2490	rVV2	11948	14923	0.25%	0.023%
61	17.957	2508	2511	2518	rVB5	9433	16184	0.27%	0.025%
62	18.027	2518	2523	2526	rBV7	8271	15105	0.25%	0.023%
63	18.121	2531	2539	2541	rVV2	67377	140226	2.35%	0.218%
64	18.151	2541	2544	2548	rVV	64039	99541	1.67%	0.155%
65	18.192	2549	2551	2554	rVV2	19794	24986	0.42%	0.039%
66	18.227	2555	2557	2562	rVV2	23441	33144	0.55%	0.052%
67	18.286	2562	2567	2572	rVV2	58048	121548	2.03%	0.189%
68	18.327	2572	2574	2580	rVB2	35864	46543	0.78%	0.072%
69	18.410	2585	2588	2590	rBV4	6487	9139	0.15%	0.014%
70	18.445	2591	2594	2598	rBV6	8642	12935	0.22%	0.020%
71	18.586	2615	2618	2622	rBV	26624	34883	0.58%	0.054%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
 Data File : BP004409.D
 Acq On : 21 Dec 2020 15:37
 Operator : CG/JU
 Sample : L5114-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54R4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

72	18.627	2622	2625	2632	rVB5	20337	35135	0.59%	0.055%
73	18.827	2657	2659	2662	rVB2	12888	12428	0.21%	0.019%
74	18.910	2671	2673	2677	rVB5	10401	12197	0.20%	0.019%
75	18.992	2684	2687	2691	rVB	25574	32909	0.55%	0.051%
76	19.139	2706	2712	2718	rBV4	35638	91048	1.52%	0.142%
77	19.215	2722	2725	2727	rVV	39844	50973	0.85%	0.079%
78	19.251	2727	2731	2737	rVB	185997	248850	4.17%	0.387%
79	19.462	2765	2767	2769	rBV	20154	22364	0.37%	0.035%
80	19.492	2769	2772	2780	rVB2	69059	104736	1.75%	0.163%
81	19.574	2780	2786	2799	rBV	3740883	5234558	87.62%	8.143%
82	19.804	2822	2825	2828	rVB	43228	44551	0.75%	0.069%
83	20.380	2919	2923	2926	rBV	36236	48287	0.81%	0.075%
84	21.039	3032	3035	3042	rBV2	180345	286934	4.80%	0.446%
85	21.327	3078	3084	3088	rBV	2773392	3618567	60.57%	5.629%
86	21.439	3100	3103	3107	rBV	100519	130384	2.18%	0.203%
87	22.962	3359	3362	3377	rVB2	184505	493834	8.27%	0.768%
88	23.533	3452	3459	3475	rVB	2786032	5974263	100.00%	9.294%
89	23.686	3478	3485	3500	rVB2	1891043	3971971	66.48%	6.179%


Sum of corrected areas: 64279169

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
Data File : BP004409.D
Acq On : 21 Dec 2020 15:37
Operator : CG/JU
Sample : L5114-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
A54R4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

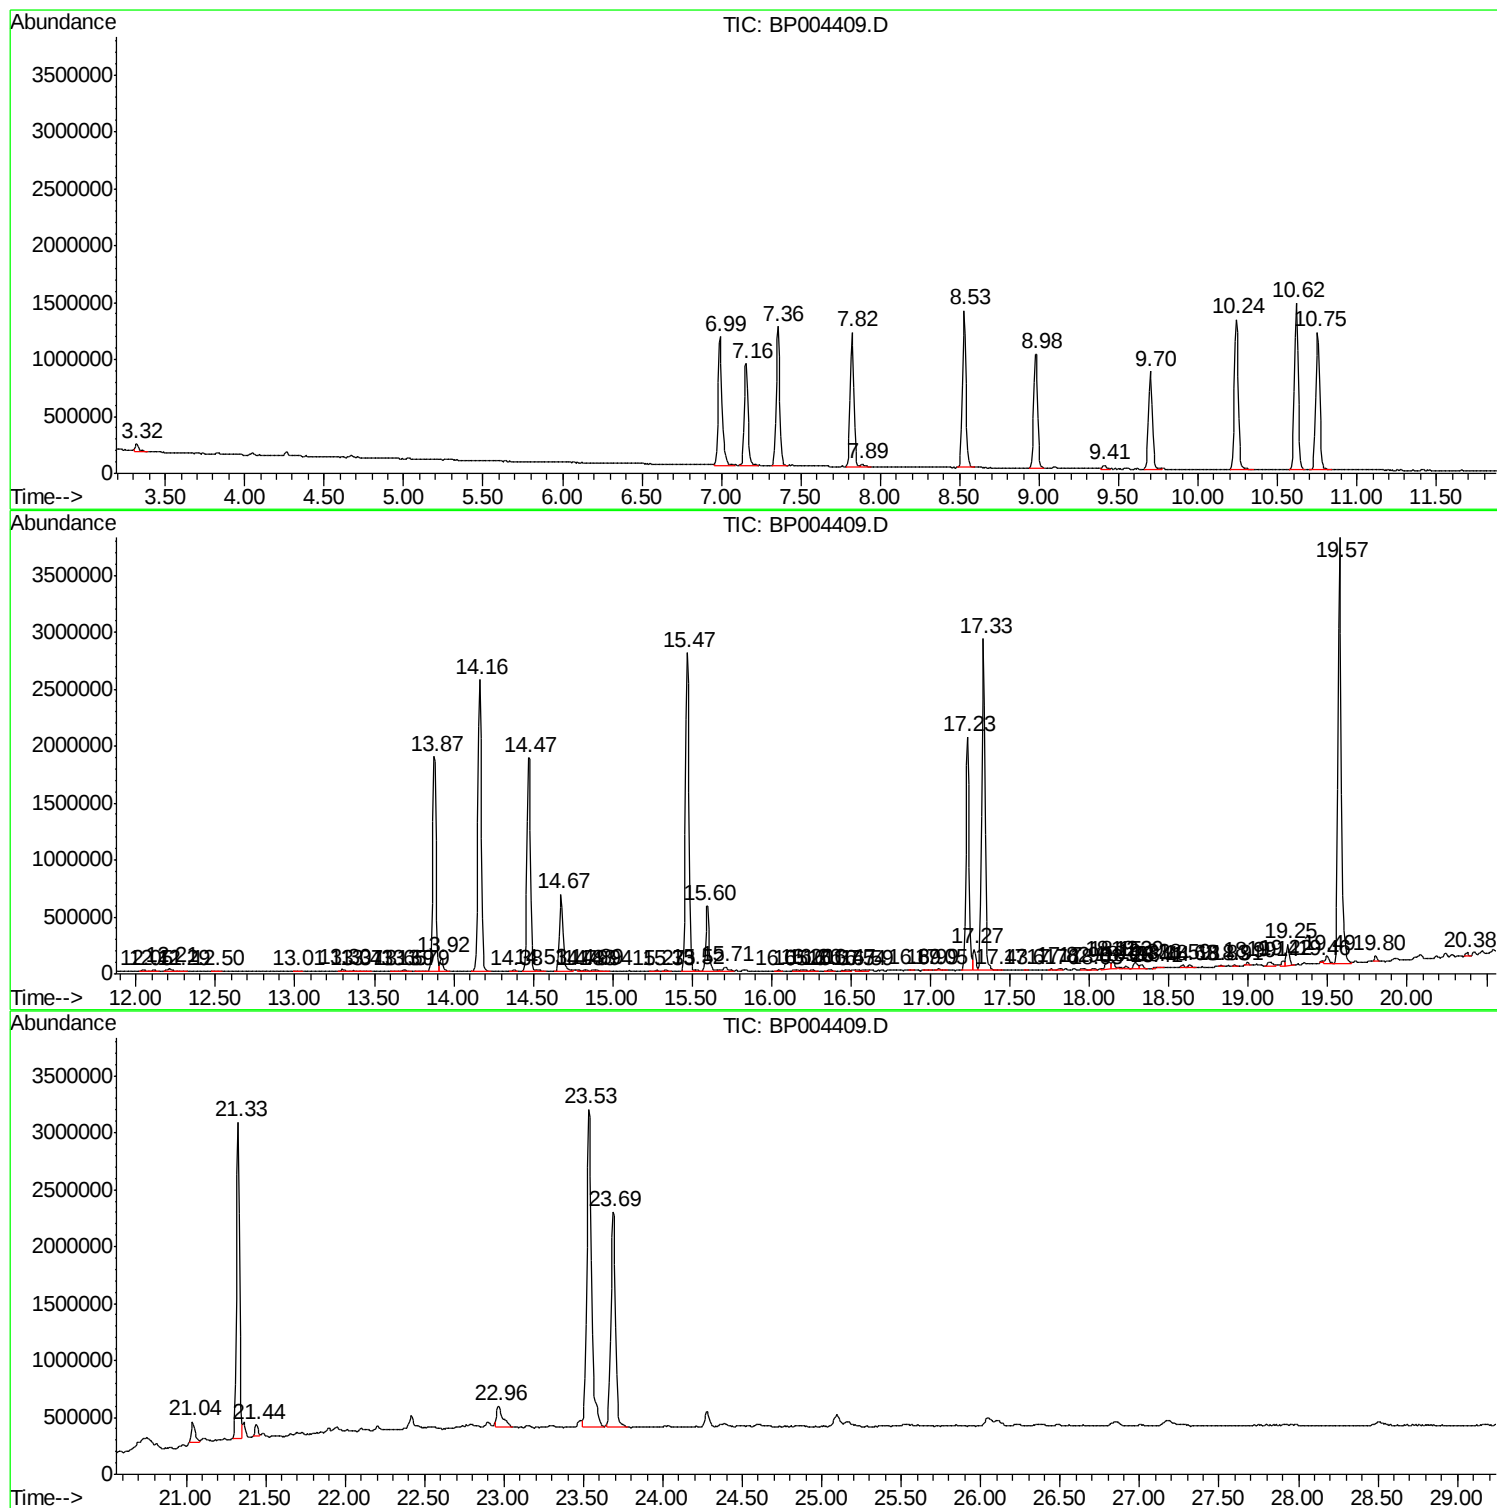

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122120\
Data File : BP004409.D
Acq On : 21 Dec 2020 15:37
Operator : CG/JU
Sample : L5114-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54R4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122120\
Data File : BP004409.D
Acq On : 21 Dec 2020 15:37
Operator : CG/JU
Sample : L5114-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54R4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc