

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
 Data File : BP004415.D
 Acq On : 21 Dec 2020 19:01
 Operator : CG/JU
 Sample : L5154-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.987	641	646	659	rVB	230792	381414	5.31%	0.696%
2	7.152	668	674	688	rVB	827374	1352698	18.84%	2.467%
3	7.357	702	709	719	rBV	888142	1477620	20.58%	2.695%
4	7.822	782	788	796	rVB	915413	1458439	20.31%	2.660%
5	8.528	901	908	919	rBV	642879	1049363	14.61%	1.914%
6	8.975	977	984	993	rBV	964402	1631805	22.73%	2.977%
7	9.410	1054	1058	1064	rVB3	12214	19412	0.27%	0.035%
8	9.698	1100	1107	1120	rBV	798414	1314593	18.31%	2.398%
9	10.240	1191	1199	1212	rBV	1164212	1989454	27.71%	3.629%
10	10.393	1223	1225	1233	rVB7	6254	12455	0.17%	0.023%
11	10.616	1256	1263	1272	rBV	1150096	1949423	27.15%	3.556%
12	10.751	1280	1286	1294	rVB	71059	127541	1.78%	0.233%
13	11.157	1350	1355	1360	rBV2	10730	18117	0.25%	0.033%
14	11.216	1361	1365	1369	rVV2	11634	19535	0.27%	0.036%
15	11.269	1371	1374	1379	rVB	8954	13891	0.19%	0.025%
16	12.210	1528	1534	1541	rVB2	21863	39450	0.55%	0.072%
17	12.822	1633	1638	1645	rBV2	16704	27396	0.38%	0.050%
18	13.075	1675	1681	1688	rBV	28094	40194	0.56%	0.073%
19	13.439	1740	1743	1748	rVB4	5441	7415	0.10%	0.014%
20	13.875	1810	1817	1822	rBV	1909910	2647617	36.87%	4.829%
21	13.922	1822	1825	1830	rVV	121705	168022	2.34%	0.306%
22	13.992	1833	1837	1843	rVB9	4786	10392	0.14%	0.019%
23	14.163	1855	1866	1879	rBV	2365065	3633762	50.61%	6.628%
24	14.469	1909	1918	1932	rBV	1508374	2284366	31.81%	4.167%
25	14.675	1948	1953	1966	rBV	126475	226960	3.16%	0.414%
26	15.292	2050	2058	2063	rBV2	25546	44837	0.62%	0.082%
27	15.469	2079	2088	2101	rBV	2948921	4311197	60.04%	7.864%
28	15.592	2103	2109	2123	rVV	740977	1062962	14.80%	1.939%
29	15.710	2124	2129	2136	rVB	35730	55132	0.77%	0.101%
30	15.833	2143	2150	2154	rVV10	4475	9847	0.14%	0.018%
31	16.157	2201	2205	2208	rBV5	4723	8222	0.11%	0.015%
32	16.257	2218	2222	2228	rVB3	12112	19257	0.27%	0.035%
33	16.375	2236	2242	2248	rBV4	8154	13111	0.18%	0.024%
34	17.010	2342	2350	2355	rBV5	9084	23422	0.33%	0.043%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
 Data File : BP004415.D
 Acq On : 21 Dec 2020 19:01
 Operator : CG/JU
 Sample : L5154-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
 Title : SVOA CALIBRATION

35	17.163	2371	2376	2380	rBV7	4922	8256	0.11%	0.015%
36	17.233	2380	2388	2398	rBV	1746169	2465062	34.33%	4.496%
37	17.333	2398	2405	2418	rVV	3403911	4766715	66.39%	8.695%
38	17.528	2432	2438	2444	rVB5	4827	9888	0.14%	0.018%
39	17.851	2490	2493	2497	rVB5	6186	8283	0.12%	0.015%
40	18.122	2536	2539	2544	rBV6	13776	19920	0.28%	0.036%
41	18.192	2547	2551	2555	rVB2	11561	17207	0.24%	0.031%
42	18.416	2585	2589	2592	rBV6	6202	9408	0.13%	0.017%
43	19.145	2710	2713	2716	rBV5	7630	11647	0.16%	0.021%
44	19.216	2721	2725	2732	rVV	38945	58078	0.81%	0.106%
45	19.463	2764	2767	2772	rBV	33860	41229	0.57%	0.075%
46	19.574	2780	2786	2792	rBV	4402431	5901987	82.20%	10.766%
47	21.045	3032	3036	3045	rBV5	57506	124830	1.74%	0.228%
48	21.327	3079	3084	3091	rBV	2496033	3099211	43.16%	5.653%
49	21.439	3100	3103	3107	rBV	86191	122030	1.70%	0.223%
50	23.539	3452	3460	3474	rVV	3544605	7180250	100.00%	13.097%
51	23.686	3478	3485	3501	rVB	1756606	3528784	49.15%	6.437%


Sum of corrected areas: 54822106

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP122120\
Data File : BP004415.D
Acq On : 21 Dec 2020 19:01
Operator : CG/JU
Sample : L5154-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

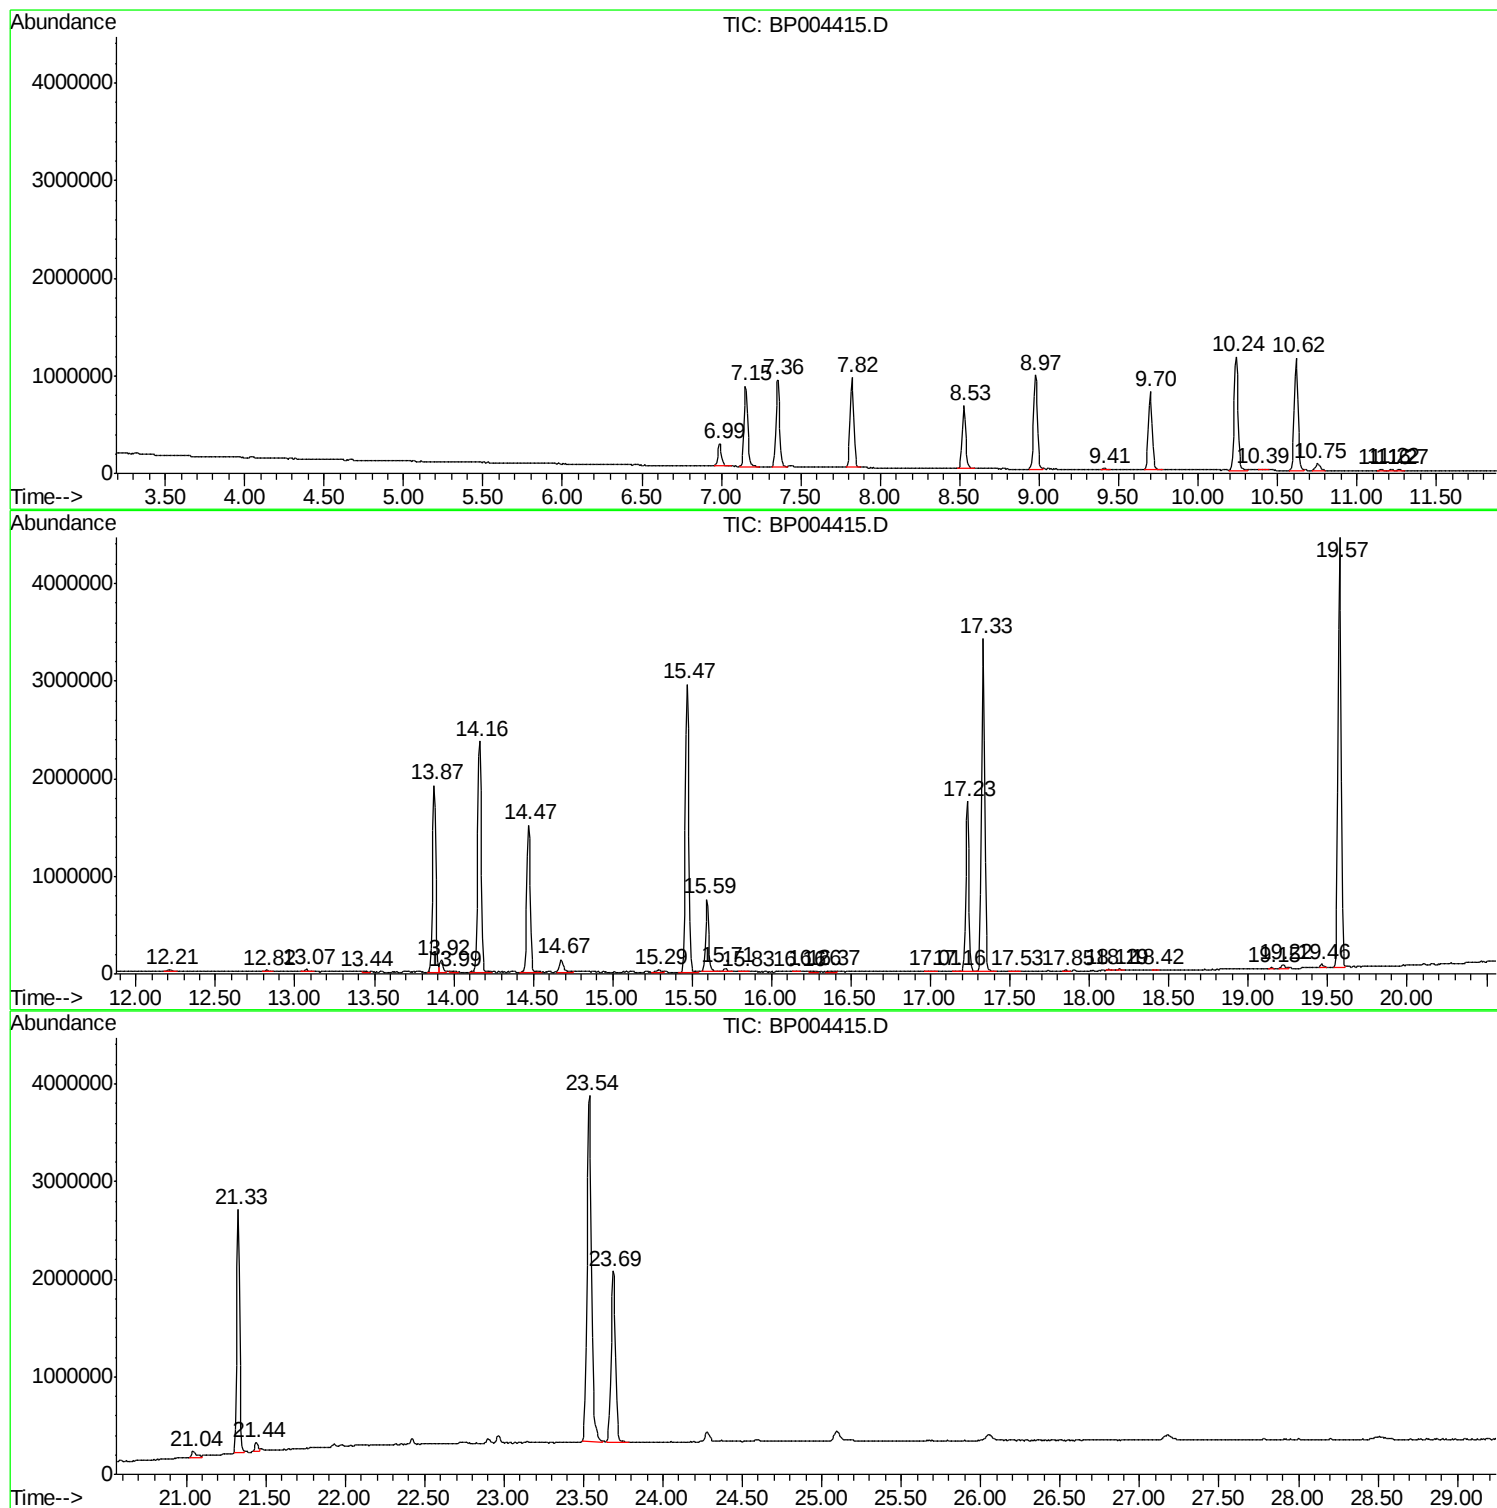

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122120\
Data File : BP004415.D
Acq On : 21 Dec 2020 19:01
Operator : CG/JU
Sample : L5154-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP122120\
Data File : BP004415.D
Acq On : 21 Dec 2020 19:01
Operator : CG/JU
Sample : L5154-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121820MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc