

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019019.D
 Acq On : 22 Dec 2023 02:59
 Operator : MA/JU
 Sample : 05808-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B22

Quant Time: Dec 22 08:52:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 21 04:46:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	162011	20.000	ng/ul	0.00
20) Naphthalene-d8	10.616	136	644562	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.451	164	438209	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	1047383	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.298	240	1093352	20.000	ng/ul	# 0.00
88) Perylene-d12	23.657	264	1293867	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	25455	5.354	ng/uL	0.00
4) Pyridine-d5	3.669	84	303155	23.806	ng/ul	0.00
7) Phenol-d5	6.999	99	493652	30.363	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.157	67	269811	28.000	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	377671	29.770	ng/ul	0.00
15) 4-Methylphenol-d8	8.534	113	406725	30.912	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	186479	32.506	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	218145	36.677	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.240	165	425487	34.985	ng/ul	0.00
31) 4-Chloroaniline-d4	10.757	131	459381	28.903	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	1324432	33.864	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	1496270	34.744	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	223468	34.809	ng/ul	0.00
60) Fluorene-d10	15.445	176	1185361	36.107	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	225617	35.926	ng/ul	0.00
73) Anthracene-d10	17.304	188	1902208	34.546	ng/ul	0.00
81) Pyrene-d10	19.545	212	2387178	28.049	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	2614040	34.650	ng/ul	0.00
Target Compounds						
12) 2-Chlorophenol	7.381	128	14236	1.109	ng/ul	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019019.D
Acq On : 22 Dec 2023 02:59
Operator : MA/JU
Sample : 05808-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B22

Quant Time: Dec 22 08:52:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 21 04:46:12 2023
Response via : Initial Calibration

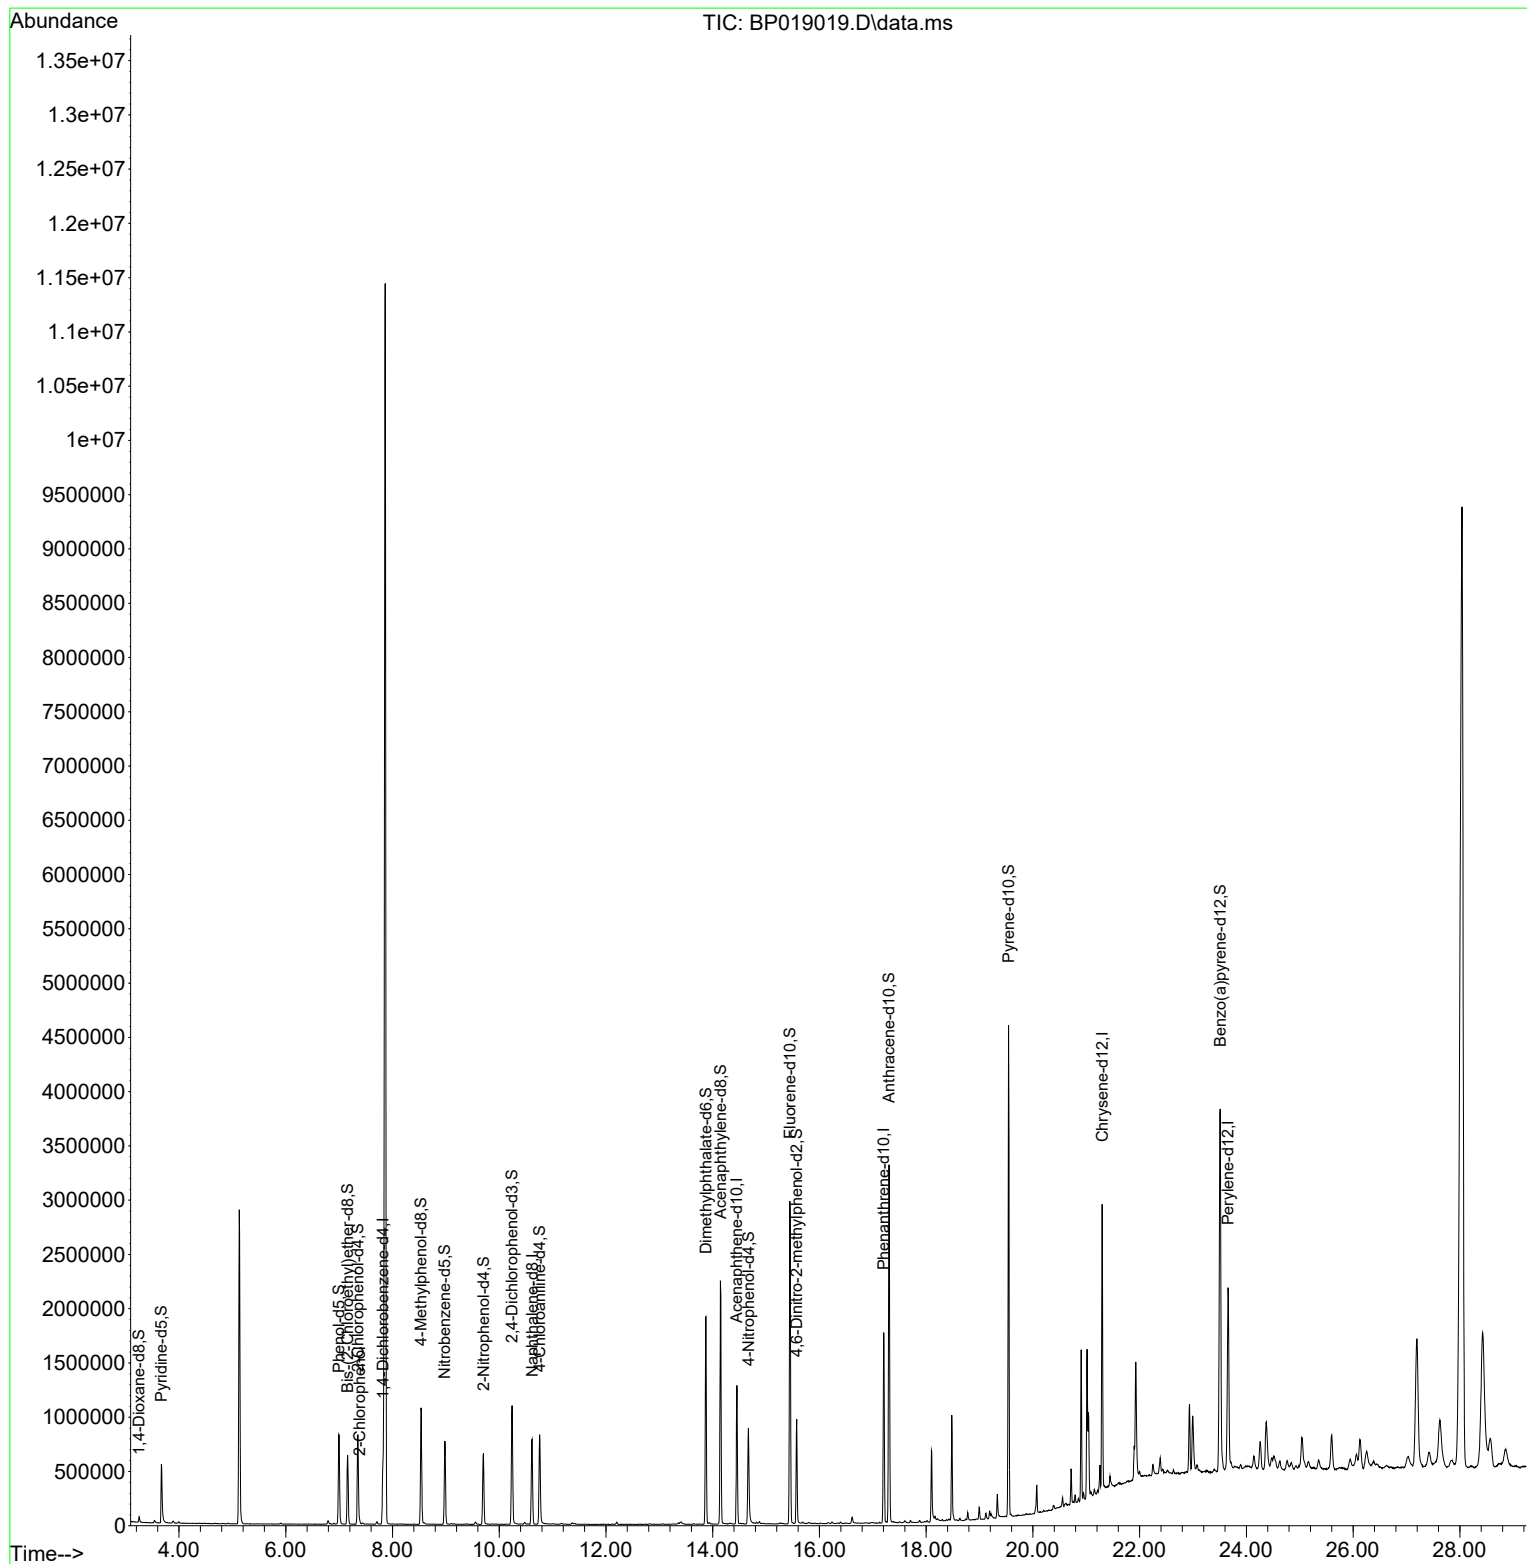

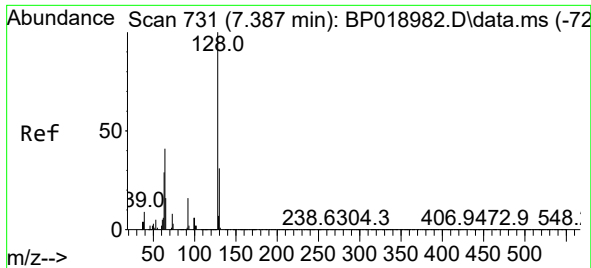

#12
 2-Chlorophenol
 Concen: 1.109 ng/ul
 RT: 7.381 min Scan# 71
 Delta R.T. -0.006 min
 Lab File: BP019019.D
 Acq: 22 Dec 2023 02:59

Instrument :
 BNA_P
 ClientSampleId :
 C0B22

Tgt Ion:128 Resp: 14236
 Ion Ratio Lower Upper
 128 100
 64 53.1 37.0 55.4
 130 36.8 26.8 40.2

