

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019026.D
 Acq On : 22 Dec 2023 06:56
 Operator : MA/JU
 Sample : 05808-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B35

Quant Time: Dec 22 08:53:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 21 04:46:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	151532	20.000	ng/ul	0.00
20) Naphthalene-d8	10.616	136	583376	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.451	164	390102	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	919870	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	968126	20.000	ng/ul	# 0.00
88) Perylene-d12	23.657	264	1135826	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	25645	5.767	ng/uL	0.00
4) Pyridine-d5	3.669	84	247835	20.808	ng/ul	0.00
7) Phenol-d5	6.999	99	474885	31.228	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.158	67	263670	29.255	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	377236	31.792	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	388906	31.601	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	182783	35.203	ng/ul	0.00
24) 2-Nitrophenol-d4	9.699	143	212330	39.444	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.240	165	410274	37.273	ng/ul	0.00
31) 4-Chloroaniline-d4	10.757	131	443286	30.815	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	1281723	36.813	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	1453967	37.925	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	210689	36.865	ng/ul	0.00
60) Fluorene-d10	15.451	176	1141778	39.068	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	203270	36.854	ng/ul	0.00
73) Anthracene-d10	17.304	188	1869039	38.649	ng/ul	0.00
81) Pyrene-d10	19.545	212	2353801	31.234	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	2550389	38.510	ng/ul	0.00
Target Compounds						
					Qvalue	
93) Benzo(a)pyrene	23.710	252	130242	1.702	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019026.D
Acq On : 22 Dec 2023 06:56
Operator : MA/JU
Sample : 05808-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B35

Quant Time: Dec 22 08:53:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 21 04:46:12 2023
Response via : Initial Calibration

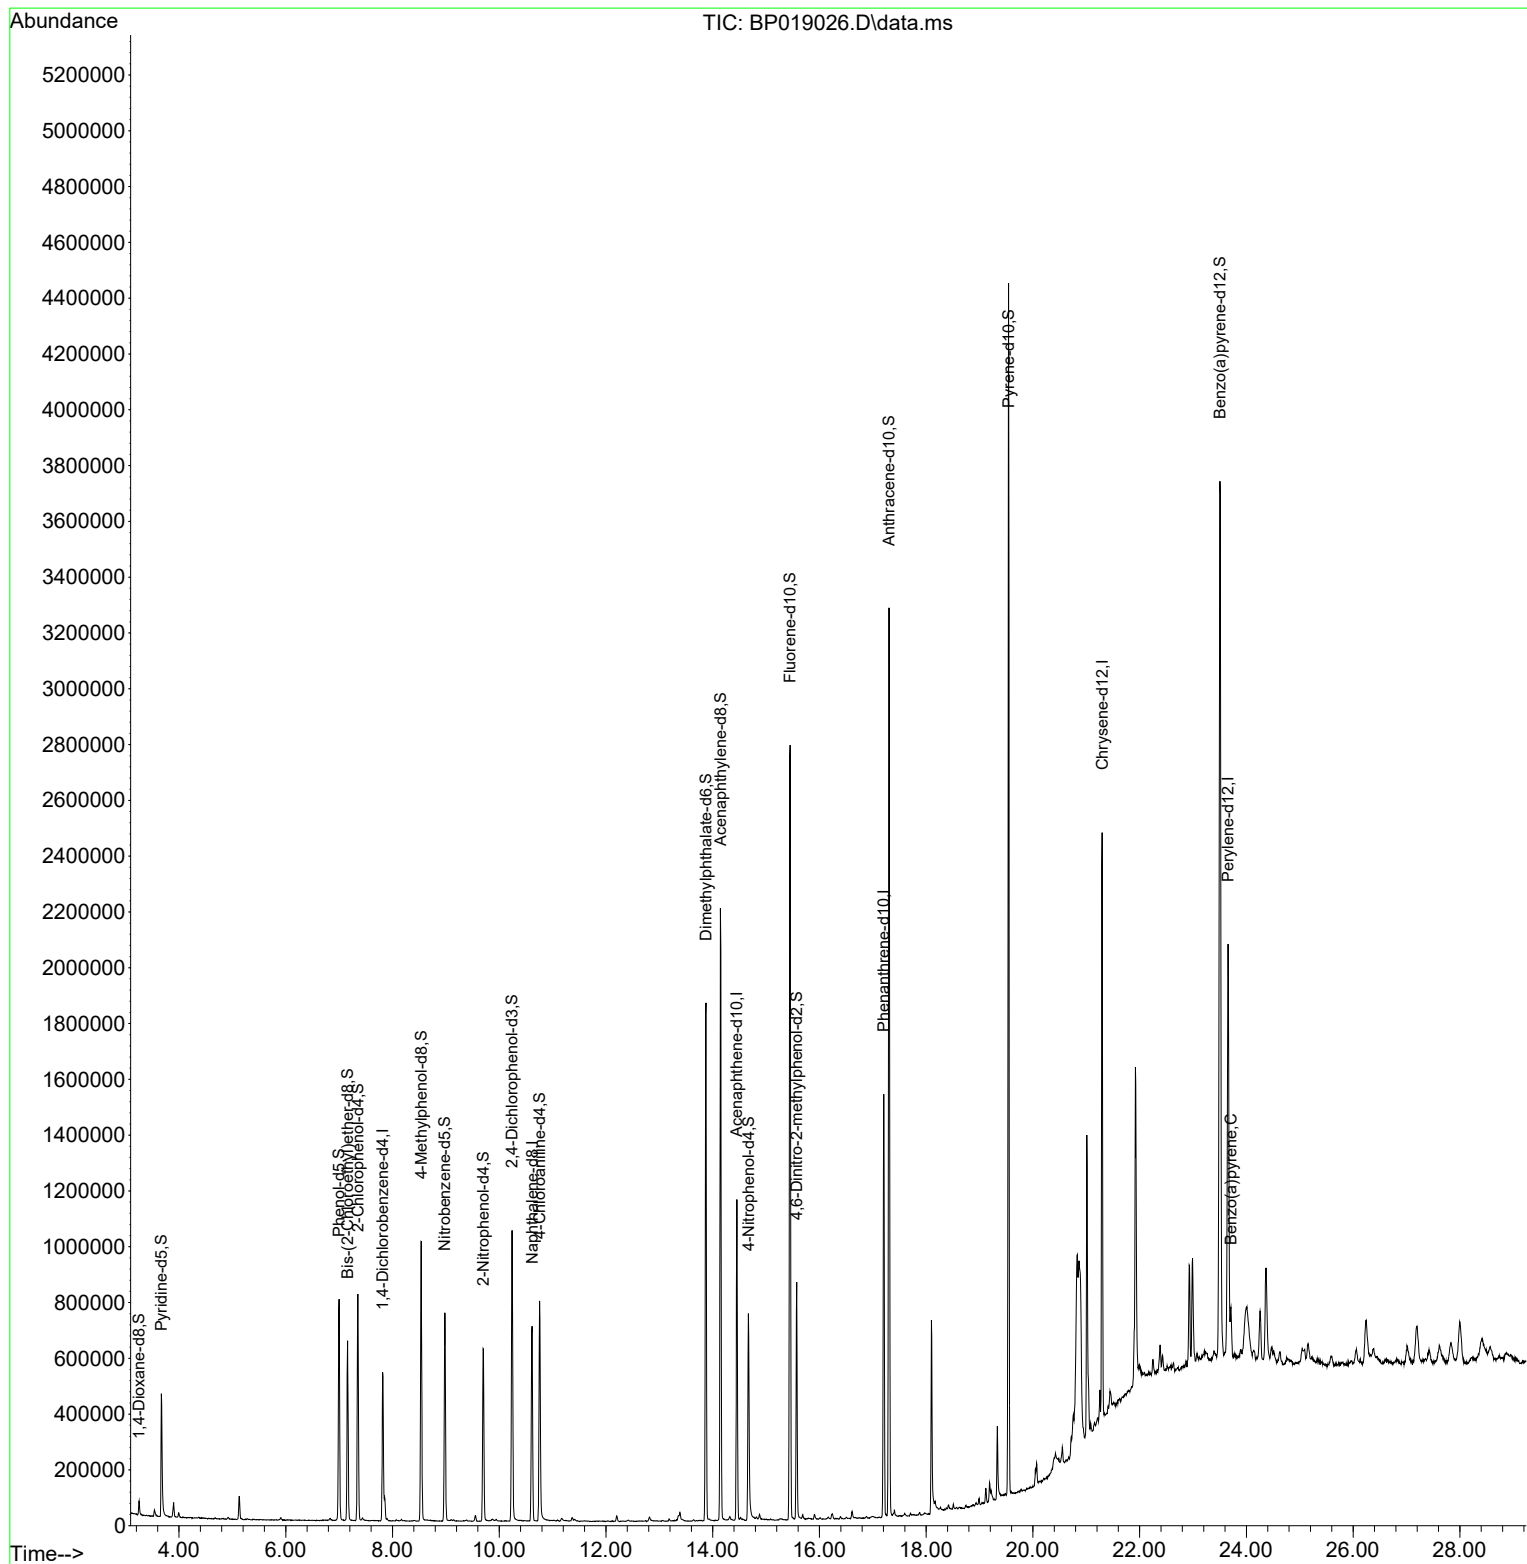

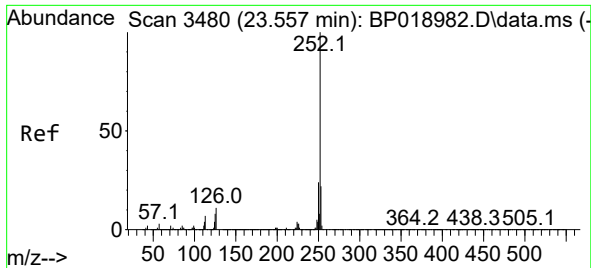

#93

Benzo(a)pyrene

Concen: 1.702 ng/ul

RT: 23.710 min Scan# 3

Delta R.T. 0.153 min

Lab File: BP019026.D


Acq: 22 Dec 2023 06:56

Instrument :

BNA_P

ClientSampleId :

C0B35

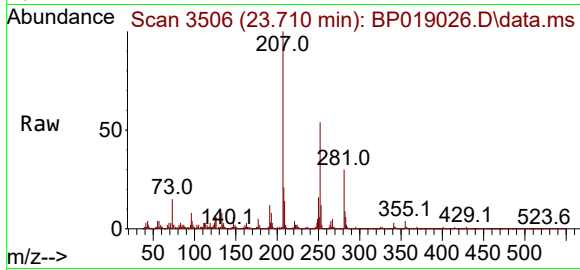

Tgt Ion:252 Resp: 130242

Ion Ratio Lower Upper

252 100

253 22.6 17.8 26.8

125 13.7 9.2 13.8

