

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019014.D
 Acq On : 21 Dec 2023 23:36
 Operator : MA/JU
 Sample : 05808-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B05

Quant Time: Dec 22 08:49:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 21 04:46:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	135271	20.000	ng/ul	0.00
20) Naphthalene-d8	10.616	136	523652	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.451	164	334959	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	784419	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	862519	20.000	ng/ul	# 0.00
88) Perylene-d12	23.657	264	1017586	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	19994	5.037	ng/uL	0.00
4) Pyridine-d5	3.675	84	213280	20.059	ng/ul	0.00
7) Phenol-d5	6.993	99	399908	29.459	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.157	67	217190	26.995	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	307733	29.052	ng/ul	0.00
15) 4-Methylphenol-d8	8.534	113	325449	29.624	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	147821	31.717	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	173182	35.840	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.240	165	334127	33.817	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	221222	17.132	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	993954	33.248	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	1120521	34.039	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	175245	35.712	ng/ul	0.00
60) Fluorene-d10	15.445	176	874464	34.847	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	164350	34.943	ng/ul	0.00
73) Anthracene-d10	17.304	188	1387060	33.635	ng/ul	0.00
81) Pyrene-d10	19.545	212	1804546	26.877	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.504	264	1992364	33.580	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.963	77	8827	1.259	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019014.D
Acq On : 21 Dec 2023 23:36
Operator : MA/JU
Sample : 05808-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B05

Quant Time: Dec 22 08:49:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 21 04:46:12 2023
Response via : Initial Calibration

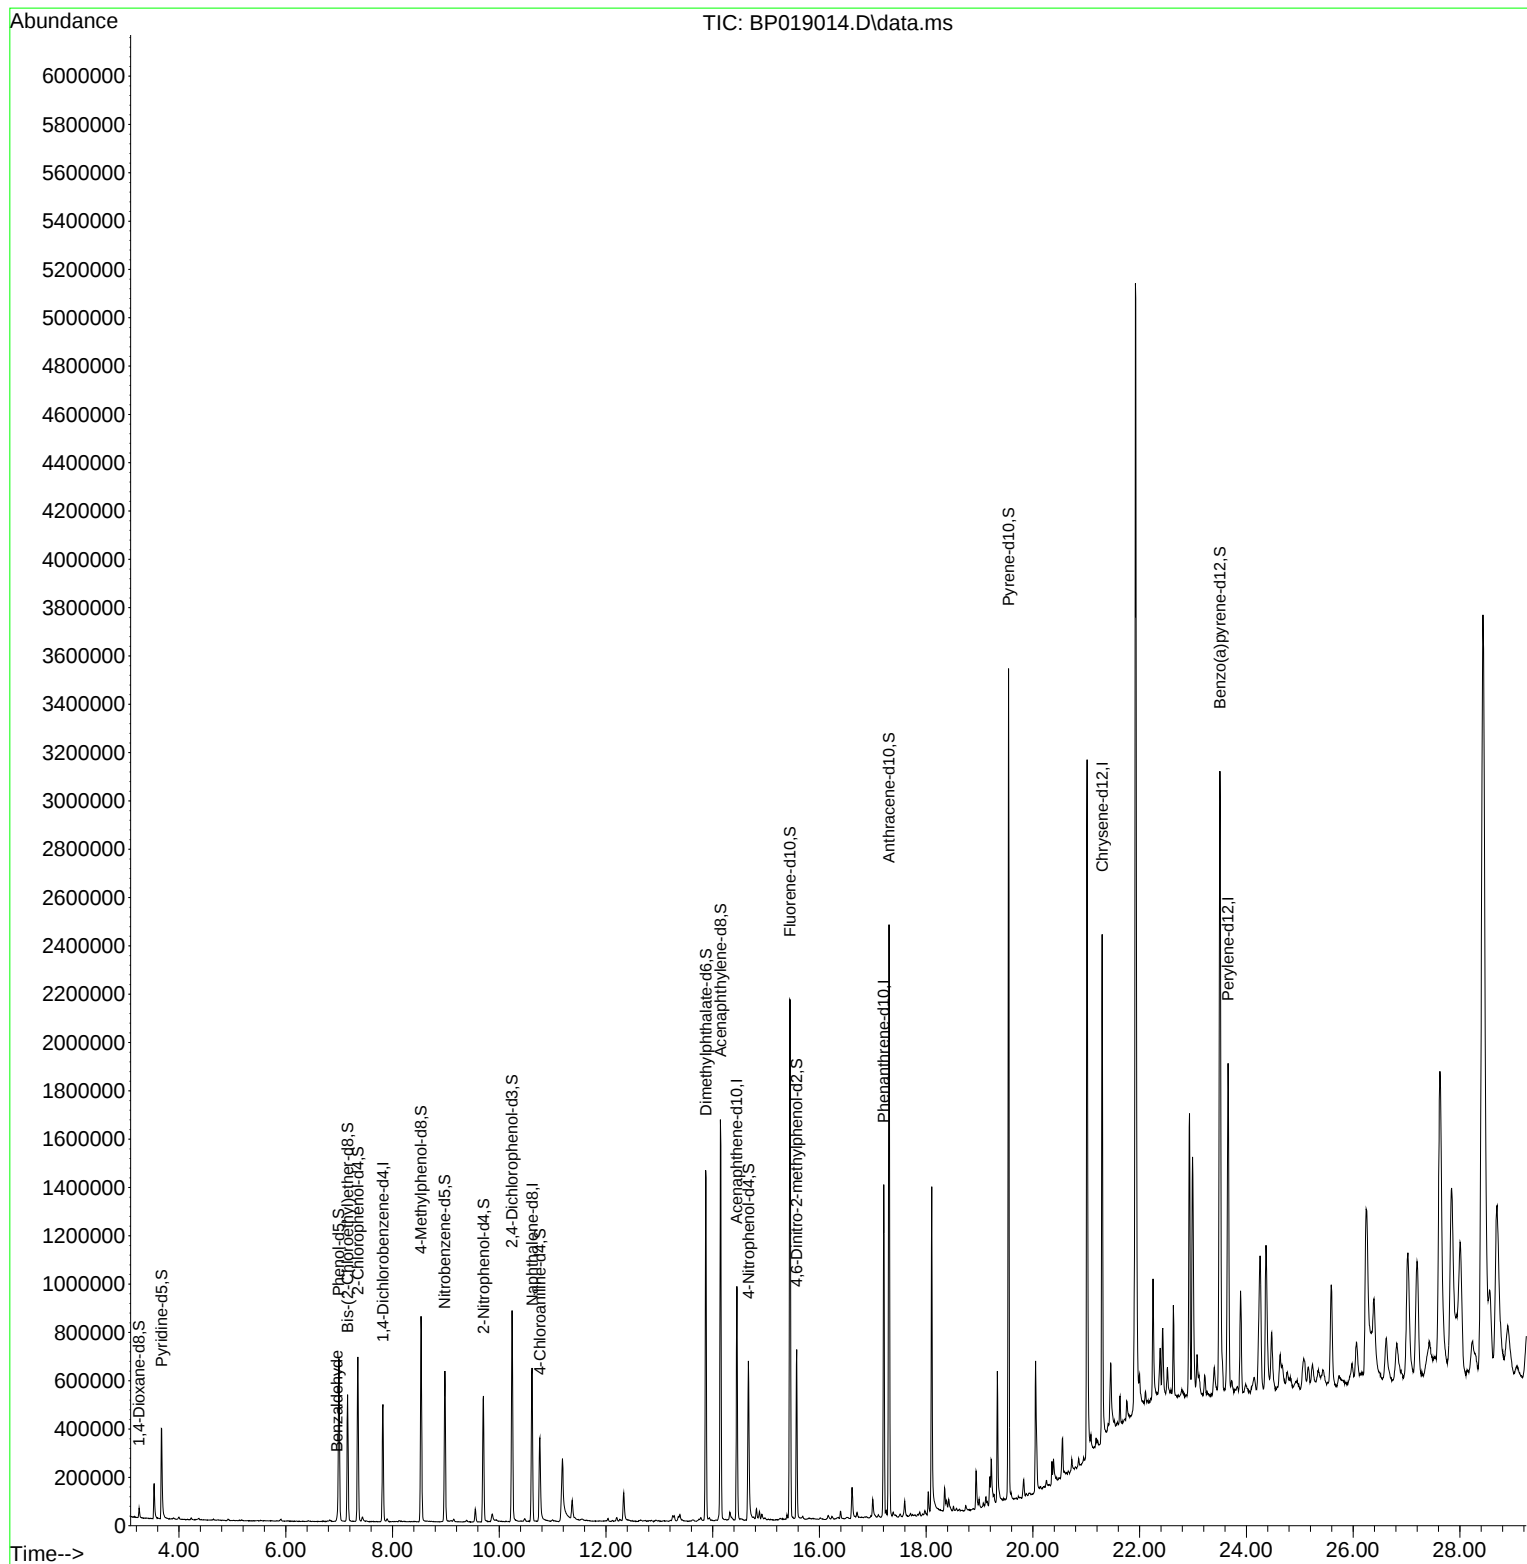

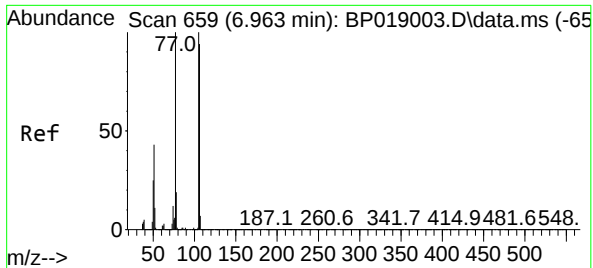

#6
Benzaldehyde
Concen: 1.259 ng/ul
RT: 6.963 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP019014.D
Acq: 21 Dec 2023 23:36

Instrument :
BNA_P
ClientSampleId :
C0B05

Tgt Ion:	77	Resp:	8827
Ion	Ratio	Lower	Upper
77	100		
105	101.2	77.9	116.9
106	107.7	74.6	111.8

