

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019020.D
 Acq On : 22 Dec 2023 03:33
 Operator : MA/JU
 Sample : 05808-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B23

Quant Time: Dec 22 08:52:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 21 04:46:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	138770	20.000	ng/u1	0.00
20) Naphthalene-d8	10.616	136	527186	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.451	164	356457	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.204	188	863675	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.298	240	927560	20.000	ng/u1	# 0.00
88) Perylene-d12	23.657	264	1081398	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	19492	4.787	ng/uL	0.00
4) Pyridine-d5	3.669	84	225221	20.648	ng/u1	0.00
7) Phenol-d5	6.993	99	341692	24.536	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.157	67	193069	23.391	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	272181	25.048	ng/u1	0.00
15) 4-Methylphenol-d8	8.534	113	273499	24.268	ng/u1	0.00
21) Nitrobenzene-d5	8.981	128	128397	27.364	ng/u1	0.00
24) 2-Nitrophenol-d4	9.698	143	146884	30.194	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.240	165	285595	28.711	ng/u1	0.00
31) 4-Chloroaniline-d4	10.757	131	307273	23.637	ng/u1	0.00
46) Dimethylphthalate-d6	13.869	166	873381	27.453	ng/u1	0.00
49) Acenaphthylene-d8	14.145	160	984670	28.108	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	141496	27.095	ng/u1	0.00
60) Fluorene-d10	15.445	176	787601	29.493	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	136484	26.355	ng/u1	0.00
73) Anthracene-d10	17.304	188	1272617	28.028	ng/u1	0.00
81) Pyrene-d10	19.539	212	1619498	22.430	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.504	264	1760305	27.918	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.022	94	16529	1.210	ng/u1#	90
12) 2-Chlorophenol	7.381	128	91265	8.299	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019020.D
Acq On : 22 Dec 2023 03:33
Operator : MA/JU
Sample : 05808-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B23

Quant Time: Dec 22 08:52:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 21 04:46:12 2023
Response via : Initial Calibration




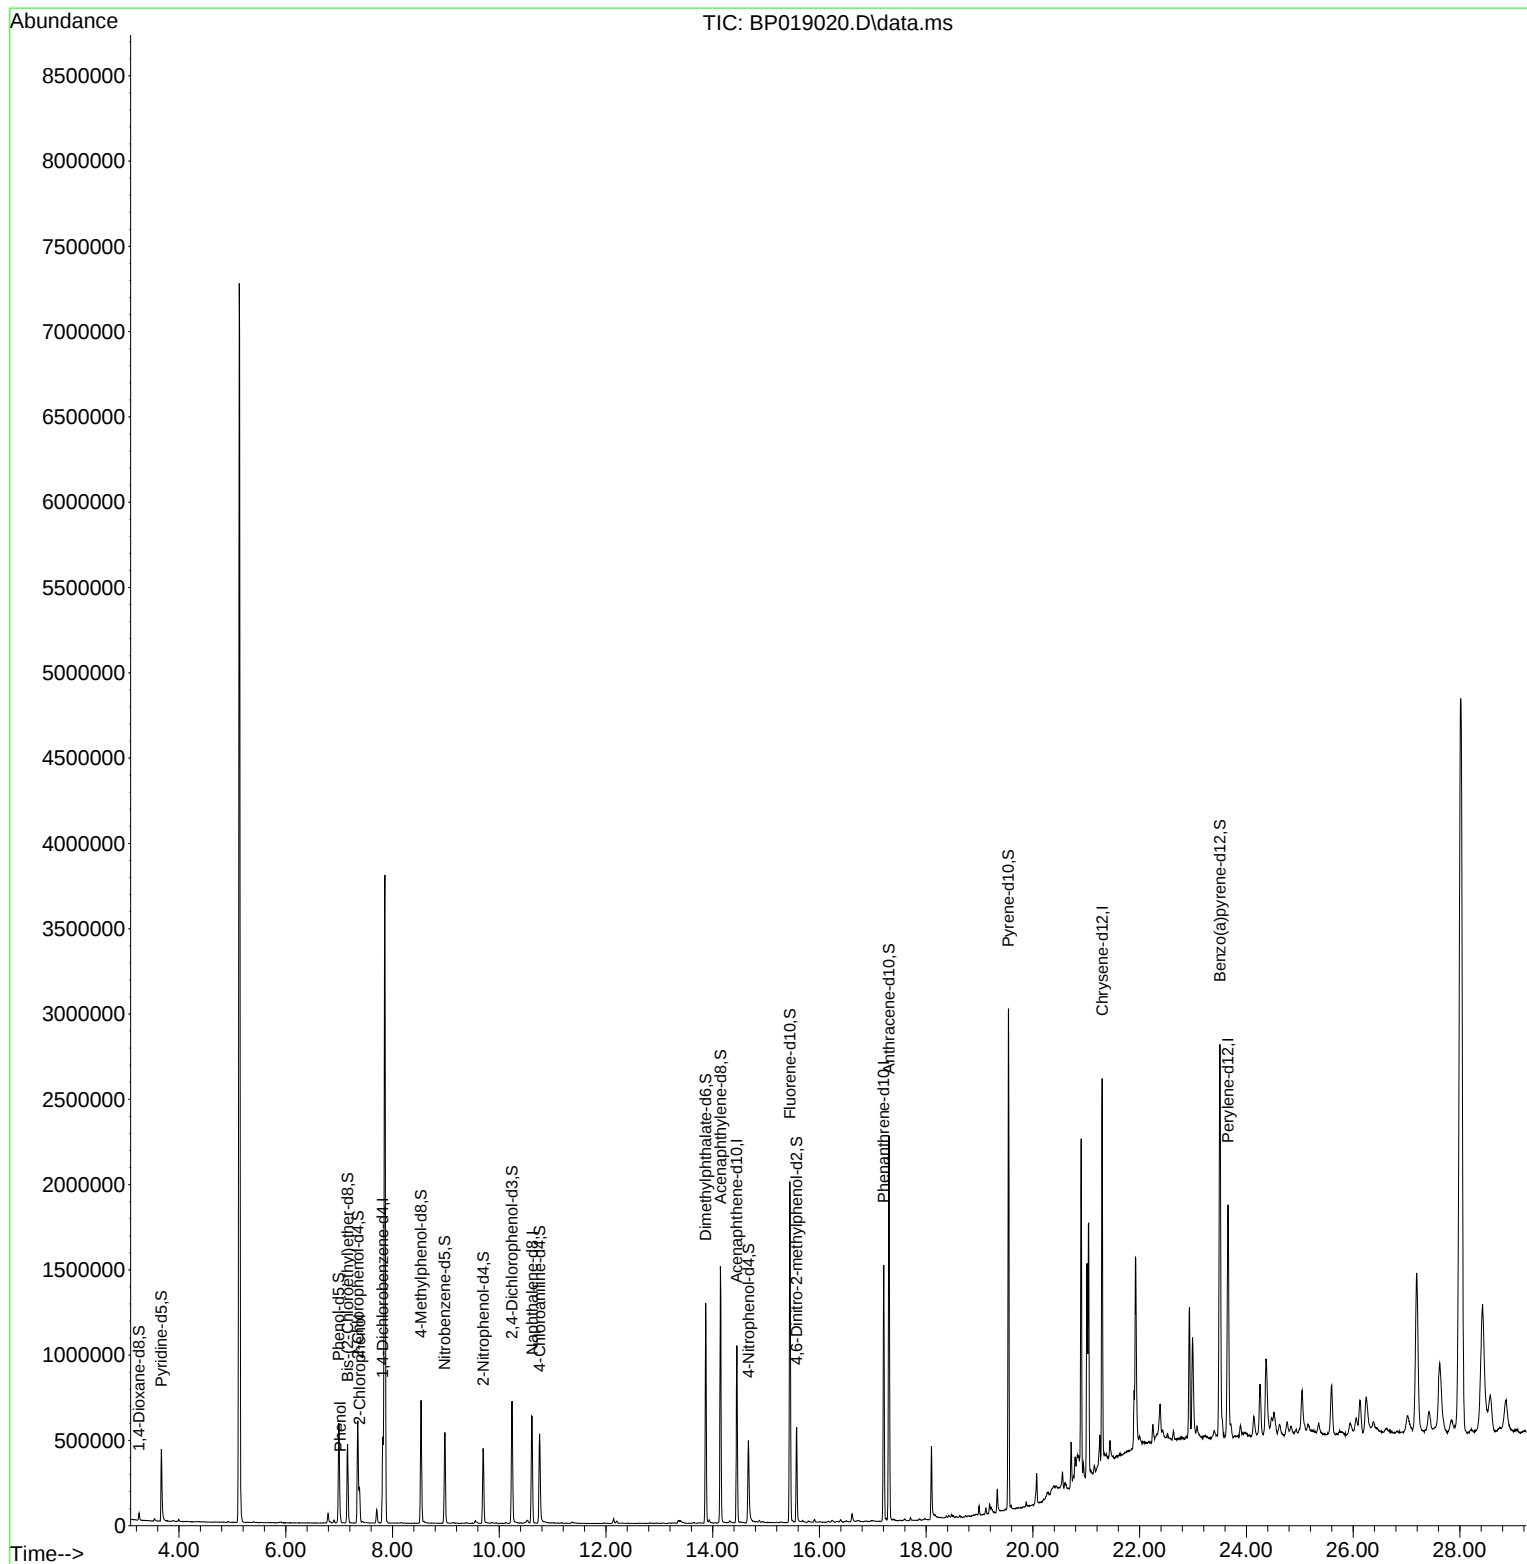


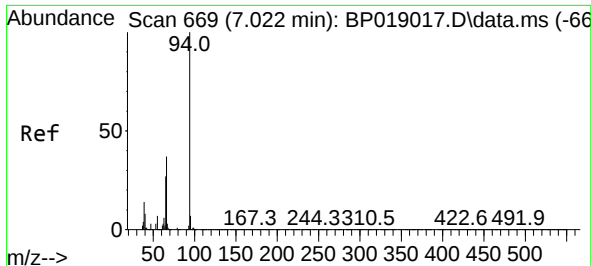

#8
Phenol
Concen: 1.210 ng/ul
RT: 7.022 min Scan# 669
Delta R.T. -0.006 min
Lab File: BP019020.D
Acq: 22 Dec 2023 03:33

Instrument :
BNA_P
ClientSampleId :
C0B23

Tgt Ion: 94 Resp: 16529
Ion Ratio Lower Upper
94 100
65 27.5 21.0 31.6
66 44.7 28.6 43.0#

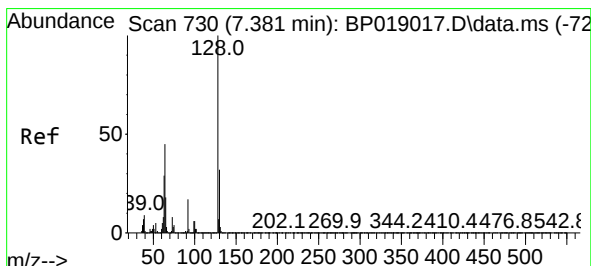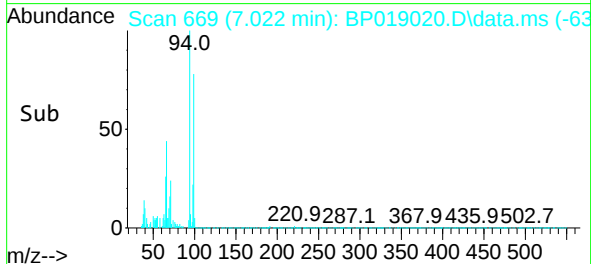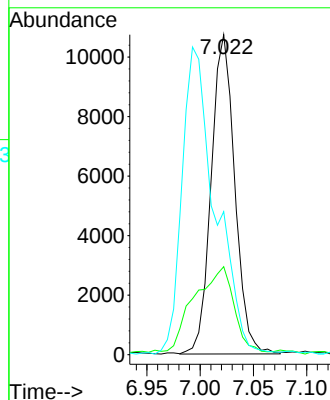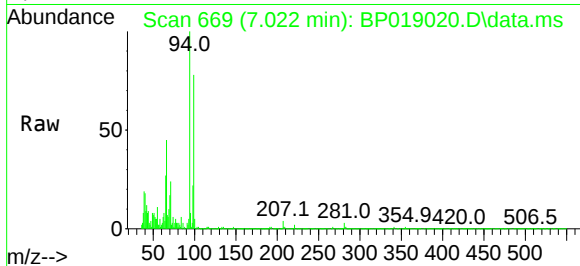

#12
2-Chlorophenol
Concen: 8.299 ng/ul
RT: 7.381 min Scan# 730
Delta R.T. -0.006 min
Lab File: BP019020.D
Acq: 22 Dec 2023 03:33

Tgt Ion: 128 Resp: 91265
Ion Ratio Lower Upper
128 100
64 45.5 37.0 55.4
130 32.7 26.8 40.2

