

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019004.D
 Acq On : 21 Dec 2023 17:57
 Operator : MA/JU
 Sample : PB157918BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK918

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	36	rVB	40563	51809	1.36%	0.162%
2	3.669	95	99	117	rBV	445981	648333	17.05%	2.027%
3	3.993	151	154	159	rVB	8906	12138	0.32%	0.038%
4	6.993	656	664	676	rBV	465352	750997	19.75%	2.348%
5	7.158	684	692	705	rVB	386377	602480	15.85%	1.884%
6	7.352	717	725	736	rBV	500931	775279	20.39%	2.424%
7	7.822	798	805	814	rBV	486987	766540	20.16%	2.397%
8	8.534	918	926	940	rBV	564103	906362	23.84%	2.834%
9	8.981	995	1002	1012	rBV	427872	702834	18.49%	2.198%
10	9.704	1117	1125	1135	rBV	346136	576869	15.17%	1.804%
11	10.240	1208	1216	1243	rBV	520556	933206	24.55%	2.918%
12	10.616	1272	1280	1288	rBV	590209	980669	25.79%	3.066%
13	10.757	1297	1304	1316	rBV	514548	895726	23.56%	2.801%
14	12.210	1545	1551	1556	rBV3	9681	17613	0.46%	0.055%
15	13.363	1740	1747	1753	rBV4	8403	15860	0.42%	0.050%
16	13.875	1827	1834	1844	rBV	925387	1348938	35.48%	4.218%
17	14.145	1874	1880	1891	rBV	1038887	1581373	41.60%	4.944%
18	14.328	1906	1911	1914	rBV7	2640	4314	0.11%	0.013%
19	14.451	1926	1932	1946	rBV	849993	1291834	33.98%	4.039%
20	14.675	1963	1970	1990	rBV	302603	631420	16.61%	1.974%
21	15.451	2095	2102	2116	rBV	1381217	2057202	54.11%	6.432%
22	15.575	2117	2123	2135	rVV	414355	607027	15.97%	1.898%
23	15.686	2139	2142	2149	rVB5	7252	11379	0.30%	0.036%
24	16.234	2230	2235	2239	rBV6	5256	8518	0.22%	0.027%
25	16.616	2294	2300	2304	rBV8	3251	7141	0.19%	0.022%
26	16.881	2340	2345	2349	rVB8	2652	5344	0.14%	0.017%
27	17.204	2393	2400	2410	rBV	1193211	1661522	43.70%	5.195%
28	17.304	2410	2417	2430	rVV	1628749	2328242	61.24%	7.280%
29	18.098	2547	2552	2559	rBV2	50878	80192	2.11%	0.251%
30	19.122	2722	2726	2734	rBV3	24082	36120	0.95%	0.113%
31	19.192	2734	2738	2742	rBV2	22889	38986	1.03%	0.122%
32	19.333	2758	2762	2766	rBV2	49563	70542	1.86%	0.221%
33	19.545	2792	2798	2805	rBV	2296302	3040919	79.99%	9.508%
34	21.298	3091	3096	3106	rBV	1726328	2234797	58.78%	6.987%
35	23.504	3465	3471	3485	rVB2	1860114	3801824	100.00%	11.887%
36	23.657	3491	3497	3509	rVB	1205011	2498785	65.73%	7.813%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019004.D
Acq On : 21 Dec 2023 17:57
Operator : MA/JU
Sample : PB157918BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK918

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 31983134

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019004.D
Acq On : 21 Dec 2023 17:57
Operator : MA/JU
Sample : PB157918BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK918

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

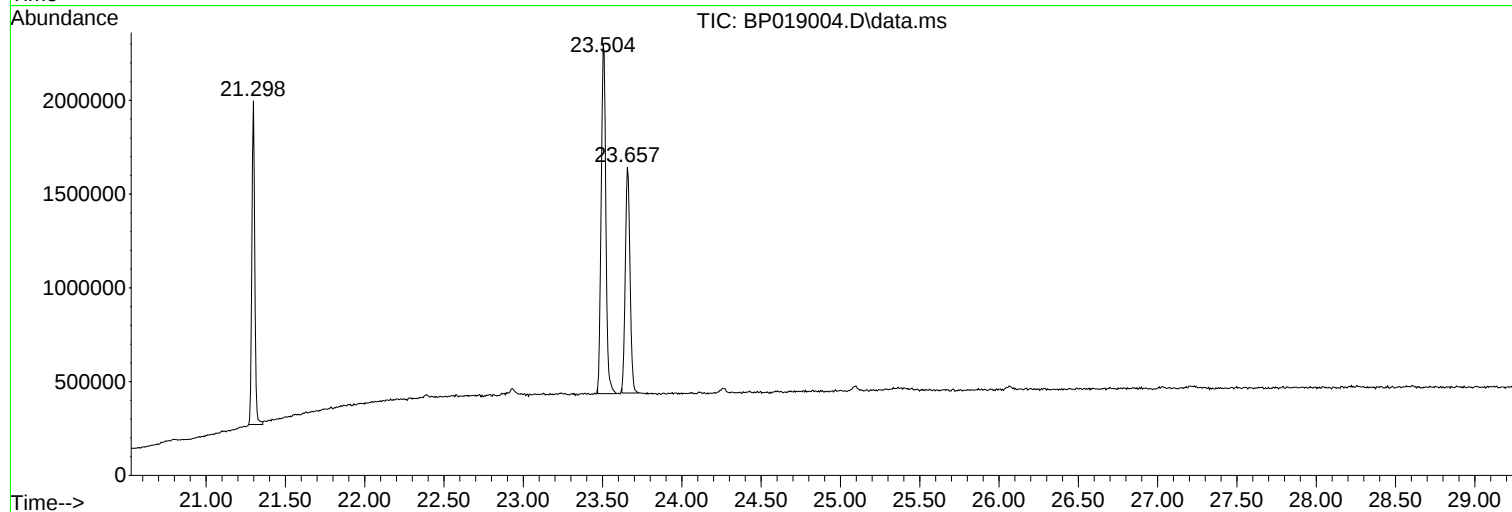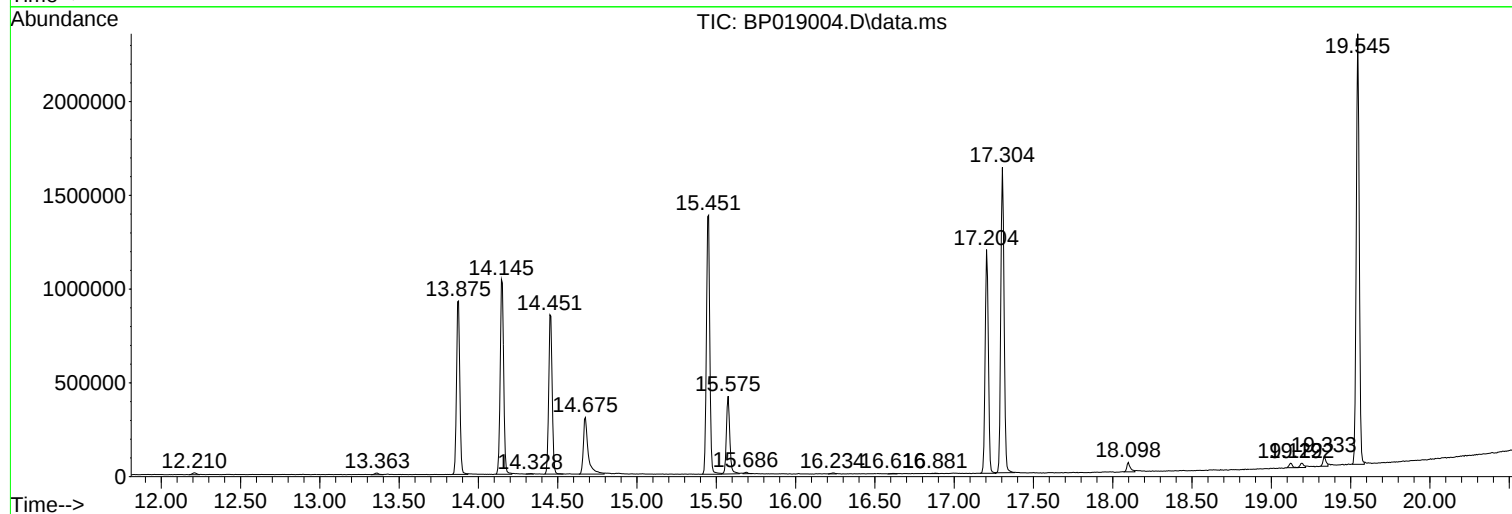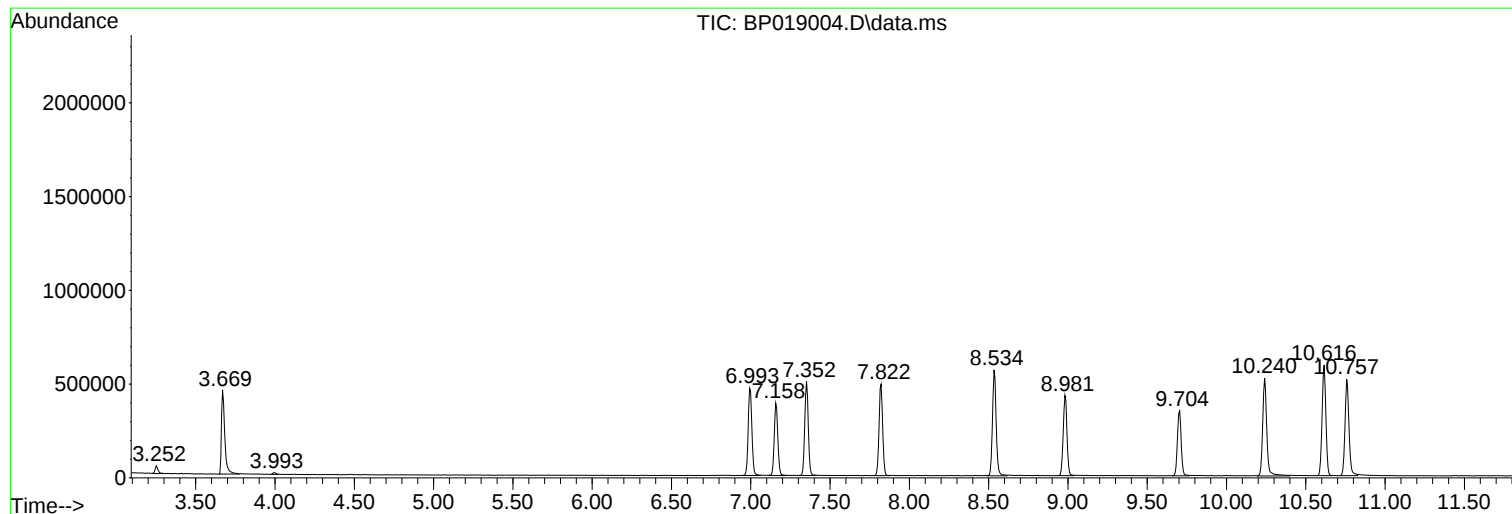

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019004.D
Acq On : 21 Dec 2023 17:57
Operator : MA/JU
Sample : PB157918BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK918

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019004.D
Acq On : 21 Dec 2023 17:57
Operator : MA/JU
Sample : PB157918BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK918

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc