

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019034.D
 Acq On : 22 Dec 2023 11:28
 Operator : MA/JU
 Sample : PB157967BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK967

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	24	27	32	rBV	42873	51307	1.16%	0.129%
2	3.669	95	99	117	rBV	530607	776711	17.51%	1.958%
3	3.993	150	154	158	rVB	11713	13124	0.30%	0.033%
4	6.993	654	664	677	rBV	595066	936927	21.12%	2.362%
5	7.158	684	692	702	rBV	469134	721925	16.28%	1.820%
6	7.346	717	724	734	rBV	590471	942547	21.25%	2.376%
7	7.816	797	804	812	rBV	596880	918956	20.72%	2.317%
8	8.269	877	881	888	rVB10	3002	5275	0.12%	0.013%
9	8.534	919	926	939	rBV	708576	1139071	25.68%	2.872%
10	8.981	993	1002	1017	rBV	514025	853871	19.25%	2.153%
11	9.557	1093	1100	1107	rBV	2377	5278	0.12%	0.013%
12	9.699	1117	1124	1132	rBV	436285	706053	15.92%	1.780%
13	9.793	1138	1140	1147	rVB7	2435	4668	0.11%	0.012%
14	10.240	1208	1216	1231	rBV	682199	1192809	26.89%	3.007%
15	10.610	1272	1279	1287	rBV	742465	1221851	27.55%	3.081%
16	10.757	1295	1304	1315	rBV	668558	1131438	25.51%	2.853%
17	12.204	1545	1550	1557	rBV2	12626	21585	0.49%	0.054%
18	12.640	1620	1624	1628	rBV7	2917	4582	0.10%	0.012%
19	13.251	1724	1728	1732	rBV5	4795	7607	0.17%	0.019%
20	13.292	1732	1735	1739	rVV2	3994	5655	0.13%	0.014%
21	13.357	1739	1746	1752	rVB4	14154	27963	0.63%	0.071%
22	13.434	1757	1759	1766	rVB8	2984	5174	0.12%	0.013%
23	13.869	1827	1833	1840	rBV	1165477	1628217	36.71%	4.105%
24	14.145	1873	1880	1894	rBV	1397063	2030861	45.78%	5.120%
25	14.451	1926	1932	1940	rBV	1103284	1699817	38.32%	4.286%
26	14.516	1940	1943	1949	rVB6	5261	8903	0.20%	0.022%
27	14.675	1962	1970	1984	rBV	420509	830352	18.72%	2.094%
28	14.851	1998	2000	2010	rVB5	6519	13847	0.31%	0.035%
29	15.086	2036	2040	2046	rBV9	3924	6981	0.16%	0.018%
30	15.281	2070	2073	2076	rBV3	4231	4600	0.10%	0.012%
31	15.445	2095	2101	2108	rBV	1756466	2579619	58.16%	6.504%
32	15.498	2108	2110	2115	rVV4	14416	22910	0.52%	0.058%
33	15.575	2116	2123	2137	rVV	498284	721726	16.27%	1.820%
34	15.686	2138	2142	2145	rVV2	11810	19553	0.44%	0.049%
35	15.716	2145	2147	2154	rVB7	5763	9063	0.20%	0.023%
36	16.016	2191	2198	2202	rBV9	2566	6115	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019034.D
 Acq On : 22 Dec 2023 11:28
 Operator : MA/JU
 Sample : PB157967BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK967

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.233	2229	2235	2239	rBV5	7025	10367	0.23%	0.026%
38	16.398	2258	2263	2270	rBV10	4375	7057	0.16%	0.018%
39	16.504	2276	2281	2286	rBV9	5217	7580	0.17%	0.019%
40	16.681	2307	2311	2315	rBV7	3828	5876	0.13%	0.015%
41	16.986	2360	2363	2367	rBV4	4221	7134	0.16%	0.018%
42	17.204	2394	2400	2411	rBV	1574958	2185232	49.26%	5.510%
43	17.304	2411	2417	2433	rVV	2089143	2960721	66.75%	7.465%
44	17.622	2467	2471	2479	rBV3	4553	9114	0.21%	0.023%
45	18.098	2549	2552	2558	rBV7	12440	18868	0.43%	0.048%
46	18.169	2561	2564	2568	rVB3	6925	10409	0.23%	0.026%
47	19.122	2722	2726	2732	rBV	32519	42916	0.97%	0.108%
48	19.192	2734	2738	2741	rBV	26918	36870	0.83%	0.093%
49	19.545	2792	2798	2807	rBV	2808951	3801286	85.70%	9.584%
50	21.298	3091	3096	3105	rBV	2158260	2834776	63.91%	7.147%
51	23.510	3465	3472	3487	rVB2	2160067	4435743	100.00%	11.184%
52	23.657	3491	3497	3508	rVB	1501937	3011302	67.89%	7.592%




Sum of corrected areas: 39662192

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019034.D
Acq On : 22 Dec 2023 11:28
Operator : MA/JU
Sample : PB157967BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

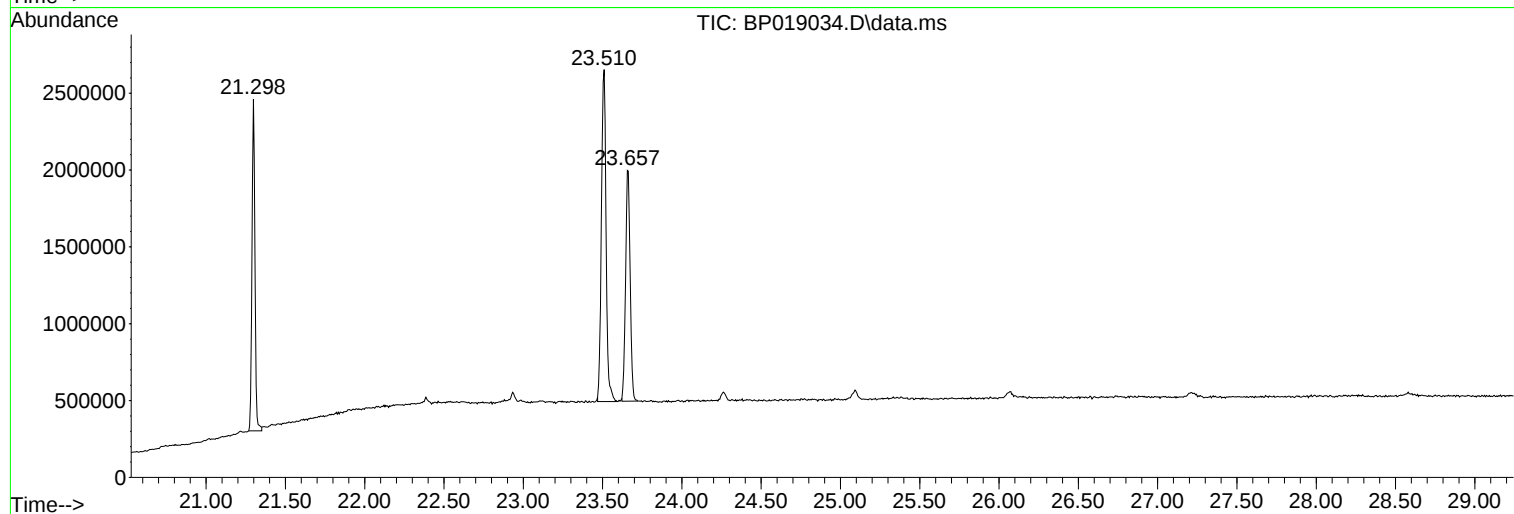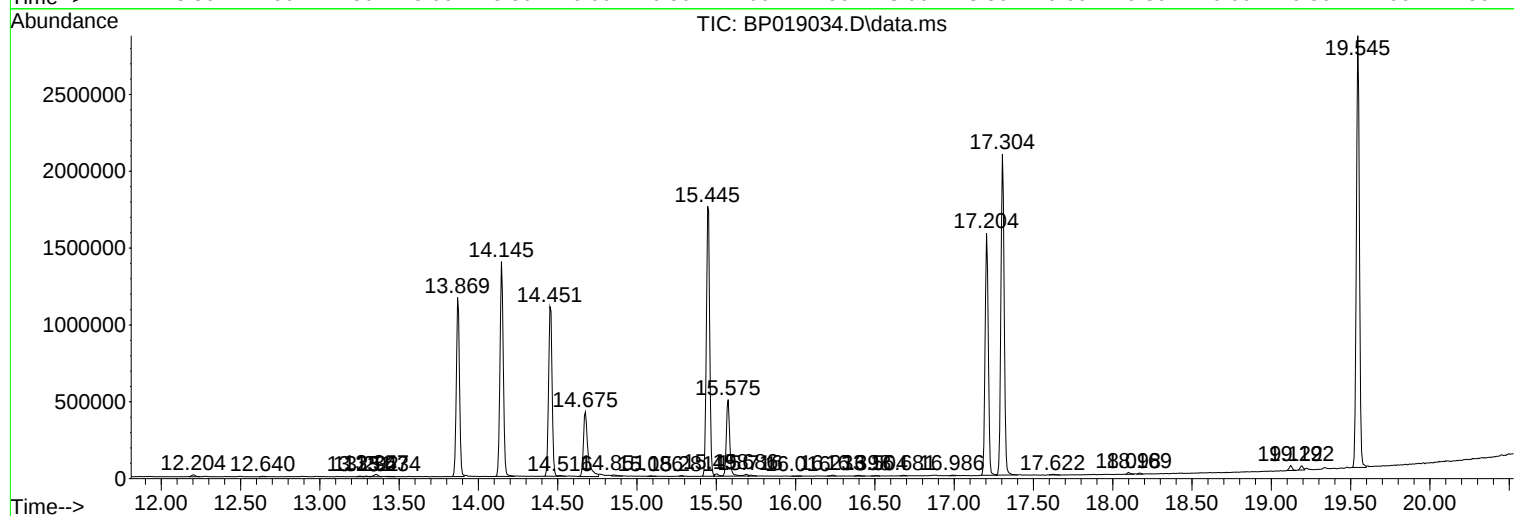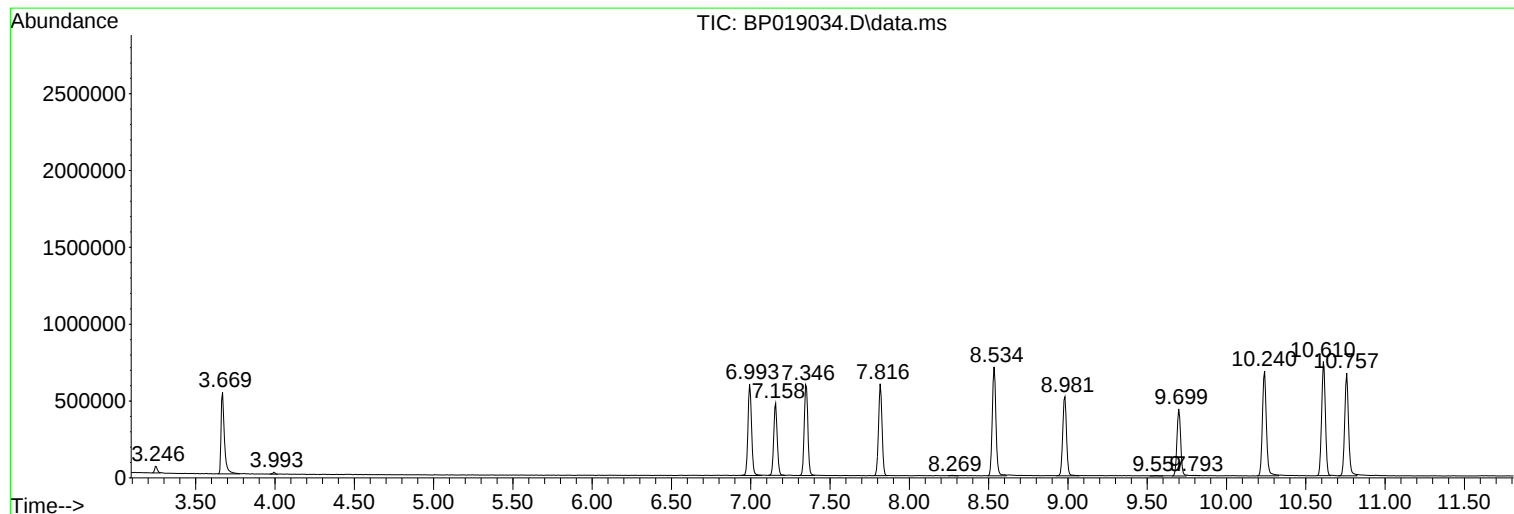

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019034.D
Acq On : 22 Dec 2023 11:28
Operator : MA/JU
Sample : PB157967BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019034.D
Acq On : 22 Dec 2023 11:28
Operator : MA/JU
Sample : PB157967BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------