

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019039.D
 Acq On : 22 Dec 2023 14:18
 Operator : MA/JU
 Sample : 05808-09DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B03DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	33	rVB2	9058	12108	0.42%	0.058%
2	3.540	75	77	83	rBV	11385	15640	0.55%	0.075%
3	3.681	97	101	112	rBV	50028	79660	2.78%	0.382%
4	3.993	151	154	158	rVB	12475	13840	0.48%	0.066%
5	4.781	284	288	291	rBV6	2218	3547	0.12%	0.017%
6	6.993	658	664	676	rVB	109994	182050	6.35%	0.873%
7	7.158	685	692	699	rBV	93242	141659	4.94%	0.680%
8	7.352	719	725	734	rVB	113413	179137	6.25%	0.859%
9	7.816	797	804	814	rBV	553782	876529	30.60%	4.205%
10	8.534	916	926	940	rBV	126416	223953	7.82%	1.074%
11	8.981	995	1002	1010	rBV	99343	165075	5.76%	0.792%
12	9.393	1068	1072	1077	rVB7	1888	3509	0.12%	0.017%
13	9.558	1094	1100	1104	rBV5	5981	11096	0.39%	0.053%
14	9.699	1118	1124	1132	rBV	71533	123292	4.30%	0.591%
15	10.240	1210	1216	1231	rBV	116338	220996	7.71%	1.060%
16	10.475	1249	1256	1264	rBV	475689	763403	26.65%	3.662%
17	10.610	1270	1279	1288	rBV	703078	1170498	40.86%	5.615%
18	10.763	1297	1305	1321	rBV	99690	203499	7.10%	0.976%
19	10.999	1337	1345	1353	rBV	245610	409934	14.31%	1.967%
20	11.369	1402	1408	1414	rBV5	6252	13614	0.48%	0.065%
21	11.899	1494	1498	1504	rVB9	2787	5420	0.19%	0.026%
22	12.181	1538	1546	1554	rBV10	4892	12932	0.45%	0.062%
23	12.357	1568	1576	1579	rBV6	5622	9414	0.33%	0.045%
24	12.610	1612	1619	1621	rBV	76022	120036	4.19%	0.576%
25	12.640	1621	1624	1630	rVV	142909	224153	7.82%	1.075%
26	12.704	1634	1635	1641	rVB6	2944	4782	0.17%	0.023%
27	13.251	1720	1728	1741	rBV	1180382	1810625	63.20%	8.686%
28	13.357	1741	1746	1751	rVB2	15274	25331	0.88%	0.122%
29	13.869	1825	1833	1843	rBV	232617	340994	11.90%	1.636%
30	14.146	1873	1880	1894	rBV2	266989	402866	14.06%	1.933%
31	14.263	1894	1900	1908	rVB2	4101	10017	0.35%	0.048%
32	14.451	1924	1932	1940	rBV	1088340	1636794	57.13%	7.852%
33	14.604	1954	1958	1964	rVB9	2053	3982	0.14%	0.019%
34	14.687	1964	1972	1980	rBV3	45851	114066	3.98%	0.547%
35	14.769	1980	1986	1999	rVB	266410	405377	14.15%	1.945%
36	14.887	2004	2006	2011	rVB6	2982	4170	0.15%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
 Data File : BP019039.D
 Acq On : 22 Dec 2023 14:18
 Operator : MA/JU
 Sample : 05808-09DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B03DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.445	2093	2101	2116	rBV	380495	566404	19.77%	2.717%
38	15.575	2117	2123	2132	rBV	65649	103620	3.62%	0.497%
39	16.222	2229	2233	2240	rVB9	6597	13226	0.46%	0.063%
40	16.504	2275	2281	2286	rBV5	8838	15132	0.53%	0.073%
41	16.616	2294	2300	2305	rBV8	3101	5781	0.20%	0.028%
42	16.992	2361	2364	2368	rBV4	3640	5594	0.20%	0.027%
43	17.204	2392	2400	2410	rBV	1494587	2128718	74.30%	10.212%
44	17.304	2411	2417	2429	rVB	425975	611169	21.33%	2.932%
45	17.604	2465	2468	2473	rBV7	3078	5718	0.20%	0.027%
46	17.881	2513	2515	2520	rVB6	4445	4730	0.17%	0.023%
47	18.098	2542	2552	2558	rBV2	73643	115456	4.03%	0.554%
48	19.334	2758	2762	2767	rBV3	30376	44521	1.55%	0.214%
49	19.545	2792	2798	2805	rBV	604792	818155	28.56%	3.925%
50	21.298	3091	3096	3106	rBV	2139799	2701342	94.29%	12.959%
51	23.504	3466	3471	3484	rVB2	430866	896702	31.30%	4.302%
52	23.657	3491	3497	3510	rVB	1430281	2864854	100.00%	13.744%




Sum of corrected areas: 20845120

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019039.D
Acq On : 22 Dec 2023 14:18
Operator : MA/JU
Sample : 05808-09DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

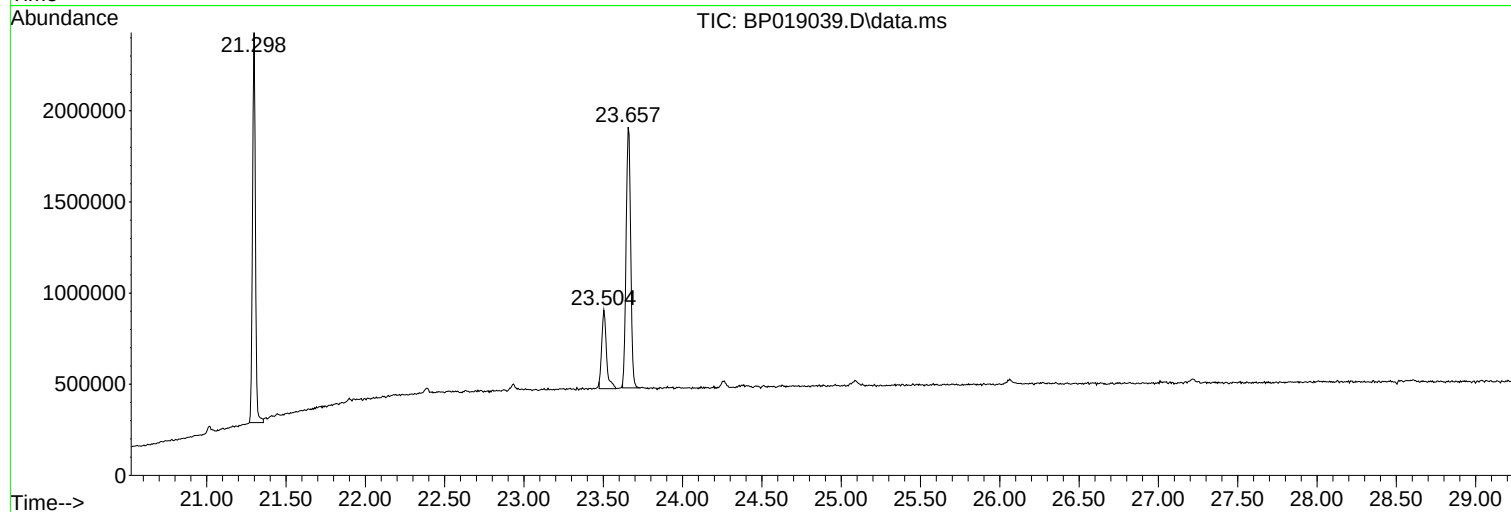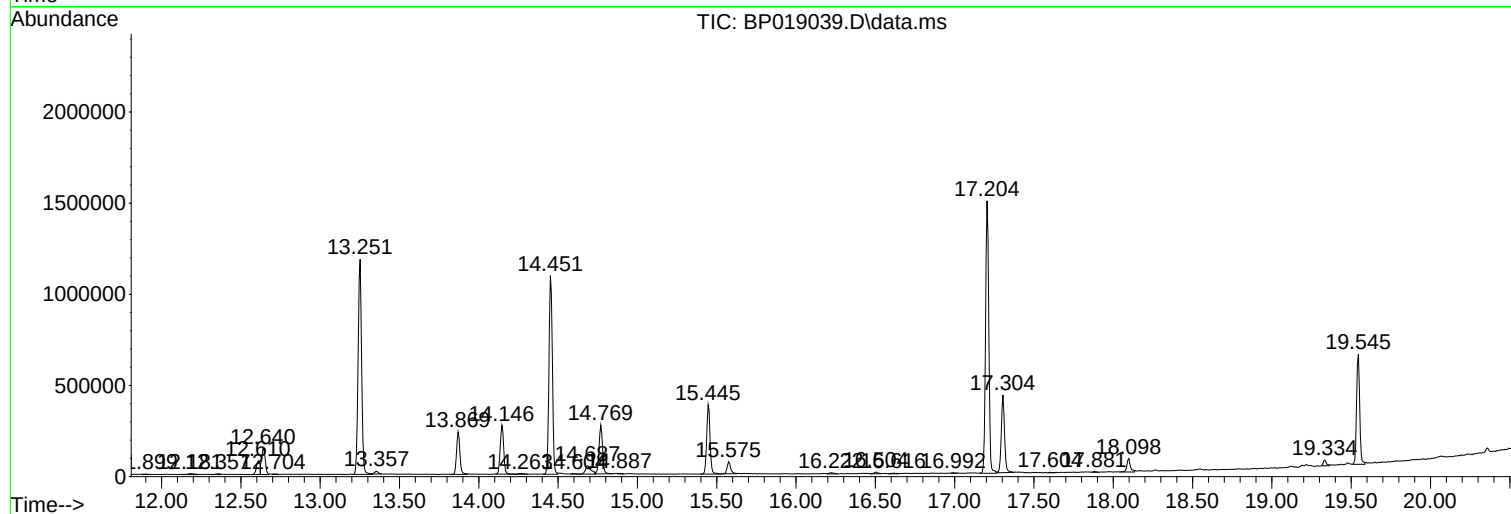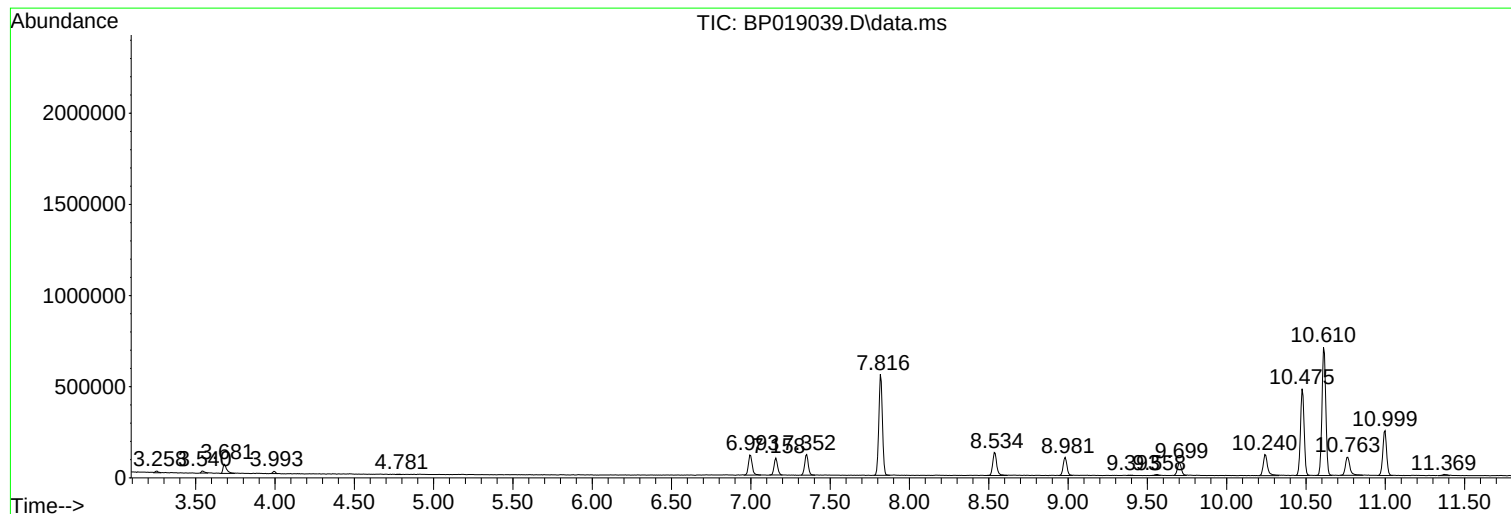

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019039.D
Acq On : 22 Dec 2023 14:18
Operator : MA/JU
Sample : 05808-09DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122123\
Data File : BP019039.D
Acq On : 22 Dec 2023 14:18
Operator : MA/JU
Sample : 05808-09DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B03DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc