

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013279.D
 Acq On : 23 Dec 2022 14:52
 Operator : CG/JU
 Sample : N6018-09
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYH9

Quant Time: Dec 24 00:25:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	640020	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	2685711	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	1598538	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	2869843	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	2288568	20.000	ng/ul	0.00
88) Perylene-d12	23.927	264	2707889	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	57009	3.808	ng/uL	0.00
4) Pyridine-d5	3.764	84	852304	20.044	ng/ul	0.00
7) Phenol-d5	7.105	99	1186944	22.768	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	743734	23.650	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	977430	23.818	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	899904	21.068	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	482009	24.427	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	550798	24.794	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	1013060	23.478	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131	1085620	17.822	ng/ul	0.00
46) Dimethylphthalate-d6	13.992	166	2885672	23.488	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	3302228	24.462	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	316168	14.307	ng/ul	0.00
60) Fluorene-d10	15.581	176	2382632	22.924	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	255069	13.811	ng/ul	0.00
73) Anthracene-d10	17.445	188	3132301	24.193	ng/ul	0.00
81) Pyrene-d10	19.680	212	3146654	23.954	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.762	264	3237123	23.984	ng/ul	0.00


Target Compounds					Qvalue
10) Bis(2-Chloroethyl)ether	7.375	93	115826	2.677 ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP12222\
Data File : BP013279.D
Acq On : 23 Dec 2022 14:52
Operator : CG/JU
Sample : N6018-09
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYH9

Quant Time: Dec 24 00:25:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

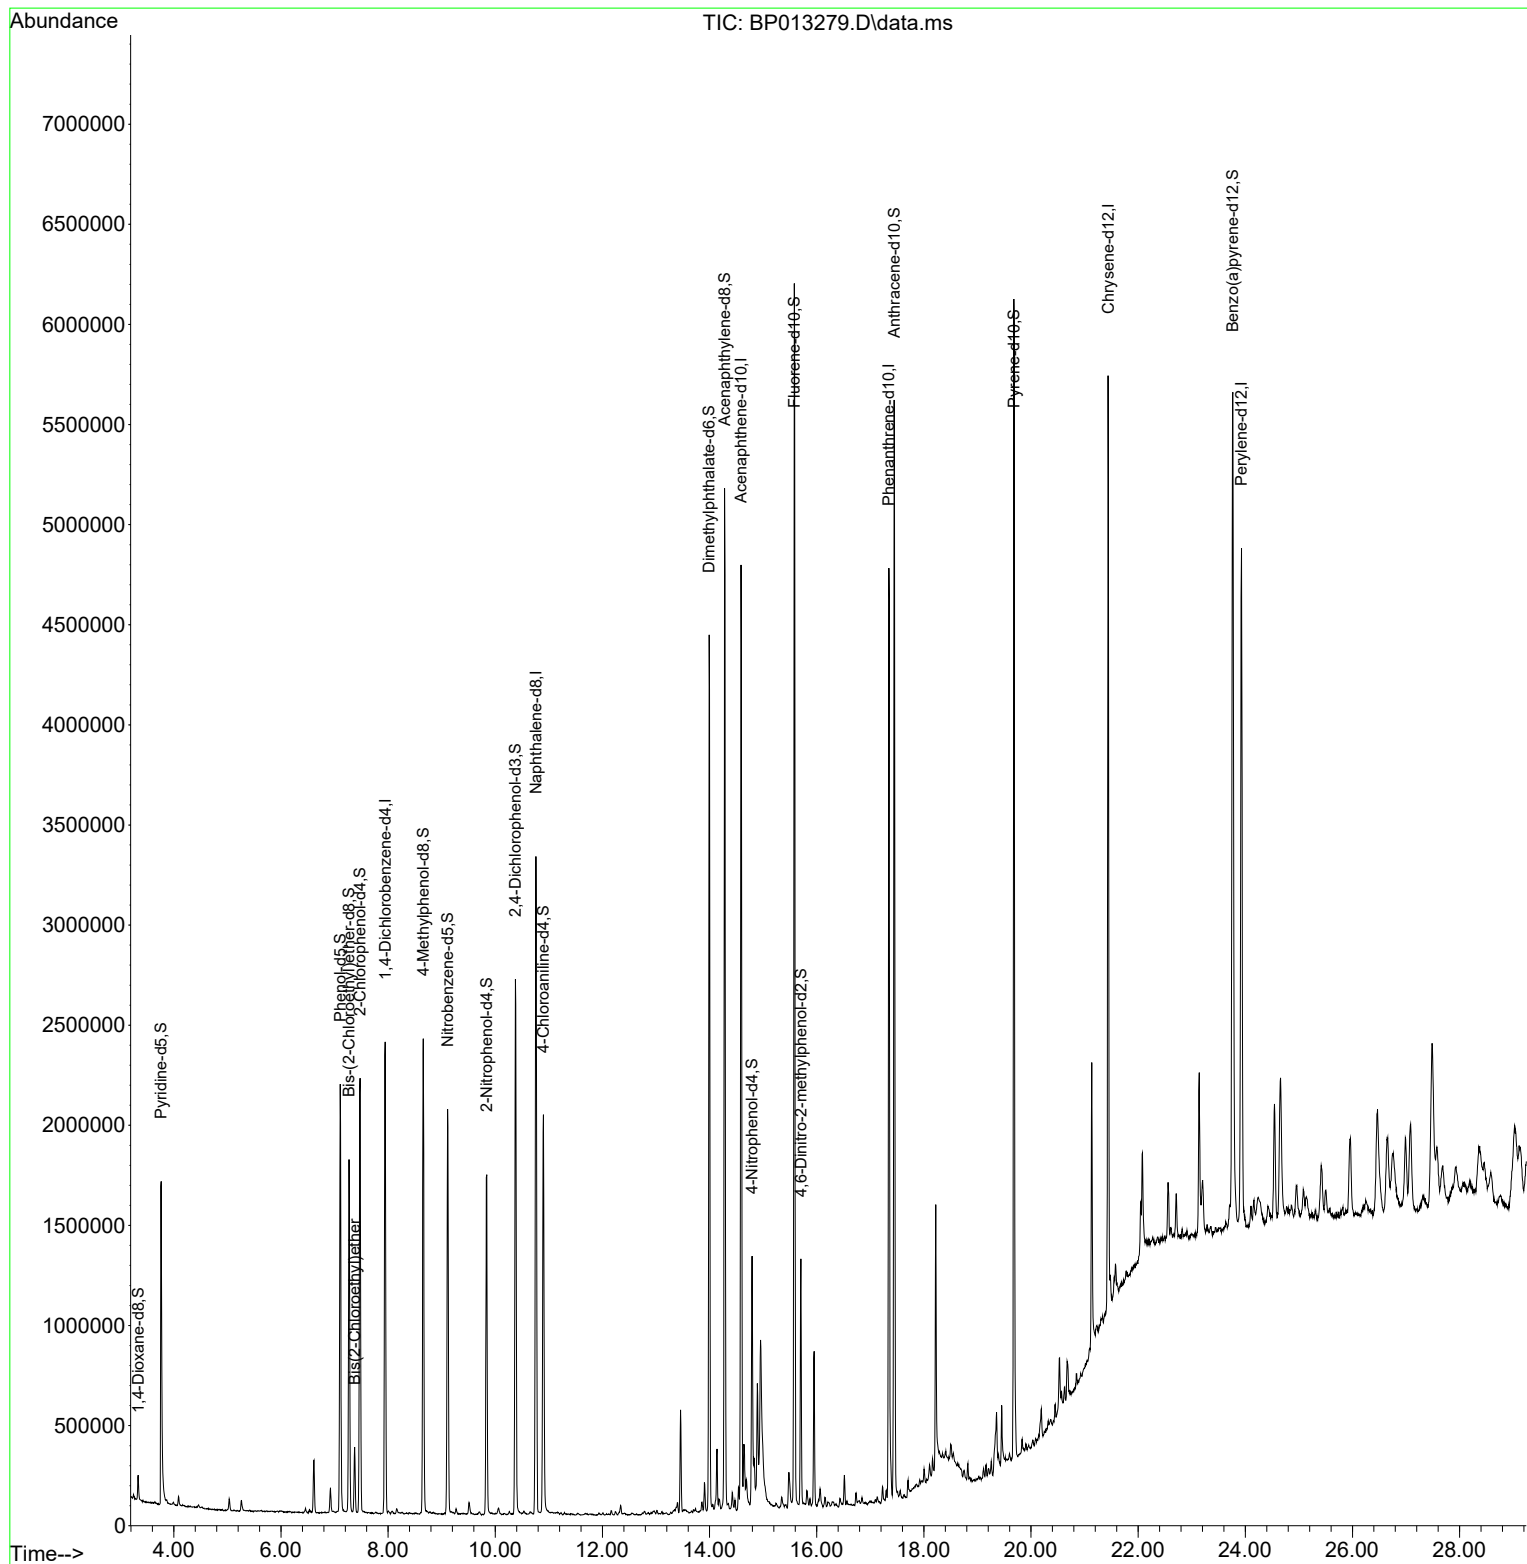

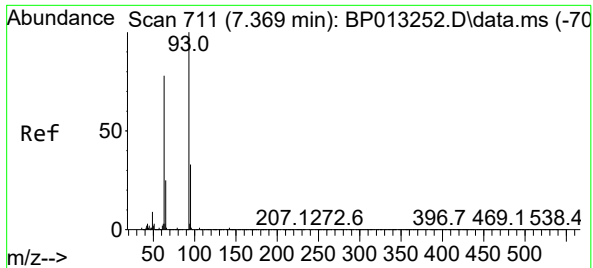

#10
 Bis(2-Chloroethyl)ether
 Concen: 2.677 ng/ul
 RT: 7.375 min Scan# 71
 Delta R.T. 0.012 min
 Lab File: BP013279.D
 Acq: 23 Dec 2022 14:52

Instrument :
 BNA_P
 ClientSampleId :
 DBYH9

Tgt Ion: 93	Resp: 115826
Ion Ratio	Lower Upper
93 100	
63 2.1	59.8 89.8#
95 2.5	26.4 39.6#

