

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013283.D
 Acq On : 23 Dec 2022 17:09
 Operator : CG/JU
 Sample : N6018-18
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYK3

Quant Time: Dec 24 00:26:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	622965	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	2269678	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	1131713	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	2267514	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	2594993	20.000	ng/ul	0.00
88) Perylene-d12	23.927	264	3026115	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	51619	3.543	ng/uL	0.00
4) Pyridine-d5	3.764	84	419572	10.137	ng/ul	0.00
7) Phenol-d5	7.105	99	974624	19.207	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	643959	21.038	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	823548	20.617	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	711994	17.125	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	383200	22.979	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	420195	22.382	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	756008	20.732	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	676535	13.142	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	1877852	21.590	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	2213612	23.161	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	193615	12.375	ng/ul	0.00
60) Fluorene-d10	15.581	176	1597614	21.712	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	146187	10.018	ng/ul	0.00
73) Anthracene-d10	17.445	188	2424549	23.701	ng/ul	0.00
81) Pyrene-d10	19.681	212	3203850	21.509	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.763	264	3482413	23.088	ng/ul	0.00


Target Compounds					Qvalue
10) Bis(2-Chloroethyl)ether	7.375	93	267113	6.343 ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013283.D
Acq On : 23 Dec 2022 17:09
Operator : CG/JU
Sample : N6018-18
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYK3


Quant Time: Dec 24 00:26:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

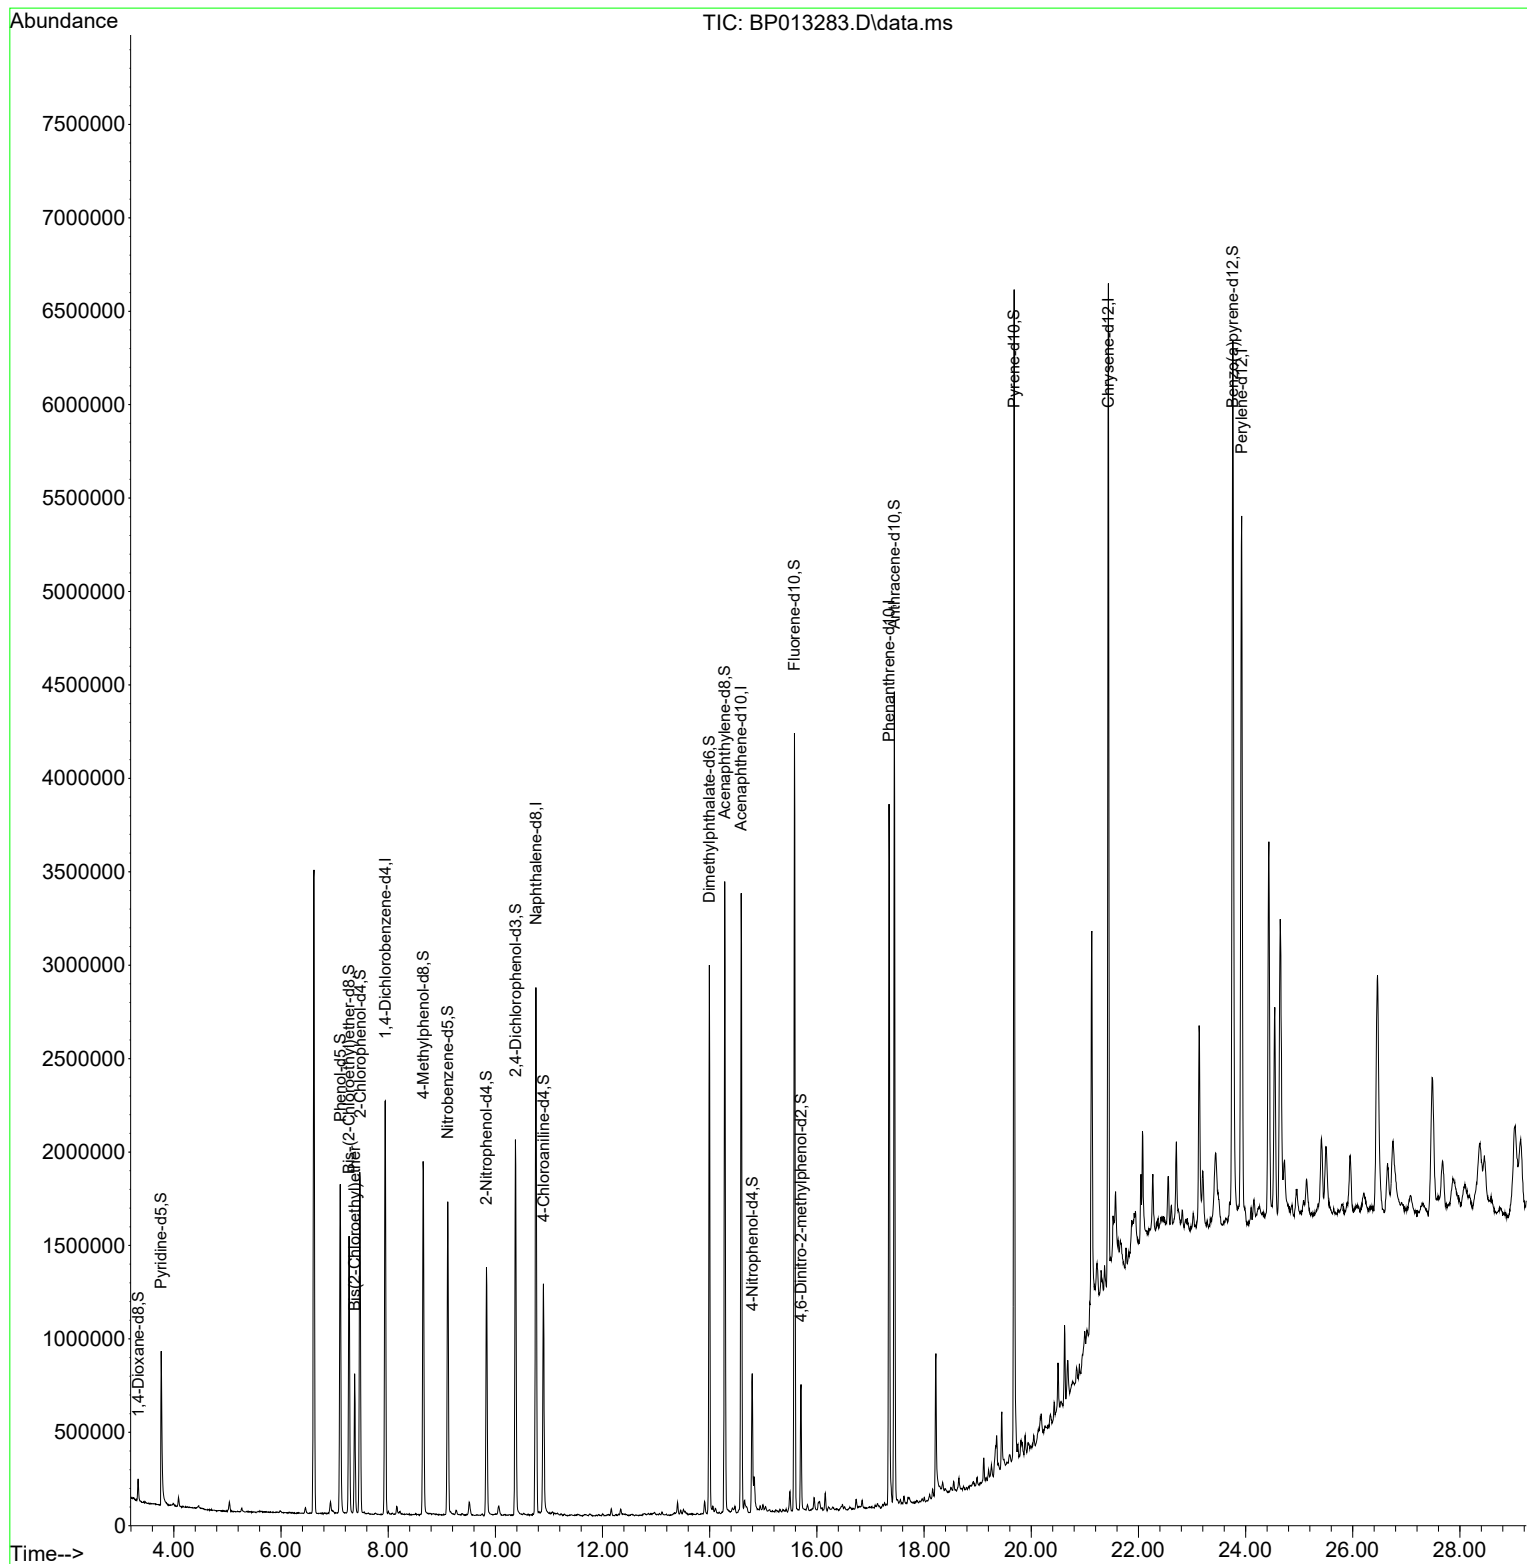

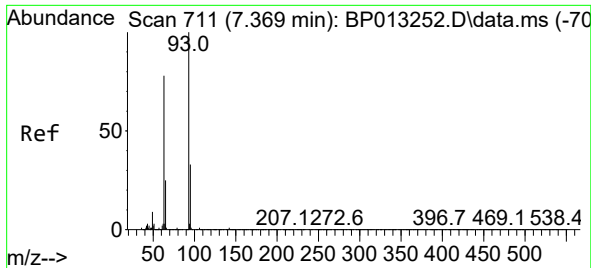

#10
 Bis(2-Chloroethyl)ether
 Concen: 6.343 ng/ul
 RT: 7.375 min Scan# 71
 Delta R.T. 0.012 min
 Lab File: BP013283.D
 Acq: 23 Dec 2022 17:09

Instrument :
 BNA_P
 ClientSampleId :
 DBYK3

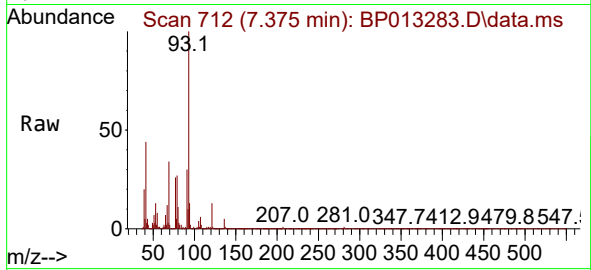

Tgt Ion: 93 Resp: 267113

Ion	Ratio	Lower	Upper
93	100		
63	2.1	59.8	89.8#
95	2.2	26.4	39.6#

