

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013285.D
 Acq On : 23 Dec 2022 18:18
 Operator : CG/JU
 Sample : N6018-10
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYJ0

Quant Time: Dec 24 00:26:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	657690	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	2662570	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	1475422	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	2611704	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	2568335	20.000	ng/ul	0.00
88) Perylene-d12	23.927	264	3029816	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	53468	3.476	ng/uL	0.00
4) Pyridine-d5	3.764	84	735920	16.842	ng/ul	0.00
7) Phenol-d5	7.105	99	1019835	19.037	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	682681	21.125	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	876707	20.789	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	726997	16.563	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	446401	22.819	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	509945	23.154	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	902924	21.107	ng/ul	0.00
31) 4-Chloroaniline-d4	10.893	131	1074926	17.799	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	2538174	22.384	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	2844848	22.832	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	269773	13.226	ng/ul	0.00
60) Fluorene-d10	15.581	176	2098759	21.878	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	191690	11.405	ng/ul	0.00
73) Anthracene-d10	17.445	188	2669841	22.659	ng/ul	0.00
81) Pyrene-d10	19.680	212	3172816	21.522	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.763	264	3455669	22.882	ng/ul	0.00


Target Compounds					Qvalue
6) Benzaldehyde	7.081	77	55221	2.633	ng/ul 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013285.D
Acq On : 23 Dec 2022 18:18
Operator : CG/JU
Sample : N6018-10
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYJ0

Quant Time: Dec 24 00:26:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

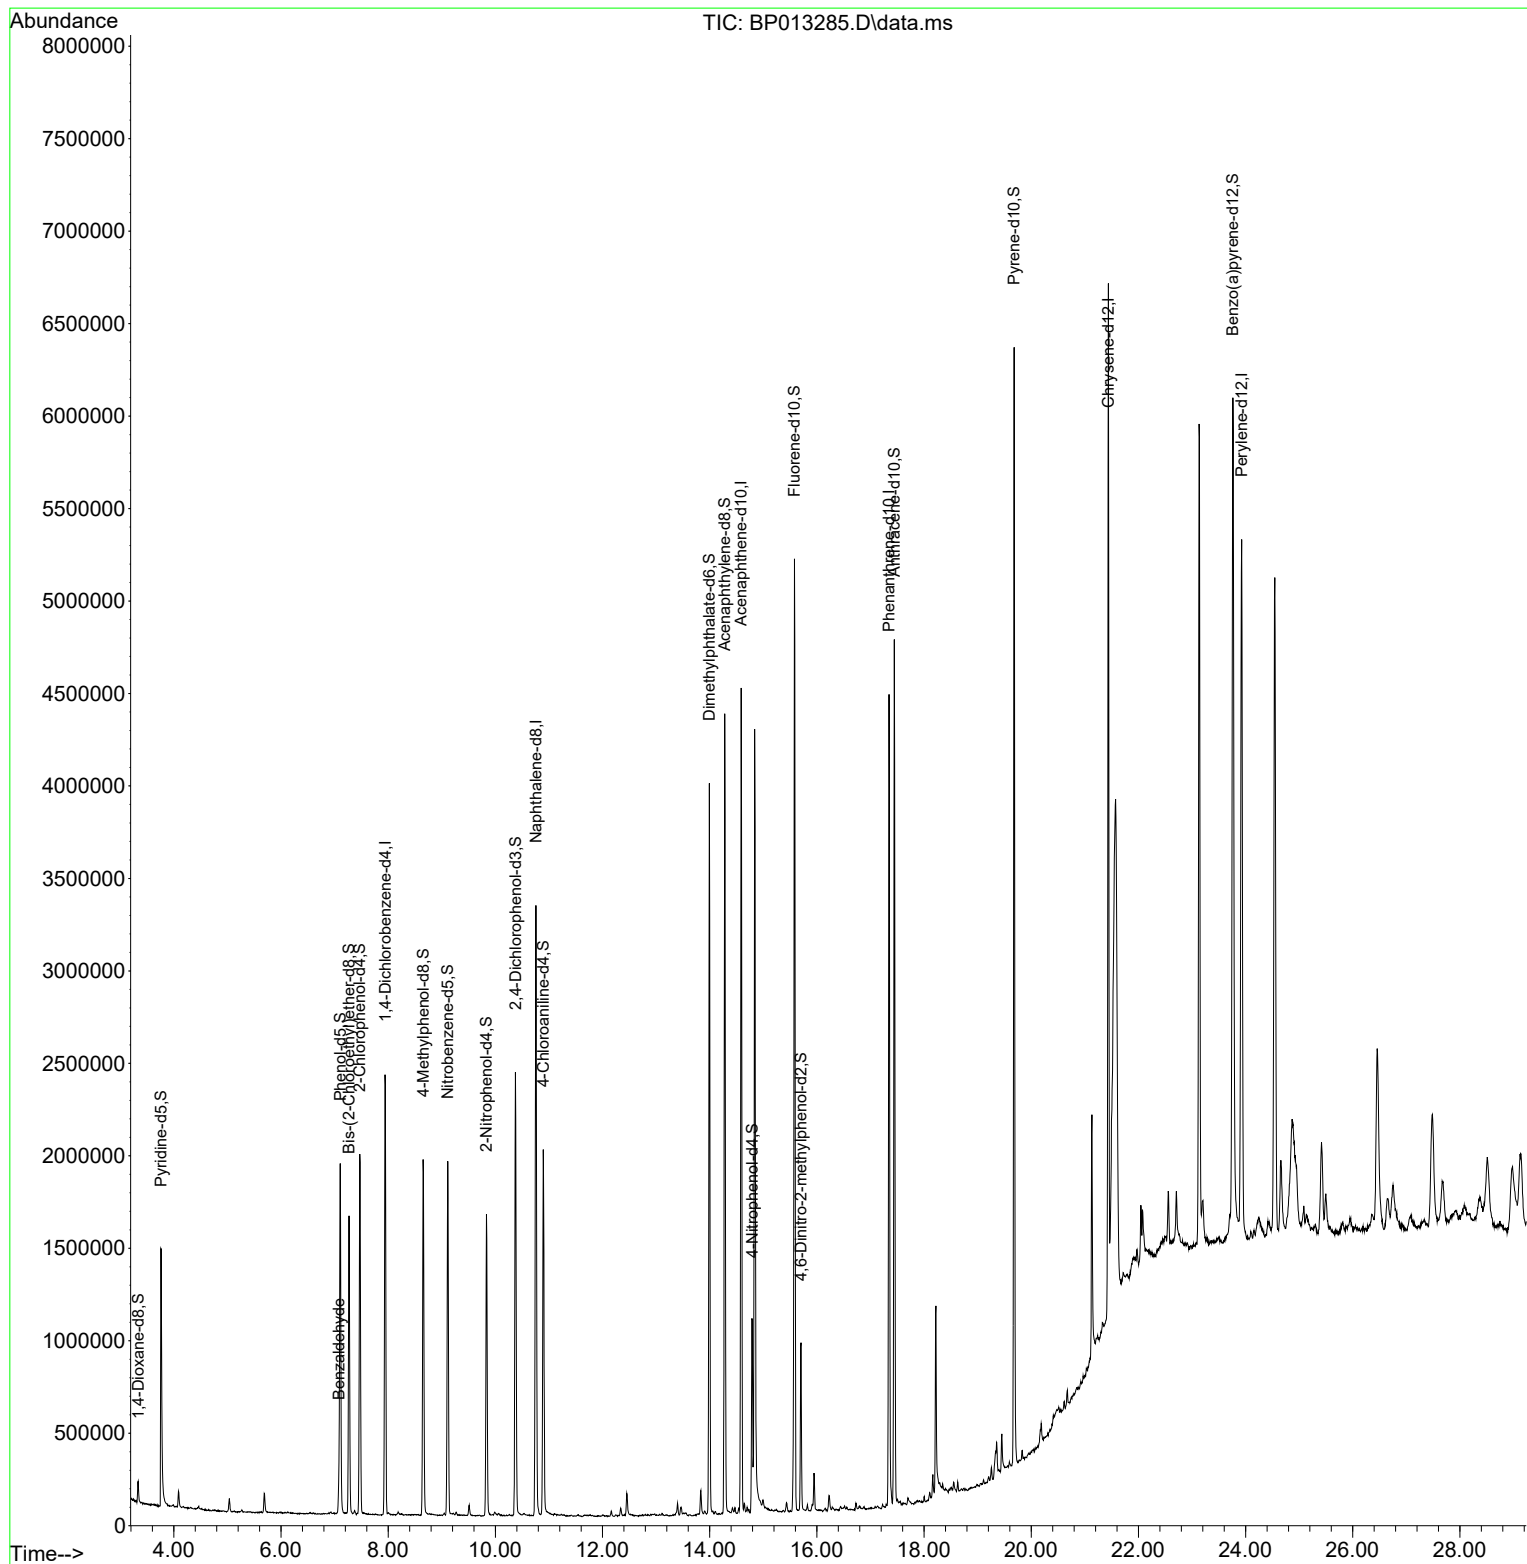

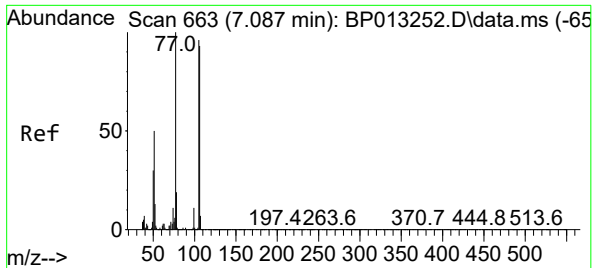

#6
Benzaldehyde
Concen: 2.633 ng/ul
RT: 7.081 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP013285.D
Acq: 23 Dec 2022 18:18

Instrument :
BNA_P
ClientSampleId :
DBYJ0

Tgt Ion: 77	Resp: 55221
Ion Ratio	Lower Upper
77	100
105	94.1 81.5 122.3
106	91.8 76.9 115.3

