

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013288.D
 Acq On : 23 Dec 2022 20:00
 Operator : CG/JU
 Sample : N6018-13
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBYJ3

Quant Time: Dec 24 00:27:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 24 00:19:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	561064	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	2023681	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.587	164	1030225	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.345	188	2194176	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	2500458	20.000	ng/ul	0.00
88) Perylene-d12	23.927	264	2912022	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	64081	4.883	ng/uL	0.00
4) Pyridine-d5	3.764	84	806834	21.645	ng/ul	0.00
7) Phenol-d5	7.105	99	1084899	23.740	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	704702	25.562	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	908769	25.261	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	775751	20.717	ng/ul	0.00
21) Nitrobenzene-d5	9.110	128	422599	28.422	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143	467263	27.914	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	820283	25.229	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	900772	19.625	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	2102262	26.551	ng/ul	0.00
49) Acenaphthylene-d8	14.281	160	2460180	28.277	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	286672	20.128	ng/ul	0.00
60) Fluorene-d10	15.581	176	1783346	26.623	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	175800	12.450	ng/ul	0.00
73) Anthracene-d10	17.445	188	2730483	27.584	ng/ul	0.00
81) Pyrene-d10	19.680	212	3746831	26.106	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.763	264	4038586	27.824	ng/ul	0.00


Target Compounds					Qvalue
10) Bis(2-Chloroethyl)ether	7.375	93	65235	1.720 ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013288.D
Acq On : 23 Dec 2022 20:00
Operator : CG/JU
Sample : N6018-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBYJ3

Quant Time: Dec 24 00:27:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 24 00:19:17 2022
Response via : Initial Calibration

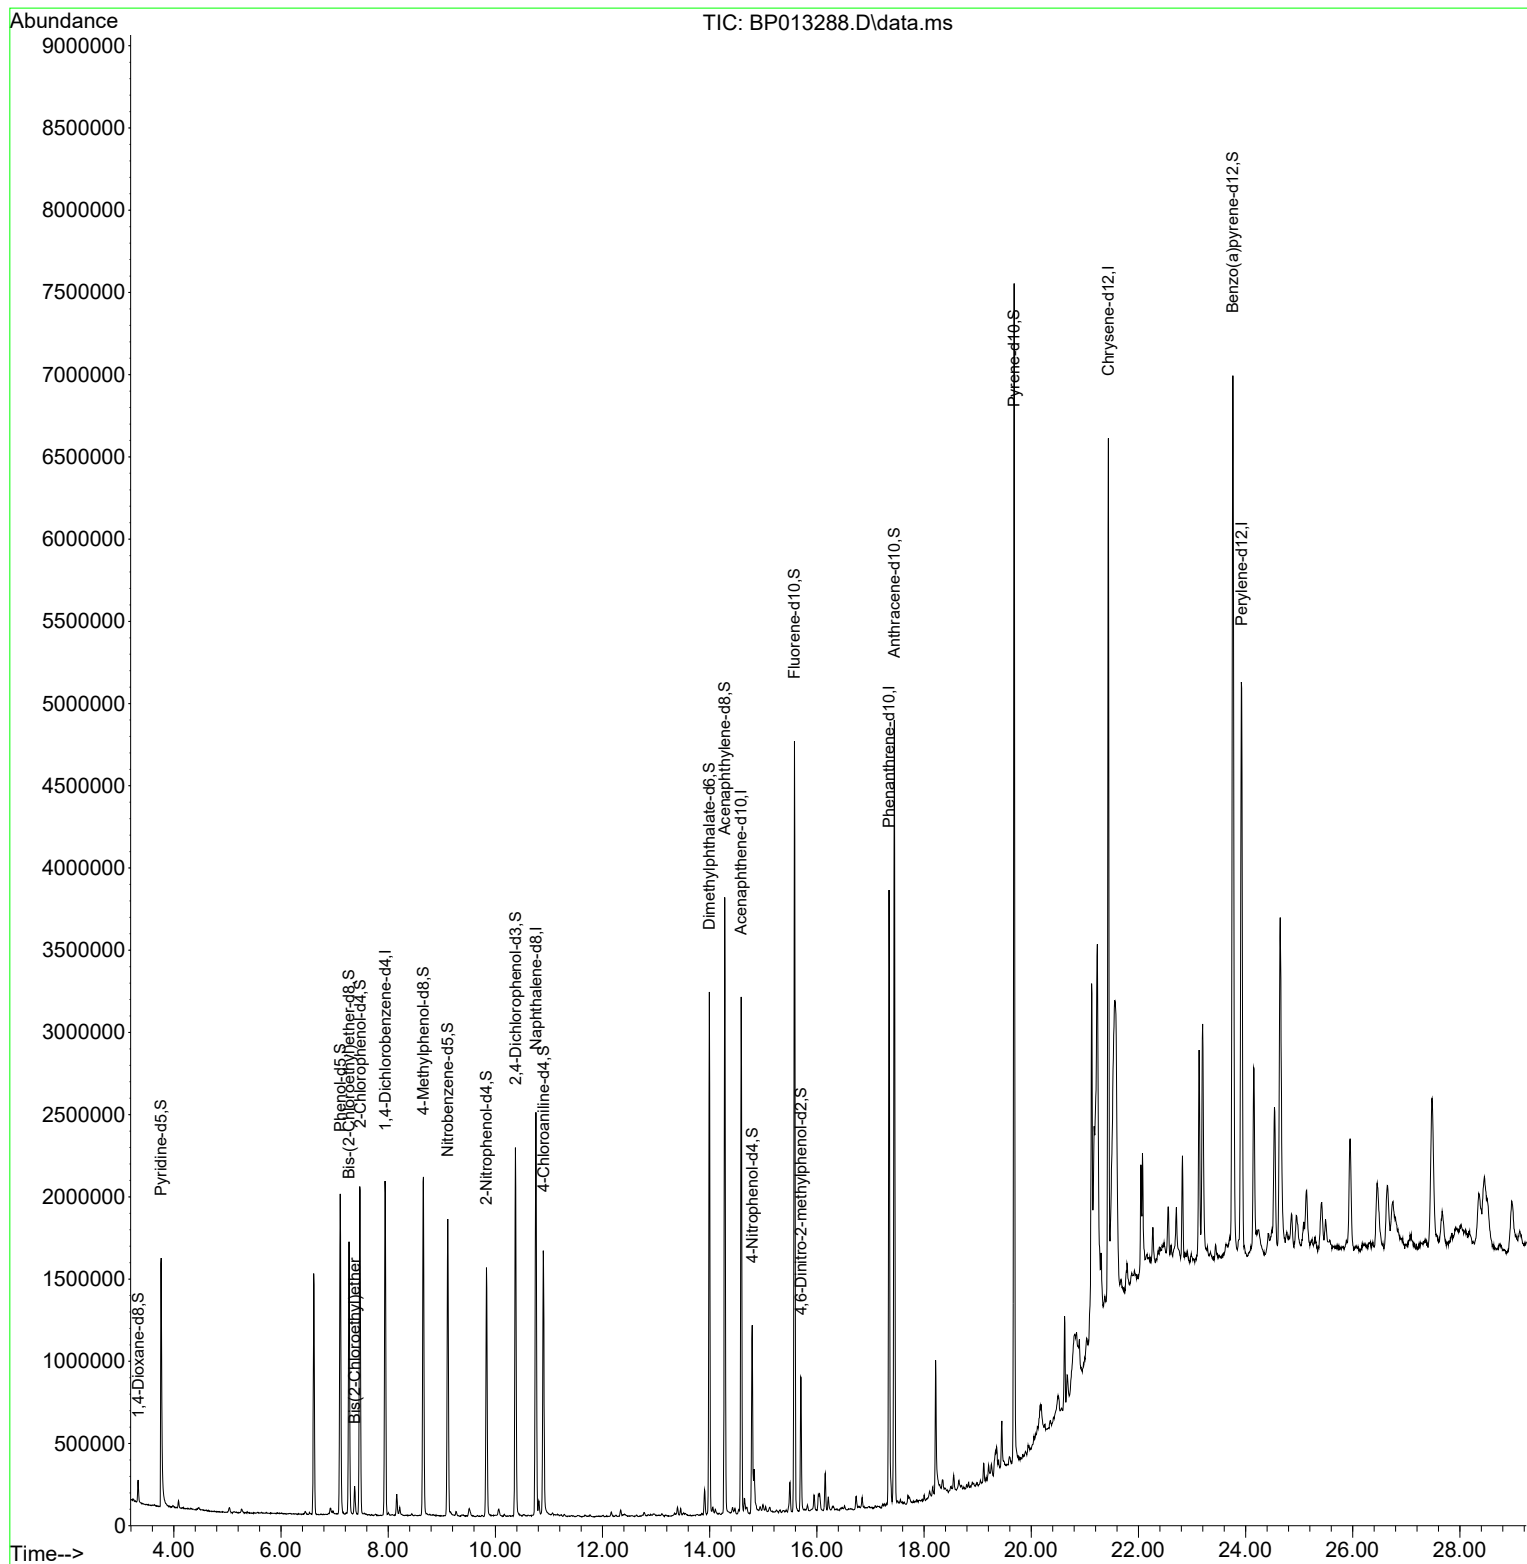

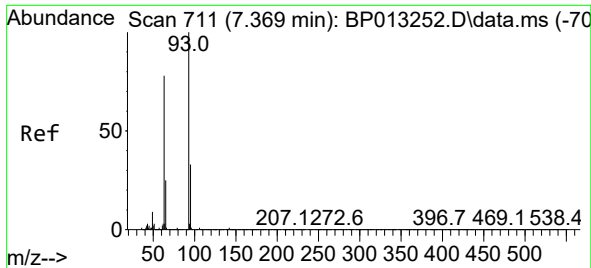

#10
 Bis(2-Chloroethyl)ether
 Concen: 1.720 ng/ul
 RT: 7.375 min Scan# 71
 Delta R.T. 0.012 min
 Lab File: BP013288.D
 Acq: 23 Dec 2022 20:00

Instrument :
 BNA_P
 ClientSampleId :
 DBYJ3

Tgt Ion: 93	Resp:	65235
Ion	Ratio	Lower Upper
93	100	
63	2.3	59.8 89.8#
95	2.6	26.4 39.6#

