

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013258.D
 Acq On : 22 Dec 2022 23:00
 Operator : CG/JU
 Sample : N6015-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXZ8

Quant Time: Dec 23 03:11:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 22 22:43:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	629447	20.000	ng/u1	0.00
20) Naphthalene-d8	10.763	136	2545439	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.586	164	1517161	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.345	188	2834601	20.000	ng/u1	-0.01
79) Chrysene-d12	21.433	240	2341785	20.000	ng/u1	0.00
88) Perylene-d12	23.909	264	2816860	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.334	96	112348	7.632	ng/uL	0.00
4) Pyridine-d5	3.758	84	1208639	28.901	ng/u1	0.00
7) Phenol-d5	7.110	99	2169286	42.311	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	1366106	44.171	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	1788870	44.323	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	1325274	31.547	ng/u1	-0.01
21) Nitrobenzene-d5	9.116	128	918077	49.090	ng/u1	0.00
24) 2-Nitrophenol-d4	9.840	143	1057482	50.225	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	1848487	45.200	ng/u1	0.00
31) 4-Chloroaniline-d4	10.898	131	1461778	25.319	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	5347491	45.862	ng/u1	0.00
49) Acenaphthylene-d8	14.286	160	6172600	48.177	ng/u1	0.00
54) 4-Nitrophenol-d4	14.792	143	651808	31.077	ng/u1	0.00
60) Fluorene-d10	15.586	176	4467230	45.286	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	656786	36.005	ng/u1	0.00
73) Anthracene-d10	17.445	188	6019258	47.069	ng/u1	-0.01
81) Pyrene-d10	19.680	212	6328631	47.082	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.757	264	6608602	47.069	ng/u1	0.00
Target Compounds						
					Qvalue	
90) Benzo(b)fluoranthene	23.151	252	200440	1.116	ng/u1#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013258.D
Acq On : 22 Dec 2022 23:00
Operator : CG/JU
Sample : N6015-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXZ8

Quant Time: Dec 23 03:11:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 22 22:43:06 2022
Response via : Initial Calibration

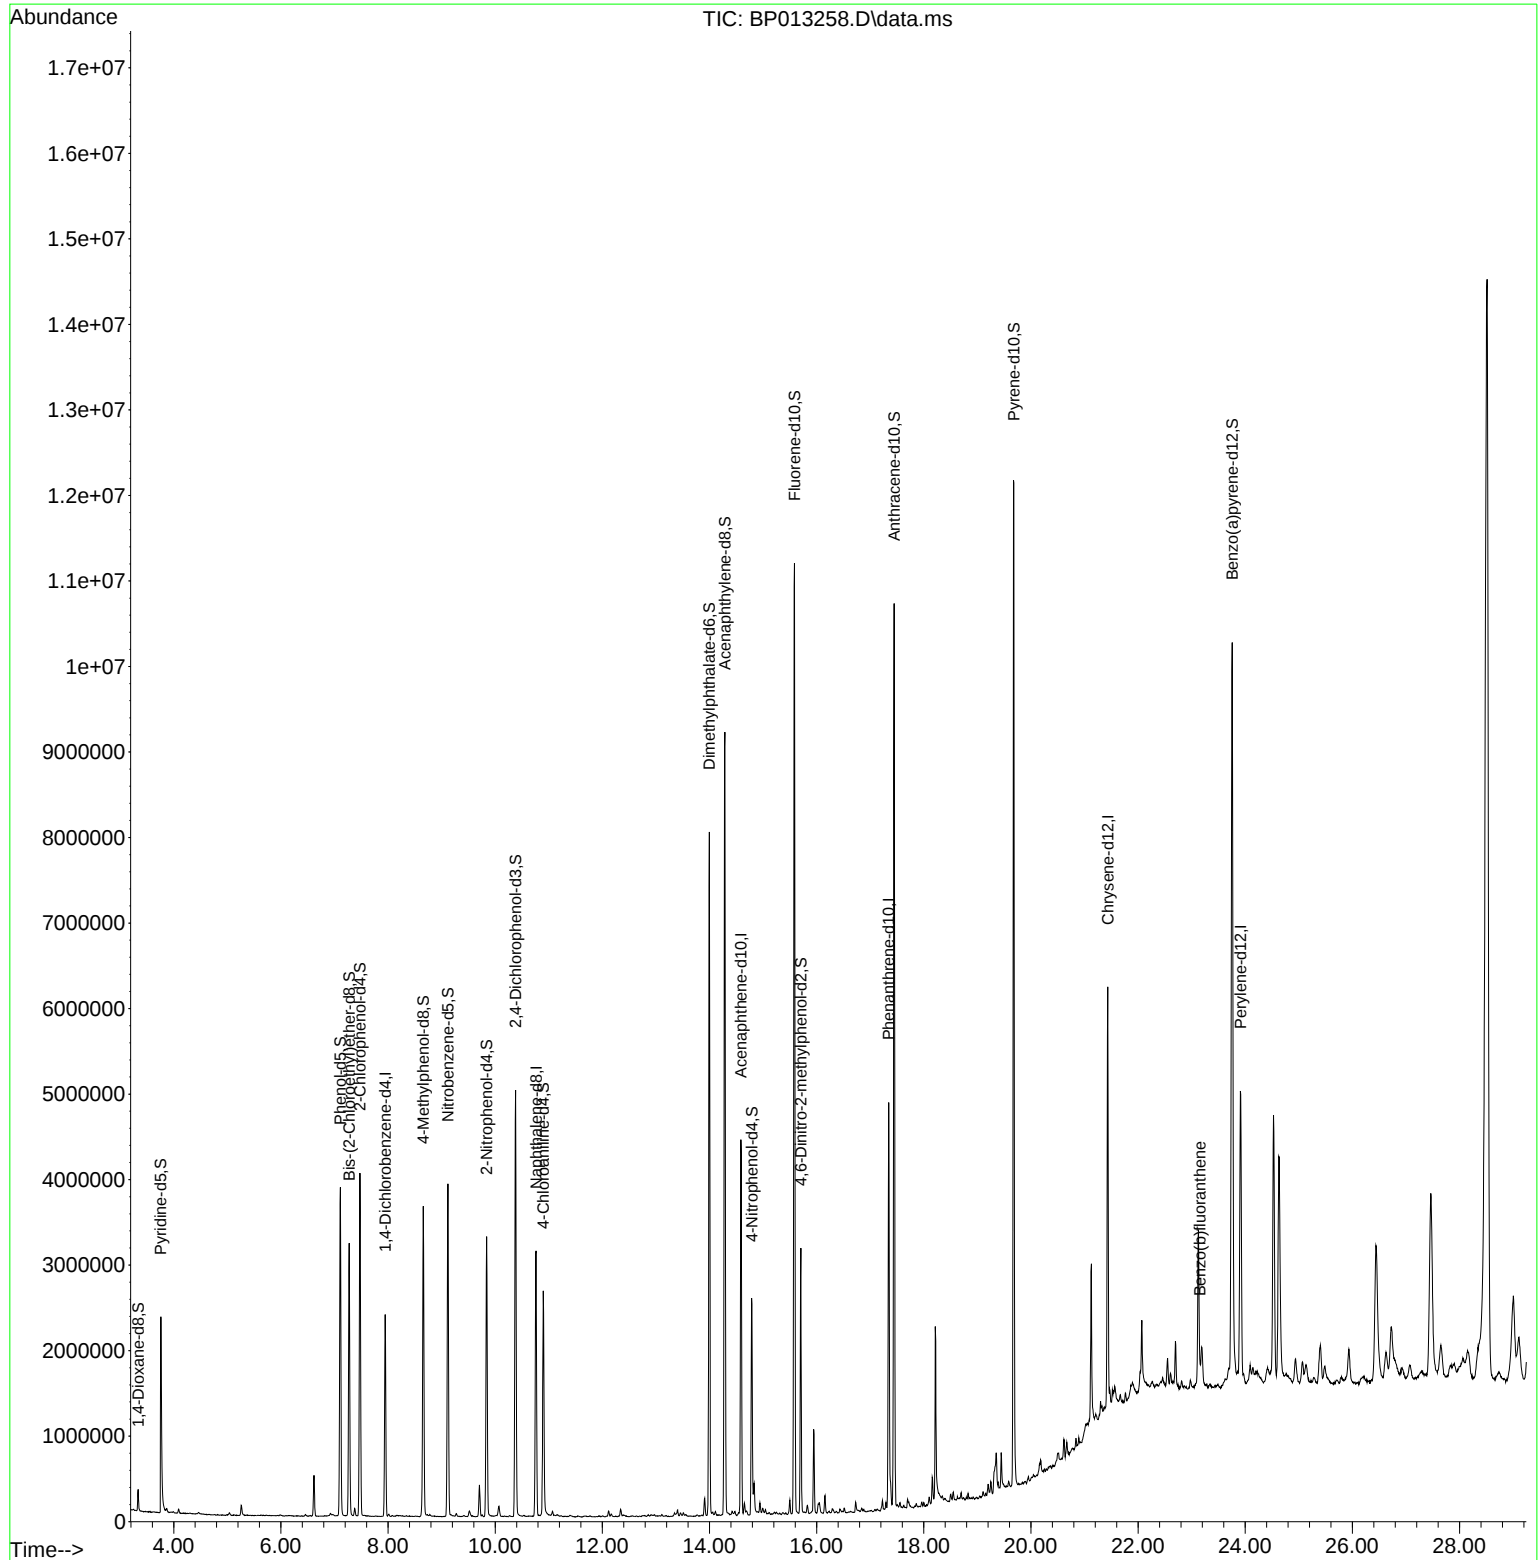

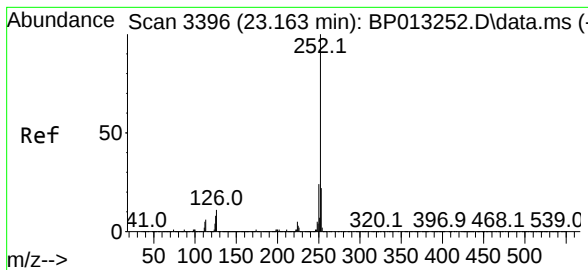

#90

Benzo(b)fluoranthene

Concen: 1.116 ng/ul

RT: 23.151 min Scan# 3394

Delta R.T. -0.012 min

Lab File: BP013258.D


Acq: 22 Dec 2022 23:00

Instrument :

BNA_P

ClientSampleId :

DBXZ8

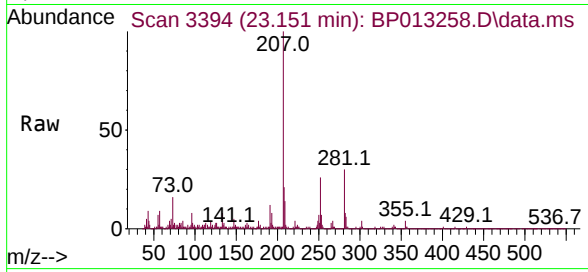

Tgt Ion:252 Resp: 200440

Ion Ratio Lower Upper

252 100

253 25.7 17.7 26.5

125 13.3 6.8 10.2#

