

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013236.D
 Acq On : 22 Dec 2022 09:23
 Operator : CG/JU
 Sample : PB149826BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK826

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	21	25	32	rVB	151419	180563	1.62%	0.172%
2	3.764	95	98	115	rBV	1712733	2574286	23.03%	2.459%
3	4.087	150	153	158	rVB2	29901	45269	0.41%	0.043%
4	7.105	659	666	678	rBV	1862355	2929208	26.21%	2.798%
5	7.275	688	695	706	rVB	1618133	2443437	21.86%	2.334%
6	7.475	722	729	738	rBV	1943887	3002464	26.86%	2.868%
7	7.946	802	809	819	rVB	1431412	2323170	20.78%	2.219%
8	8.658	923	930	939	rBV	2203803	3476406	31.10%	3.321%
9	9.116	999	1008	1017	rBV	1734027	2805123	25.10%	2.680%
10	9.840	1124	1131	1139	rBV	1425055	2266804	20.28%	2.166%
11	10.381	1216	1223	1244	rBV	2161167	3585015	32.07%	3.425%
12	10.763	1280	1288	1298	rBV	1918483	3178193	28.43%	3.036%
13	10.899	1302	1311	1330	rBV	2115056	3620152	32.39%	3.458%
14	12.346	1551	1557	1565	rBV	36455	66715	0.60%	0.064%
15	13.998	1827	1838	1852	rBV	3541319	4847597	43.37%	4.631%
16	14.104	1852	1856	1863	rVB9	6244	13586	0.12%	0.013%
17	14.287	1879	1887	1898	rBV	4013563	5814597	52.02%	5.555%
18	14.592	1931	1939	1946	rBV	2638469	3902708	34.92%	3.728%
19	14.787	1964	1972	1995	rBV	1237862	2201151	19.69%	2.103%
20	15.587	2100	2108	2122	rBV	5077541	7383864	66.06%	7.054%
21	15.704	2122	2128	2143	rVV	1411708	1923257	17.21%	1.837%
22	15.828	2145	2149	2153	rVB3	22524	35952	0.32%	0.034%
23	17.345	2400	2407	2418	rBV	3213739	4612369	41.27%	4.406%
24	17.445	2418	2424	2438	rBV	5608382	8139232	72.82%	7.776%
25	19.257	2728	2732	2736	rBV2	64774	86718	0.78%	0.083%
26	19.322	2739	2743	2752	rBV	65910	117390	1.05%	0.112%
27	19.680	2798	2804	2813	rBV	8068188	10436007	93.37%	9.970%
28	21.433	3097	3102	3111	rBV	4171772	5498025	49.19%	5.253%
29	23.751	3489	3496	3508	rBV2	5458345	11177424	100.00%	10.678%
30	23.916	3517	3524	3539	rVB2	2830261	5987723	53.57%	5.720%




Sum of corrected areas: 104674405

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013236.D
Acq On : 22 Dec 2022 09:23
Operator : CG/JU
Sample : PB149826BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK826

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

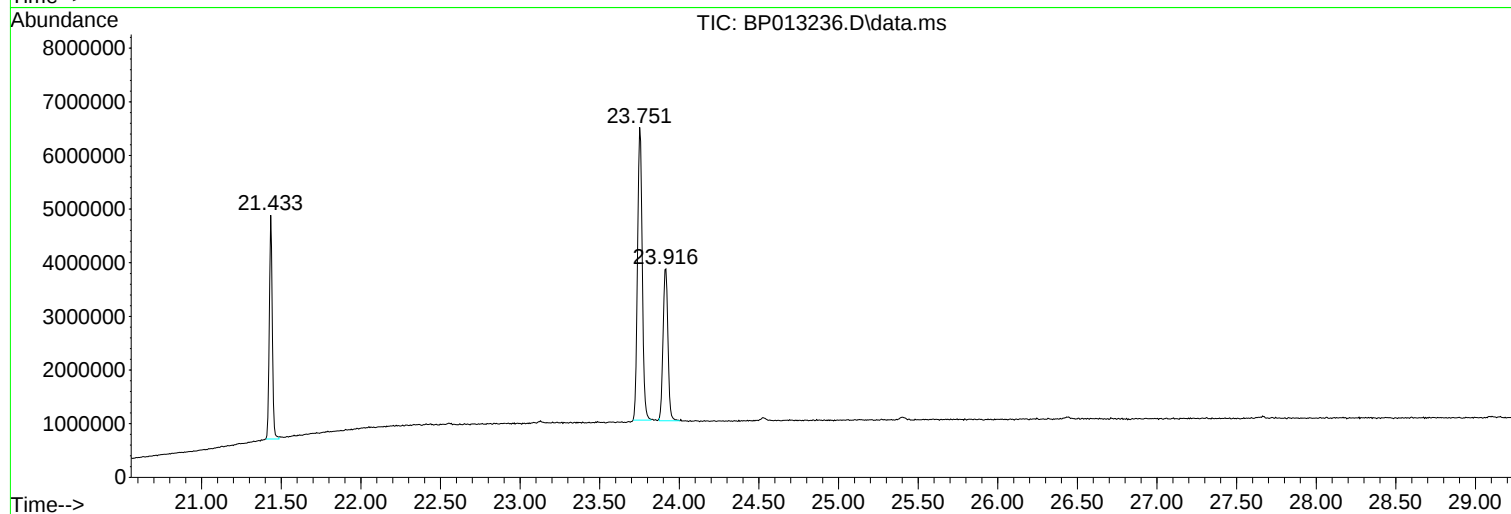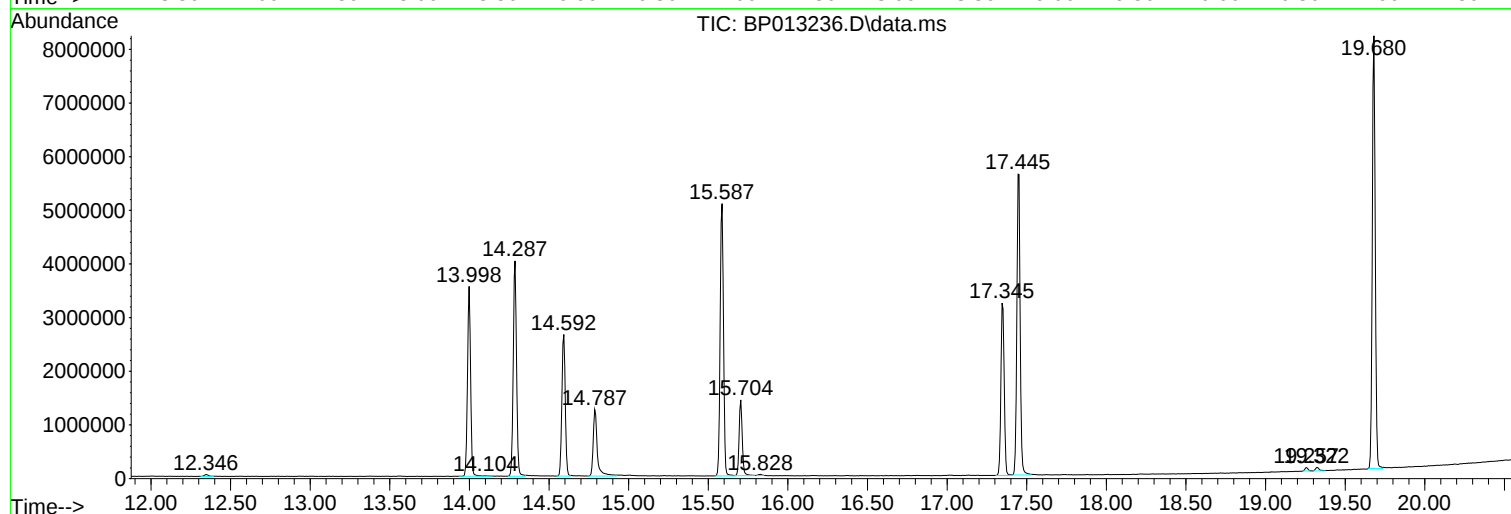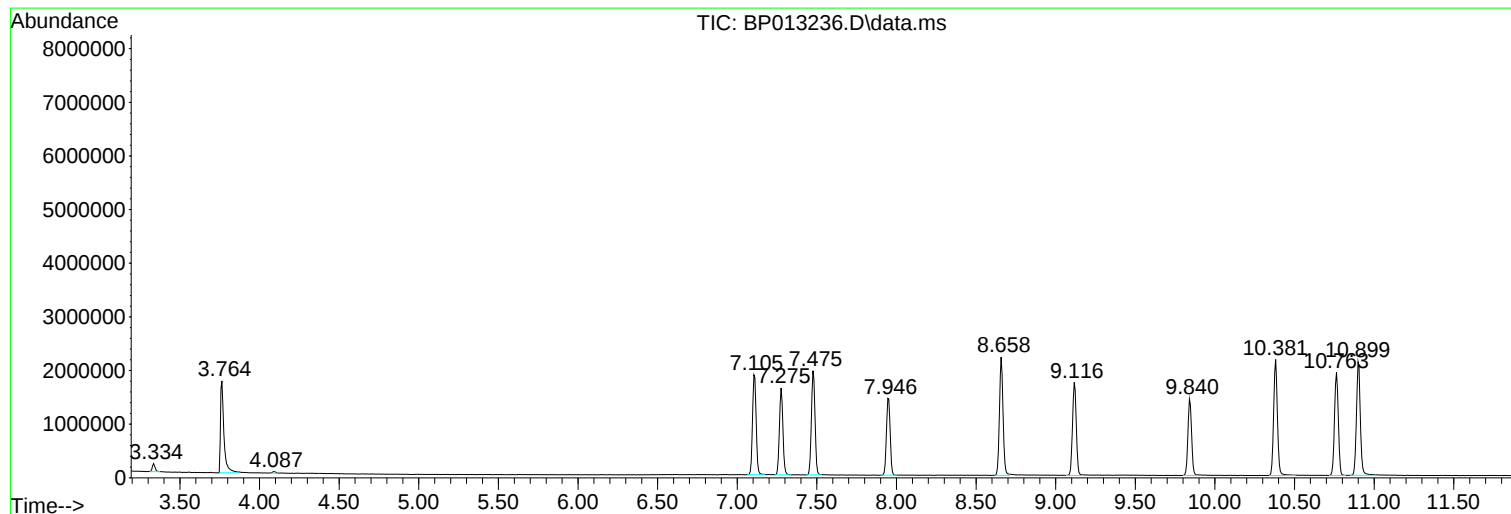

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013236.D
Acq On : 22 Dec 2022 09:23
Operator : CG/JU
Sample : PB149826BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK826

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013236.D
Acq On : 22 Dec 2022 09:23
Operator : CG/JU
Sample : PB149826BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK826

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc