

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013237.D
 Acq On : 22 Dec 2022 09:57
 Operator : CG/JU
 Sample : PB149758TB 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB758

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	21	25	31	rVB	134052	158648	1.84%	0.172%
2	3.764	95	98	116	rBV	1183957	1793030	20.84%	1.949%
3	4.093	150	154	159	rVB	38515	51272	0.60%	0.056%
4	7.105	659	666	680	rVB	1754868	2629672	30.56%	2.858%
5	7.275	688	695	703	rVB	1412071	2168382	25.20%	2.357%
6	7.475	722	729	742	rBV	1744934	2647559	30.77%	2.878%
7	7.946	802	809	816	rBV	1798206	2770488	32.20%	3.012%
8	8.657	920	930	942	rBV	1918440	3138600	36.47%	3.412%
9	9.116	1000	1008	1016	rBV	1515806	2471894	28.73%	2.687%
10	9.840	1122	1131	1145	rBV	1247491	2007708	23.33%	2.182%
11	10.375	1214	1222	1238	rBV	1853583	3164203	36.77%	3.440%
12	10.763	1279	1288	1297	rBV	2261089	3848034	44.72%	4.183%
13	10.898	1303	1311	1325	rBV	1565490	2667035	30.99%	2.899%
14	12.345	1550	1557	1564	rBV2	31059	54124	0.63%	0.059%
15	13.563	1757	1764	1769	rVB10	7412	12451	0.14%	0.014%
16	13.992	1831	1837	1849	rBV	2737259	3956668	45.98%	4.301%
17	14.281	1876	1886	1901	rBV	3294827	4923619	57.22%	5.352%
18	14.587	1931	1938	1948	rBV	3060707	4541632	52.78%	4.937%
19	14.787	1965	1972	1987	rBV	902992	1590054	18.48%	1.728%
20	14.945	1997	1999	2003	rVB4	7445	8637	0.10%	0.009%
21	14.998	2005	2008	2014	rVB8	10841	16542	0.19%	0.018%
22	15.581	2100	2107	2120	rBV	4428389	6153555	71.51%	6.689%
23	15.698	2121	2127	2138	rVV	923292	1298985	15.10%	1.412%
24	15.822	2145	2148	2152	rVB4	17032	25485	0.30%	0.028%
25	16.375	2235	2242	2243	rBV7	8320	12584	0.15%	0.014%
26	17.133	2367	2371	2374	rBV4	8621	13101	0.15%	0.014%
27	17.345	2400	2407	2417	rBV	3594772	4884422	56.76%	5.309%
28	17.445	2418	2424	2445	rVB	4531326	6336274	73.63%	6.888%
29	18.004	2517	2519	2522	rVB4	9954	10019	0.12%	0.011%
30	18.210	2552	2554	2558	rBV5	9095	14078	0.16%	0.015%
31	19.251	2728	2731	2736	rBV4	50374	65932	0.77%	0.072%
32	19.322	2740	2743	2747	rVV	39486	53813	0.63%	0.058%
33	19.675	2797	2803	2815	rBV	5970740	7754804	90.12%	8.430%
34	21.433	3097	3102	3112	rBV	4386749	5795429	67.35%	6.300%
35	23.745	3489	3495	3513	rVB2	4060052	8605253	100.00%	9.354%
36	23.910	3516	3523	3535	rVB	3189469	6351139	73.81%	6.904%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013237.D
Acq On : 22 Dec 2022 09:57
Operator : CG/JU
Sample : PB149758TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB758

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 91995125

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013237.D
Acq On : 22 Dec 2022 09:57
Operator : CG/JU
Sample : PB149758TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB758

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

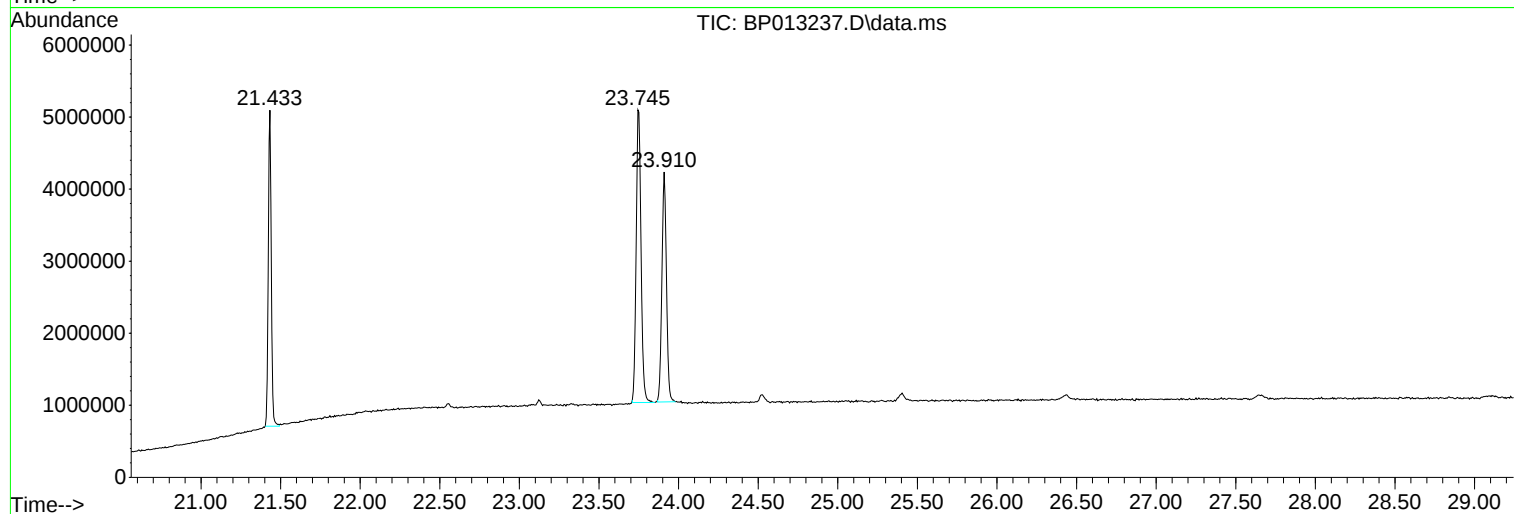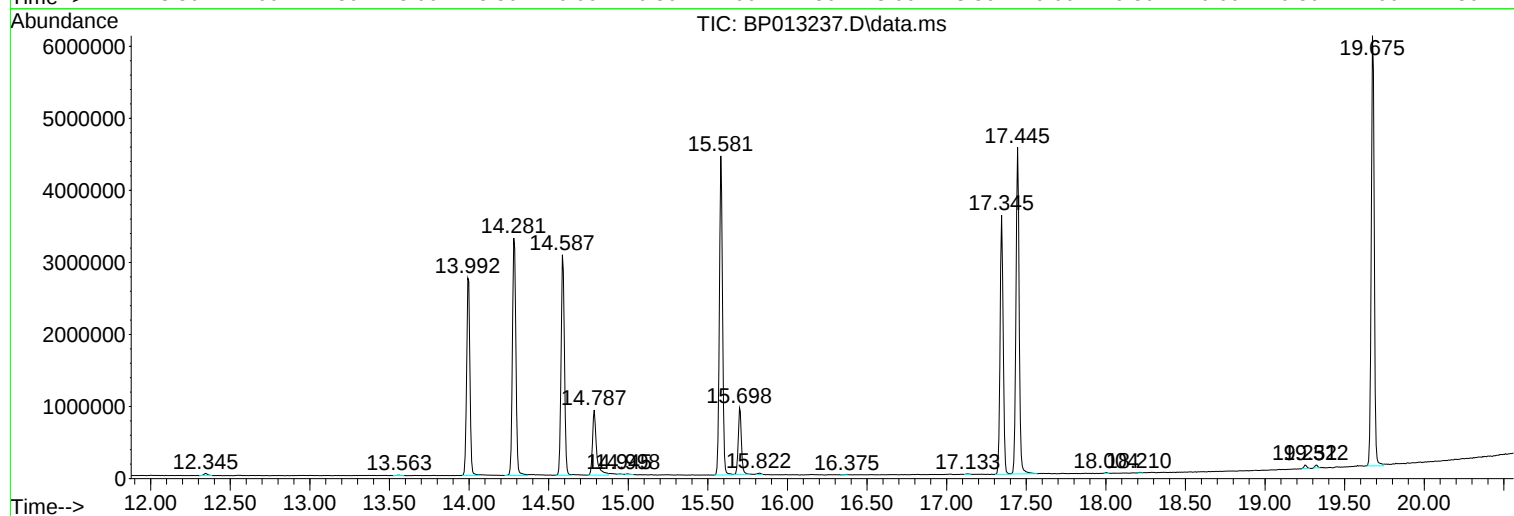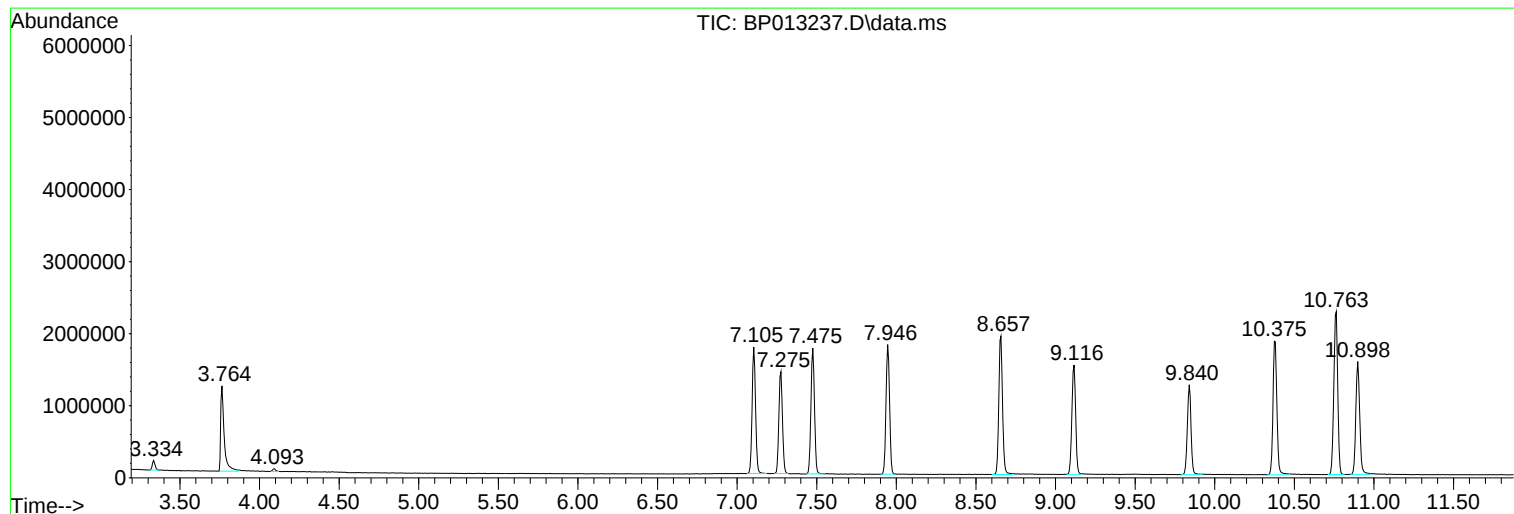

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013237.D
Acq On : 22 Dec 2022 09:57
Operator : CG/JU
Sample : PB149758TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB758

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013237.D
Acq On : 22 Dec 2022 09:57
Operator : CG/JU
Sample : PB149758TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB758

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc