

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013253.D
 Acq On : 22 Dec 2022 20:08
 Operator : CG/JU
 Sample : PB149781BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK781

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	21	25	33	rVB	158951	218764	1.79%	0.142%
2	3.764	94	98	125	rVB	2131557	3360578	27.50%	2.183%
3	4.093	150	154	158	rVB	53018	72555	0.59%	0.047%
4	7.105	659	666	678	rBV	2626222	4148352	33.94%	2.694%
5	7.275	688	695	708	rVB	2101519	3267925	26.74%	2.122%
6	7.475	722	729	744	rBV	2694738	4185973	34.25%	2.719%
7	7.946	802	809	816	rBV	2708520	4142717	33.90%	2.691%
8	8.658	923	930	946	rBV	3329260	5251117	42.97%	3.410%
9	9.116	1000	1008	1022	rBV	2587389	4176607	34.18%	2.713%
10	9.840	1123	1131	1142	rBV	2159621	3560902	29.14%	2.313%
11	10.375	1215	1222	1242	rBV	3225529	5632266	46.09%	3.658%
12	10.763	1279	1288	1300	rBV	3685595	6318832	51.71%	4.104%
13	10.899	1303	1311	1322	rBV	3269863	5517655	45.15%	3.583%
14	12.346	1551	1557	1564	rBV	59477	96082	0.79%	0.062%
15	13.557	1761	1763	1770	rVB7	12193	20769	0.17%	0.013%
16	13.998	1831	1838	1849	rBV	5503612	7869063	64.39%	5.111%
17	14.281	1879	1886	1899	rBV	6738537	9716959	79.51%	6.311%
18	14.587	1931	1938	1950	rBV	5677886	8592994	70.31%	5.581%
19	14.787	1965	1972	1991	rBV	2063936	3335657	27.29%	2.166%
20	14.992	2003	2007	2013	rVB9	15718	34959	0.29%	0.023%
21	15.581	2100	2107	2120	rBV	8359919	11927940	97.60%	7.747%
22	15.698	2121	2127	2141	rVV	2119114	2974852	24.34%	1.932%
23	15.822	2144	2148	2154	rVB2	40092	62391	0.51%	0.041%
24	16.375	2237	2242	2243	rBV5	11217	14878	0.12%	0.010%
25	17.016	2349	2351	2355	rVB4	12386	14833	0.12%	0.010%
26	17.134	2367	2371	2376	rVB2	15694	23001	0.19%	0.015%
27	17.345	2400	2407	2417	rBV	6955018	9728165	79.60%	6.318%
28	17.445	2417	2424	2438	rVV	8589641	12218160	99.98%	7.935%
29	17.998	2515	2518	2522	rBV5	18796	27216	0.22%	0.018%
30	18.210	2552	2554	2557	rBV4	13253	15462	0.13%	0.010%
31	19.251	2727	2731	2737	rBV	101123	145981	1.19%	0.095%
32	19.322	2739	2743	2747	rBV	100858	130476	1.07%	0.085%
33	19.592	2786	2789	2792	rVB3	41693	45405	0.37%	0.029%
34	19.675	2798	2803	2812	rBV	9459340	12220805	100.00%	7.937%
35	20.610	2958	2962	2966	rBV	213605	244981	2.00%	0.159%
36	21.433	3097	3102	3108	rBV	5356149	7041259	57.62%	4.573%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013253.D
Acq On : 22 Dec 2022 20:08
Operator : CG/JU
Sample : PB149781BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK781

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

37	23.751	3489	3496	3509	rVB	5032569	10235091	83.75%	6.647%
38	23.910	3516	3523	3532	rVB2	3594222	7382639	60.41%	4.795%




Sum of corrected areas: 153974261

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013253.D
Acq On : 22 Dec 2022 20:08
Operator : CG/JU
Sample : PB149781BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

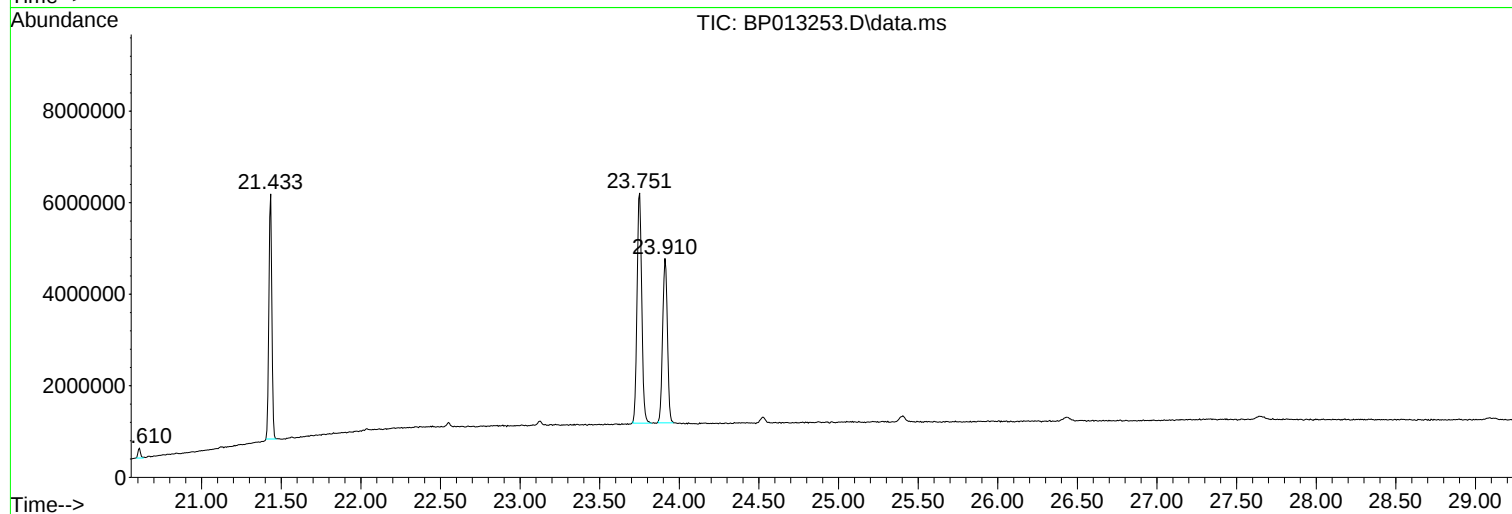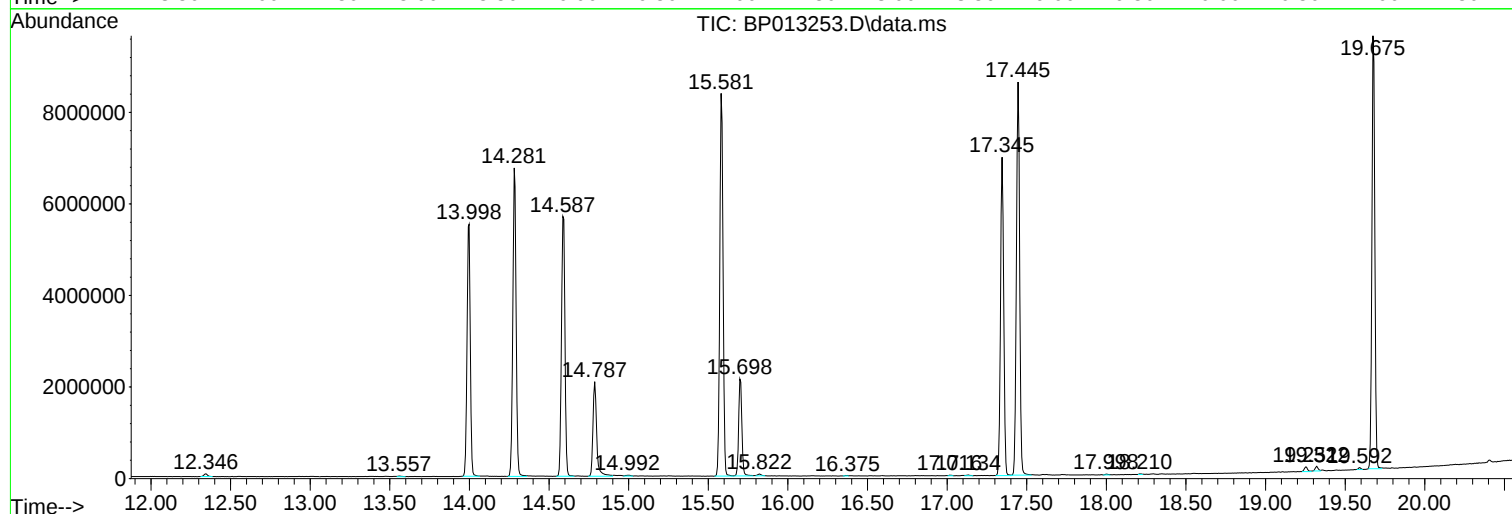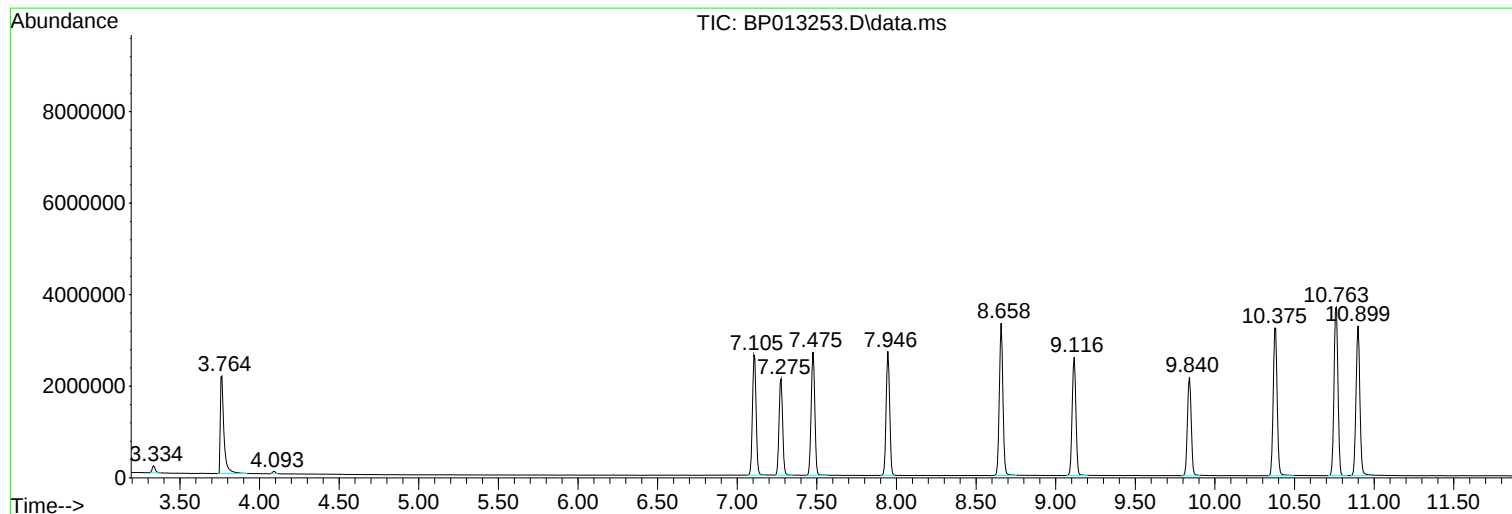

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013253.D
Acq On : 22 Dec 2022 20:08
Operator : CG/JU
Sample : PB149781BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013253.D
Acq On : 22 Dec 2022 20:08
Operator : CG/JU
Sample : PB149781BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc