

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013268.D
 Acq On : 23 Dec 2022 08:31
 Operator : CG/JU
 Sample : PB149784BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK784

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013268.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	22	25	32	rVB	146744	182006	1.60%	0.160%
2	3.763	94	98	120	rBV	1883957	2813140	24.74%	2.475%
3	4.093	150	154	166	rVB	49981	86696	0.76%	0.076%
4	7.110	660	667	681	rVB	2157471	3346811	29.43%	2.944%
5	7.275	689	695	705	rVB	1762031	2653363	23.33%	2.334%
6	7.475	722	729	738	rBV	2182626	3400489	29.91%	2.992%
7	7.951	803	810	818	rBV	1846122	2990598	26.30%	2.631%
8	8.663	921	931	941	rBV	2469251	4030024	35.44%	3.545%
9	9.116	999	1008	1017	rBV	1940165	3204563	28.18%	2.819%
10	9.845	1124	1132	1141	rBV	1614522	2657056	23.37%	2.338%
11	10.387	1216	1224	1233	rBV	2428759	4053715	35.65%	3.566%
12	10.763	1281	1288	1301	rVB	2465438	4202286	36.96%	3.697%
13	10.904	1304	1312	1332	rBV	2313791	3994712	35.13%	3.514%
14	12.351	1552	1558	1566	rVB2	45193	74705	0.66%	0.066%
15	13.833	1805	1810	1813	rBV7	8259	19348	0.17%	0.017%
16	14.004	1832	1839	1849	rVB	3740536	5074745	44.63%	4.465%
17	14.292	1881	1888	1898	rBV	4390862	6278381	55.21%	5.524%
18	14.539	1925	1930	1933	rBV7	7529	13368	0.12%	0.012%
19	14.598	1933	1940	1951	rVB	3338920	4915360	43.23%	4.324%
20	14.798	1968	1974	1994	rBV	1378633	2215278	19.48%	1.949%
21	15.533	2094	2099	2102	rBV6	23139	45439	0.40%	0.040%
22	15.592	2103	2109	2118	rVB	5228423	7399250	65.07%	6.510%
23	15.710	2124	2129	2139	rBV	1084562	1539400	13.54%	1.354%
24	15.833	2146	2150	2154	rVB3	23642	32896	0.29%	0.029%
25	15.992	2173	2177	2184	rVB4	15029	27672	0.24%	0.024%
26	16.286	2223	2227	2233	rVB9	13639	29068	0.26%	0.026%
27	16.374	2238	2242	2246	rBV7	11023	22450	0.20%	0.020%
28	16.516	2261	2266	2273	rVB4	44006	77217	0.68%	0.068%
29	16.598	2276	2280	2283	rBV6	7054	13564	0.12%	0.012%
30	16.733	2301	2303	2309	rVB7	9934	13888	0.12%	0.012%
31	16.810	2311	2316	2324	rBV6	42848	99198	0.87%	0.087%
32	17.039	2352	2355	2360	rBV7	12817	20191	0.18%	0.018%
33	17.092	2362	2364	2368	rVB5	10621	12610	0.11%	0.011%
34	17.133	2369	2371	2376	rVB4	10950	15988	0.14%	0.014%
35	17.357	2402	2409	2417	rBV	3755773	5192130	45.66%	4.568%
36	17.457	2420	2426	2444	rVB	5303609	7536044	66.27%	6.630%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
 Data File : BP013268.D
 Acq On : 23 Dec 2022 08:31
 Operator : CG/JU
 Sample : PB149784BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK784

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	17.616	2447	2453	2455	rBV7	23019	38771	0.34%	0.034%
38	17.739	2471	2474	2482	rVB10	19533	34090	0.30%	0.030%
39	17.839	2487	2491	2495	rBV4	27070	32978	0.29%	0.029%
40	17.892	2495	2500	2502	rBV4	22193	32860	0.29%	0.029%
41	18.016	2518	2521	2525	rVB6	15111	18699	0.16%	0.016%
42	18.174	2544	2548	2552	rBV7	37405	66390	0.58%	0.058%
43	18.227	2552	2557	2566	rVV	157742	234042	2.06%	0.206%
44	18.351	2573	2578	2586	rVB	232772	321122	2.82%	0.283%
45	18.474	2597	2599	2602	rVB4	17735	15201	0.13%	0.013%
46	18.510	2602	2605	2608	rBV3	23295	30713	0.27%	0.027%
47	19.268	2730	2734	2739	rVB2	67544	92840	0.82%	0.082%
48	19.339	2742	2746	2749	rBV	75370	111806	0.98%	0.098%
49	19.692	2801	2806	2811	rBV	7190224	9211820	81.01%	8.104%
50	20.510	2943	2945	2947	rBV3	75420	74370	0.65%	0.065%
51	20.627	2961	2965	2968	rBV	201095	255260	2.24%	0.225%
52	21.451	3100	3105	3111	rVB	4598269	6112969	53.76%	5.378%
53	21.562	3121	3124	3133	rVB4	227077	337822	2.97%	0.297%
54	23.780	3494	3501	3519	rVB	5587606	11370901	100.00%	10.004%
55	23.939	3522	3528	3538	rVB2	3350854	6989876	61.47%	6.149%




Sum of corrected areas: 113666179

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013268.D
Acq On : 23 Dec 2022 08:31
Operator : CG/JU
Sample : PB149784BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

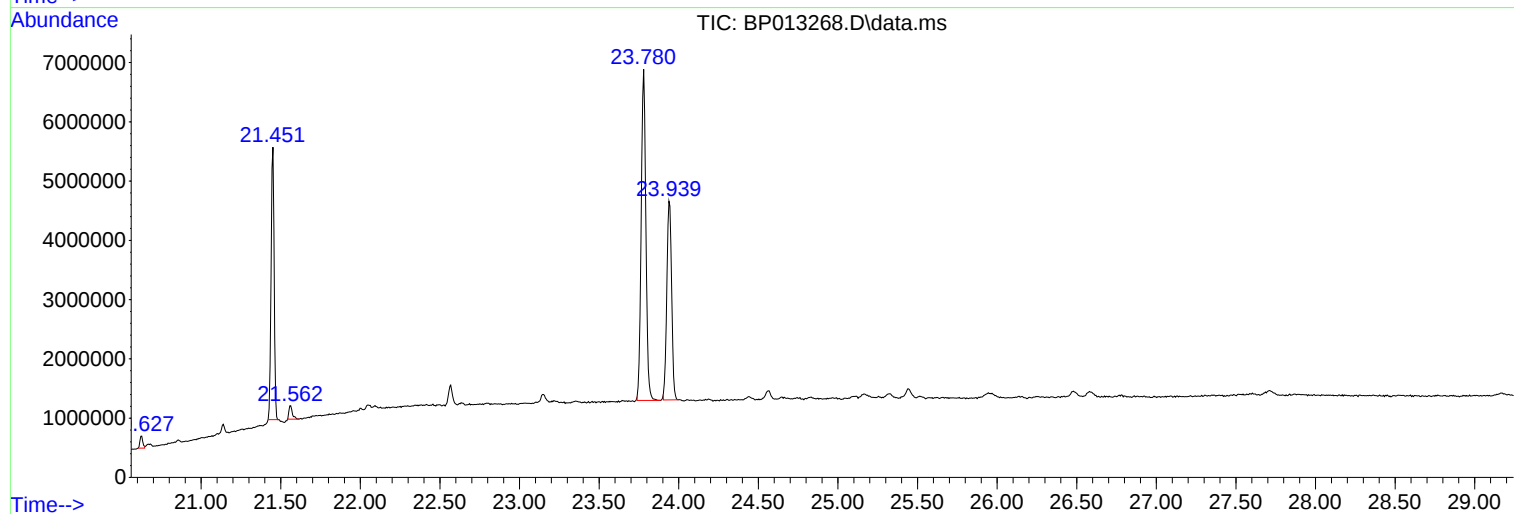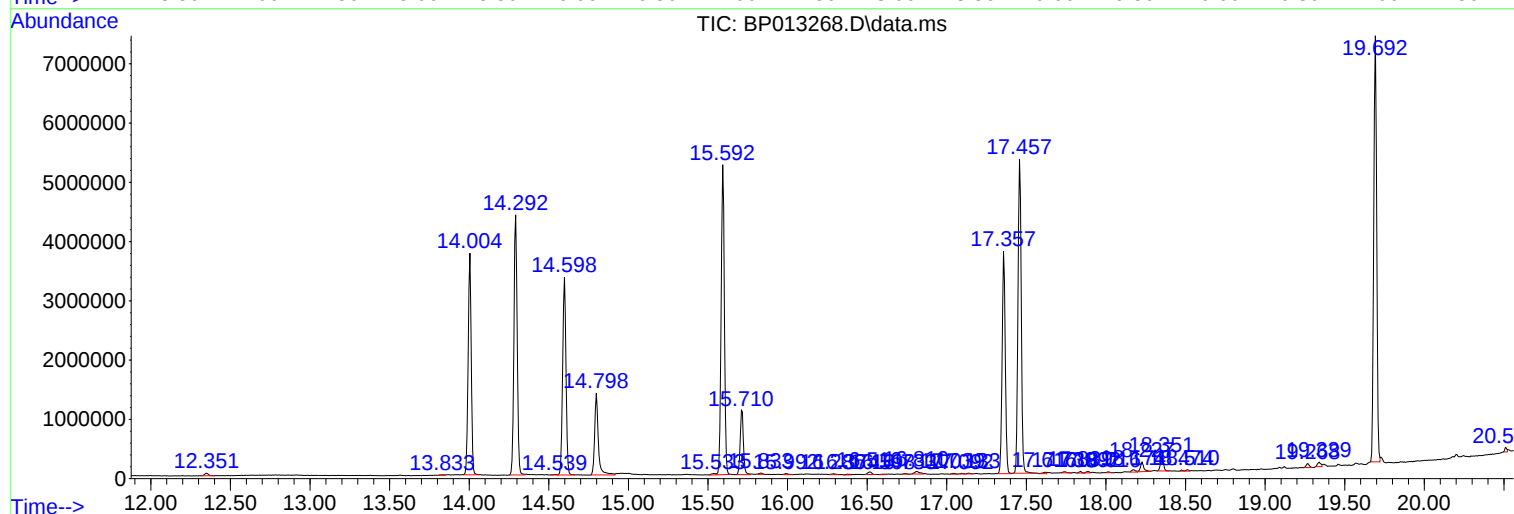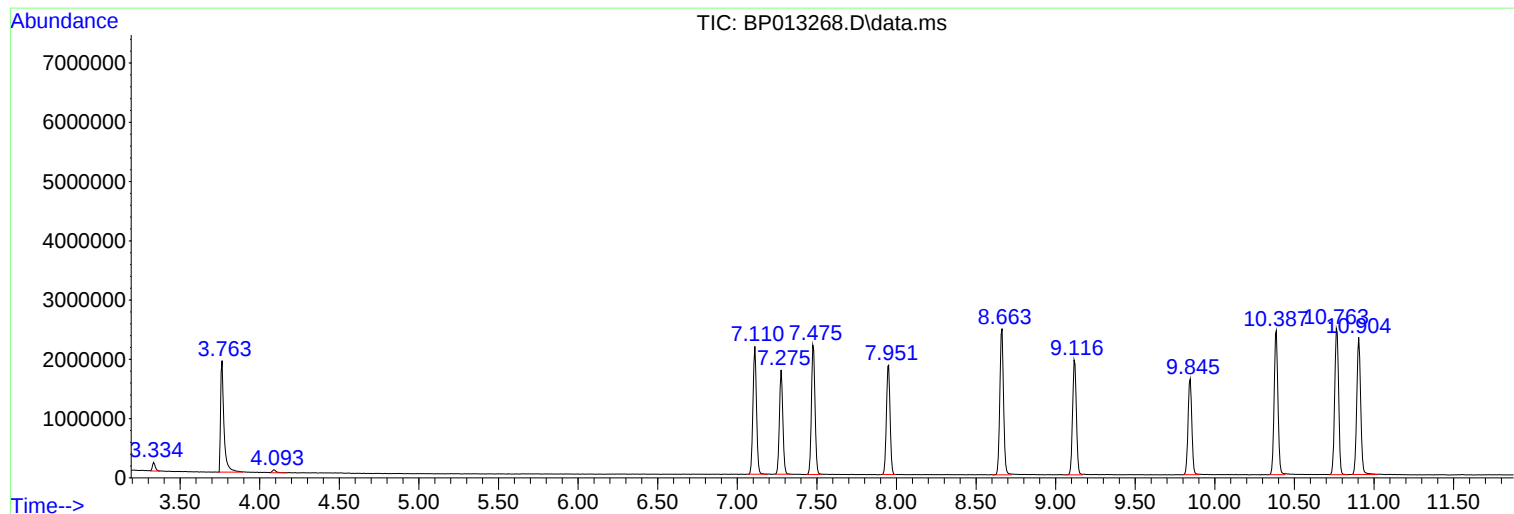

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013268.D
Acq On : 23 Dec 2022 08:31
Operator : CG/JU
Sample : PB149784BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122222\
Data File : BP013268.D
Acq On : 23 Dec 2022 08:31
Operator : CG/JU
Sample : PB149784BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK784

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc