

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122320\
 Data File : BP004422.D
 Acq On : 23 Dec 2020 13:59
 Operator : CG/JU
 Sample : L5059-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CALTANK2-20201209

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	373	379	394	rVB	1746060	2638834	16.21%	4.094%
2	6.999	641	648	663	rVB	1015759	1807302	11.10%	2.804%
3	7.828	783	789	798	rVB	943230	1483127	9.11%	2.301%
4	8.987	978	986	1005	rVB	2949492	4934528	30.31%	7.656%
5	10.622	1257	1264	1275	rBV	1227013	2092074	12.85%	3.246%
6	13.092	1675	1684	1700	rBV	7219879	11212693	68.88%	17.397%
7	13.928	1818	1826	1837	rBV	286068	412012	2.53%	0.639%
8	14.475	1908	1919	1931	rBV	1900514	2823288	17.34%	4.381%
9	15.975	2167	2174	2193	rBV	6120820	8732730	53.65%	13.549%
10	17.239	2381	2389	2400	rBV	2302212	3371908	20.71%	5.232%
11	19.804	2819	2825	2840	rBV	13063630	16278573	100.00%	25.257%
12	21.045	3033	3036	3047	rBV3	82773	192662	1.18%	0.299%
13	21.327	3079	3084	3095	rVV	3231205	4151997	25.51%	6.442%
14	23.692	3478	3486	3500	rVB2	2130052	4319029	26.53%	6.701%




Sum of corrected areas: 64450757

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122320\
Data File : BP004422.D
Acq On : 23 Dec 2020 13:59
Operator : CG/JU
Sample : L5059-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CALTANK2-20201209

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

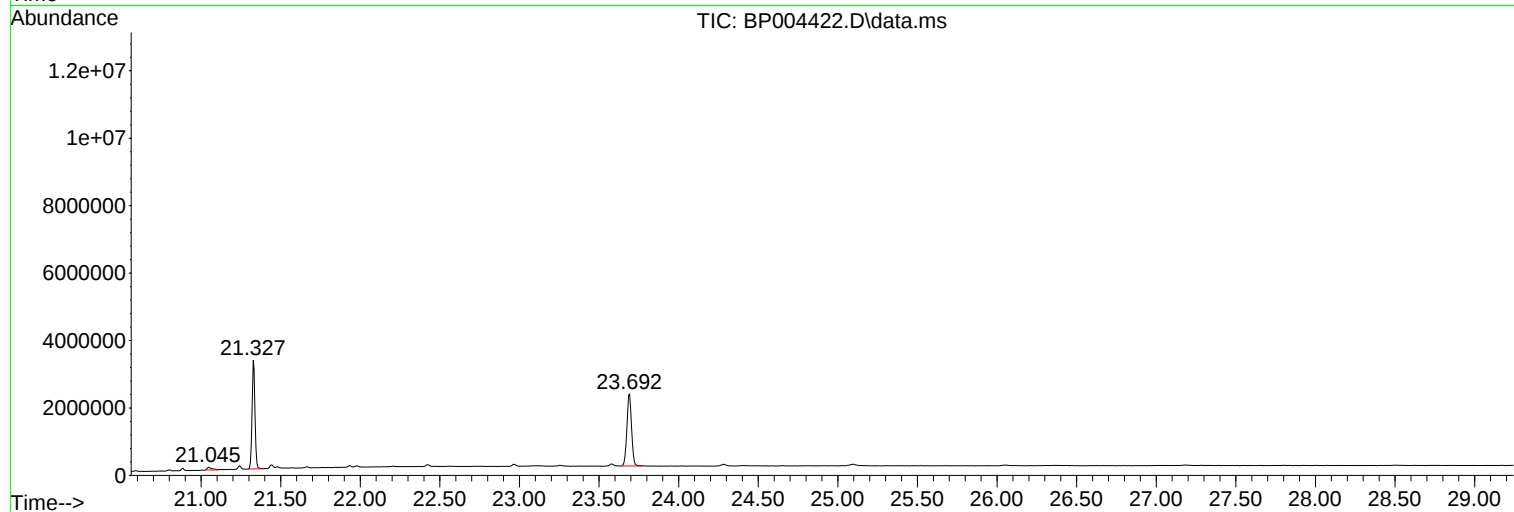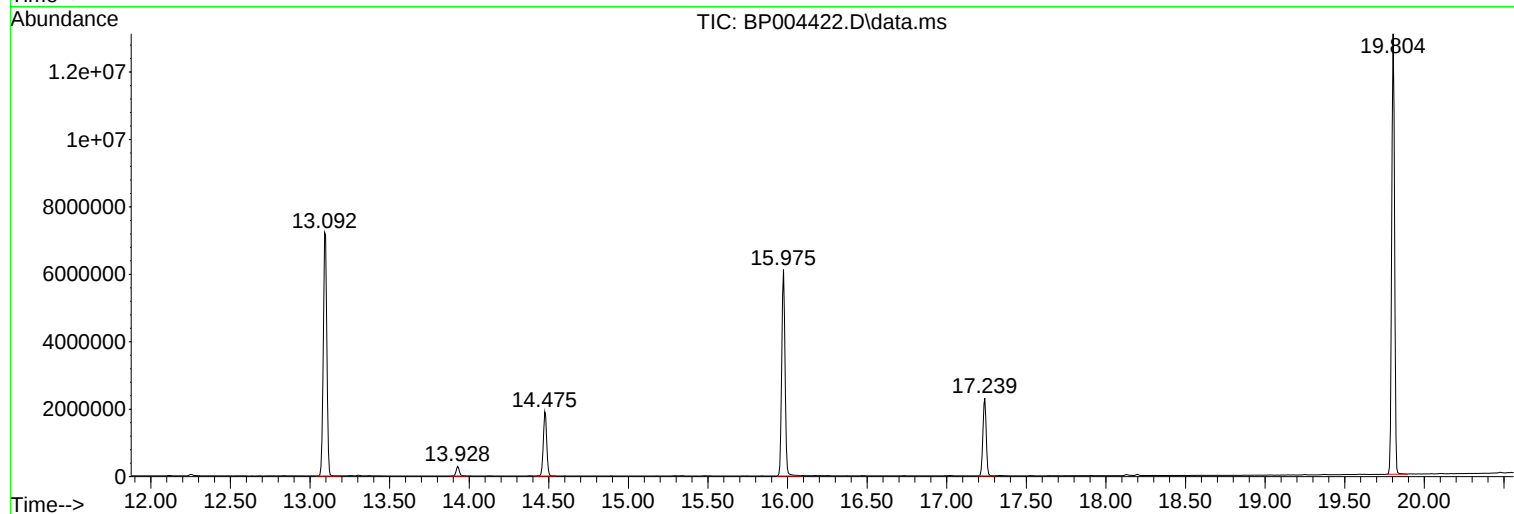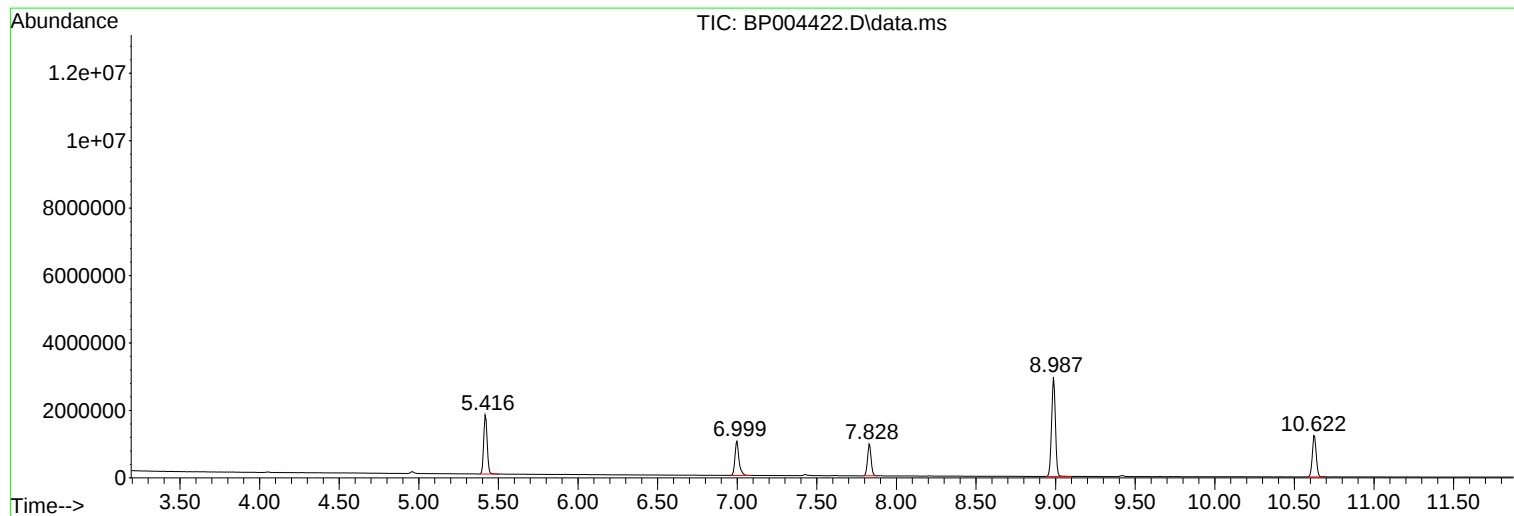

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122320\
Data File : BP004422.D
Acq On : 23 Dec 2020 13:59
Operator : CG/JU
Sample : L5059-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CALTANK2-20201209

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122320\
Data File : BP004422.D
Acq On : 23 Dec 2020 13:59
Operator : CG/JU
Sample : L5059-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CALTANK2-20201209

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc