
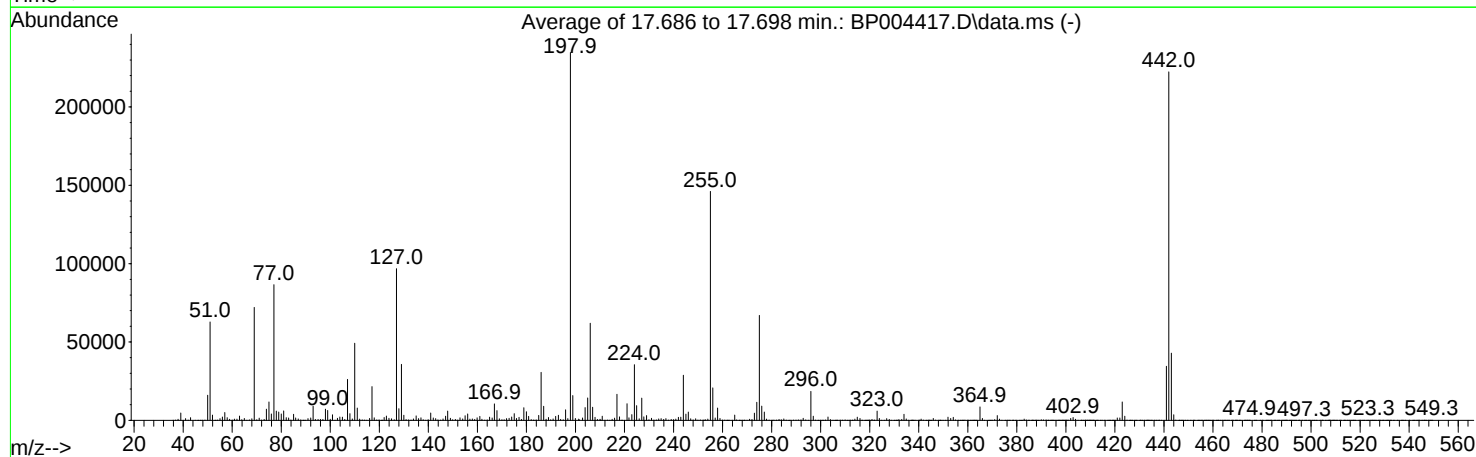


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122320\
 Data File : BP004417.D
 Acq On : 23 Dec 2020 09:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 10:27:21 2020

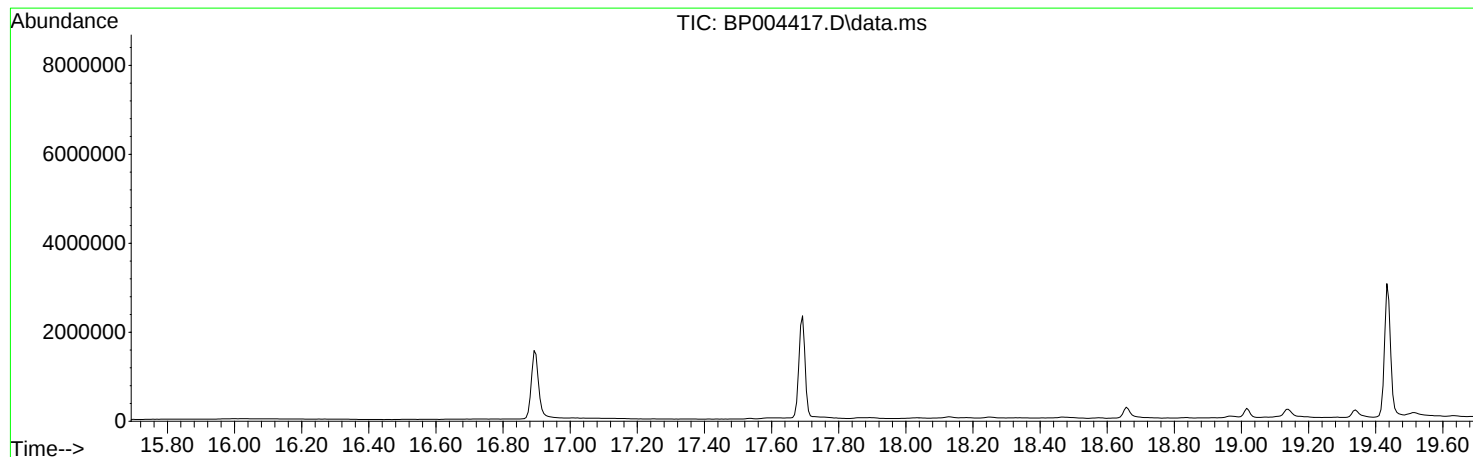

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	62792	PASS
68	69	0.00	2	1.4	1031	PASS
69	198	0.00	100	30.7	72110	PASS
70	69	0.00	2	0.6	402	PASS
127	198	10	80	41.2	96772	PASS
197	198	0.00	2	0.5	1109	PASS
198	198	100	100	100.0	234752	PASS
199	198	5	9	6.7	15814	PASS
275	198	10	60	28.5	66956	PASS
365	198	1	100	3.7	8602	PASS
441	198	0.01	100	14.7	34483	PASS
442	442	100	100	100.0	222411	PASS
443	442	15	24	19.3	42907	PASS