

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122324\
 Data File : BP023562.D
 Acq On : 23 Dec 2024 14:21
 Operator : RC/JU
 Sample : PB165779BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK779

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	23	rVB	31003	43359	1.73%	0.161%
2	3.499	84	87	112	rVV	311512	585769	23.31%	2.181%
3	3.716	122	124	127	rVB3	2737	2768	0.11%	0.010%
4	3.799	134	138	142	rBV2	7504	12351	0.49%	0.046%
5	4.628	274	279	282	rBV6	1472	2612	0.10%	0.010%
6	5.428	412	415	417	rVB4	2750	2555	0.10%	0.010%
7	5.493	422	426	429	rVV6	1937	2960	0.12%	0.011%
8	6.022	514	516	519	rVB4	2806	2545	0.10%	0.009%
9	6.652	618	623	624	rBV5	2259	3410	0.14%	0.013%
10	6.746	631	639	655	rBV	278754	676918	26.94%	2.520%
11	6.875	655	661	672	rVB	312951	514265	20.46%	1.914%
12	6.987	679	680	684	rVB4	2674	2760	0.11%	0.010%
13	7.075	689	695	707	rBV	392070	668552	26.60%	2.489%
14	7.522	764	771	785	rBV	395640	734000	29.21%	2.732%
15	8.257	888	896	918	rBV	340970	818808	32.58%	3.048%
16	8.581	947	951	953	rBV5	2798	3277	0.13%	0.012%
17	8.675	960	967	981	rBV	311156	606873	24.15%	2.259%
18	9.387	1081	1088	1103	rBV	266418	516231	20.54%	1.922%
19	9.740	1144	1148	1151	rVV6	1607	2931	0.12%	0.011%
20	9.763	1151	1152	1156	rVV4	2296	2520	0.10%	0.009%
21	9.940	1174	1182	1209	rBV	306840	827227	32.92%	3.079%
22	10.275	1230	1239	1253	rBV	500482	954524	37.98%	3.553%
23	10.440	1260	1267	1285	rBV	272879	692792	27.57%	2.579%
24	11.087	1372	1377	1379	rBV6	2121	2680	0.11%	0.010%
25	11.881	1506	1512	1515	rBV5	6431	11618	0.46%	0.043%
26	12.440	1602	1607	1612	rBV8	4567	10119	0.40%	0.038%
27	12.604	1632	1635	1638	rBV5	1760	2535	0.10%	0.009%
28	12.869	1675	1680	1682	rBV5	2693	4573	0.18%	0.017%
29	13.128	1717	1724	1725	rBV7	3064	4328	0.17%	0.016%
30	13.163	1727	1730	1732	rVV3	2524	2812	0.11%	0.010%
31	13.198	1732	1736	1739	rVB6	1888	2683	0.11%	0.010%
32	13.522	1786	1791	1792	rBV4	8042	10906	0.43%	0.041%
33	13.569	1792	1799	1809	rVB	783813	1141703	45.43%	4.250%
34	13.851	1839	1847	1856	rBV	794473	1340591	53.35%	4.990%
35	14.075	1878	1885	1891	rBV6	6920	21041	0.84%	0.078%
36	14.163	1892	1900	1908	rVV	773560	1280485	50.95%	4.767%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122324\
 Data File : BP023562.D
 Acq On : 23 Dec 2024 14:21
 Operator : RC/JU
 Sample : PB165779BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK779

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

37	14.322	1925	1927	1934	rVB8	6414	10494	0.42%	0.039%
38	14.487	1950	1955	1967	rBV	124255	382216	15.21%	1.423%
39	14.757	1997	2001	2007	rVB3	14082	24224	0.96%	0.090%
40	15.163	2063	2070	2085	rBV	1022374	1710436	68.06%	6.367%
41	15.345	2095	2101	2117	rBV	239459	503019	20.02%	1.873%
42	15.592	2140	2143	2148	rBV7	2723	4009	0.16%	0.015%
43	15.686	2155	2159	2162	rBV5	3088	4568	0.18%	0.017%
44	15.745	2167	2169	2172	rVB4	3389	3454	0.14%	0.013%
45	15.781	2172	2175	2178	rBV5	1779	2553	0.10%	0.010%
46	15.975	2204	2208	2209	rBV4	4621	5590	0.22%	0.021%
47	16.004	2209	2213	2223	rVB6	12170	25332	1.01%	0.094%
48	16.298	2259	2263	2266	rBV6	4333	5299	0.21%	0.020%
49	16.386	2275	2278	2280	rBV4	2802	2660	0.11%	0.010%
50	16.545	2300	2305	2307	rBV6	4233	6111	0.24%	0.023%
51	16.751	2334	2340	2346	rBV4	7581	16923	0.67%	0.063%
52	16.963	2369	2376	2386	rBV	1036882	1607752	63.98%	5.985%
53	17.075	2388	2395	2409	rVV2	1103612	1868091	74.34%	6.954%
54	17.310	2434	2435	2439	rBV4	3360	4864	0.19%	0.018%
55	17.386	2447	2448	2451	rBV3	3077	2730	0.11%	0.010%
56	17.657	2491	2494	2496	rBV3	3800	4971	0.20%	0.019%
57	17.904	2531	2536	2545	rBV4	38150	76294	3.04%	0.284%
58	18.280	2598	2600	2606	rBV7	4756	6037	0.24%	0.022%
59	18.992	2718	2721	2726	rVB4	15560	22433	0.89%	0.084%
60	19.080	2732	2736	2740	rBV2	13216	22702	0.90%	0.085%
61	19.451	2793	2799	2813	rBV	1353828	2386363	94.96%	8.883%
62	21.404	3125	3131	3142	rBV	1104175	1905312	75.82%	7.093%
63	24.368	3627	3635	3649	rVB	936672	2513008	100.00%	9.355%
64	24.580	3663	3671	3689	rVB	742302	2219762	88.33%	8.263%



Sum of corrected areas: 26863288

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122324\
Data File : BP023562.D
Acq On : 23 Dec 2024 14:21
Operator : RC/JU
Sample : PB165779BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

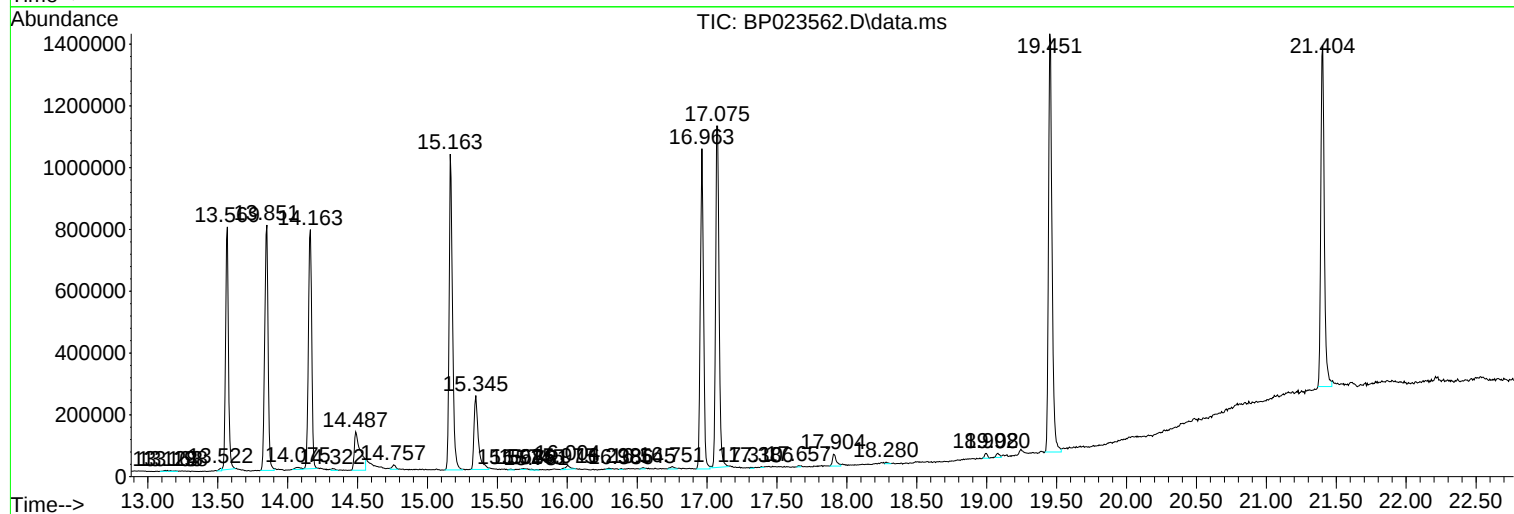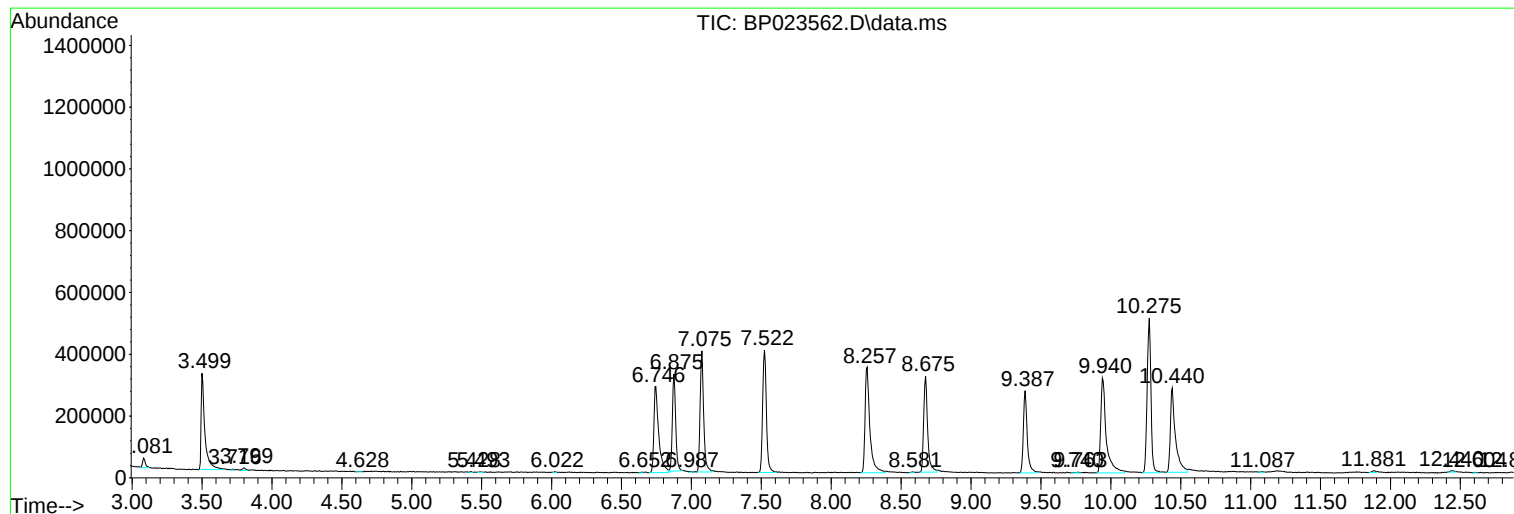

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122324\
Data File : BP023562.D
Acq On : 23 Dec 2024 14:21
Operator : RC/JU
Sample : PB165779BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122324\
Data File : BP023562.D
Acq On : 23 Dec 2024 14:21
Operator : RC/JU
Sample : PB165779BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc