
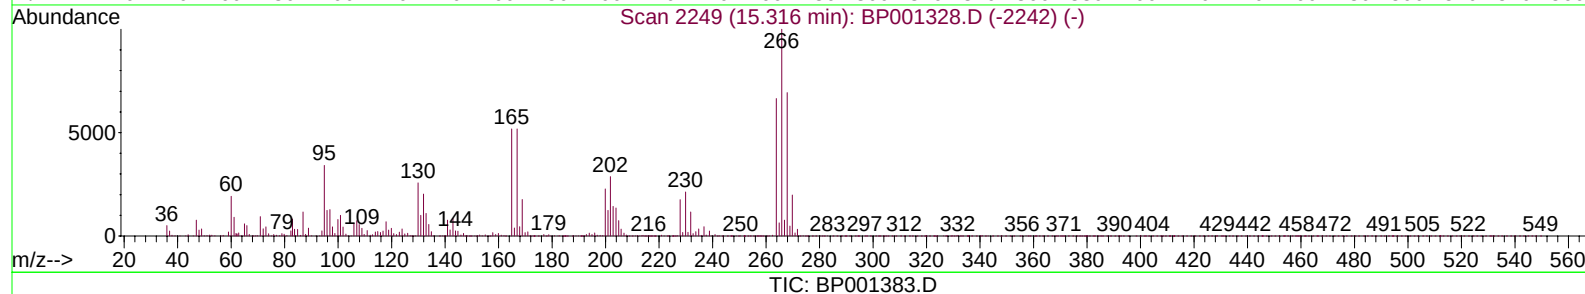
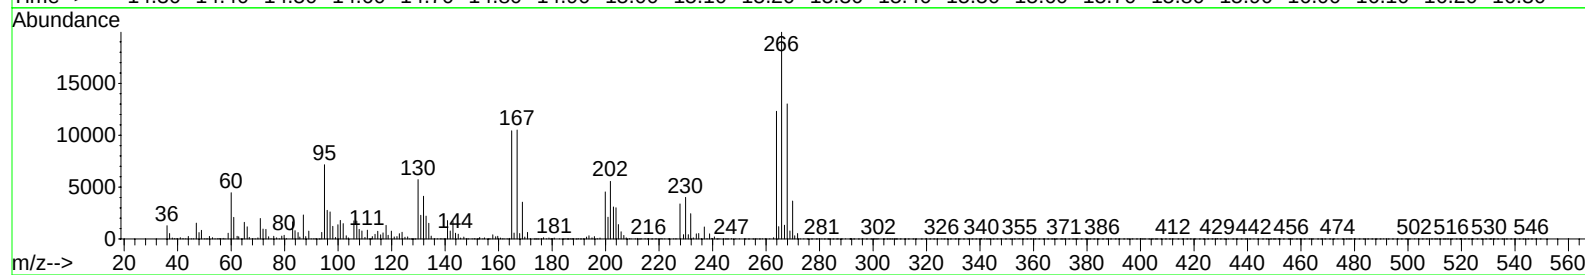


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122419\
Data File : BP001383.D
Acq On : 24 Dec 2019 13:21
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 18:00:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 16:04:49 2019
Response via : Initial Calibration

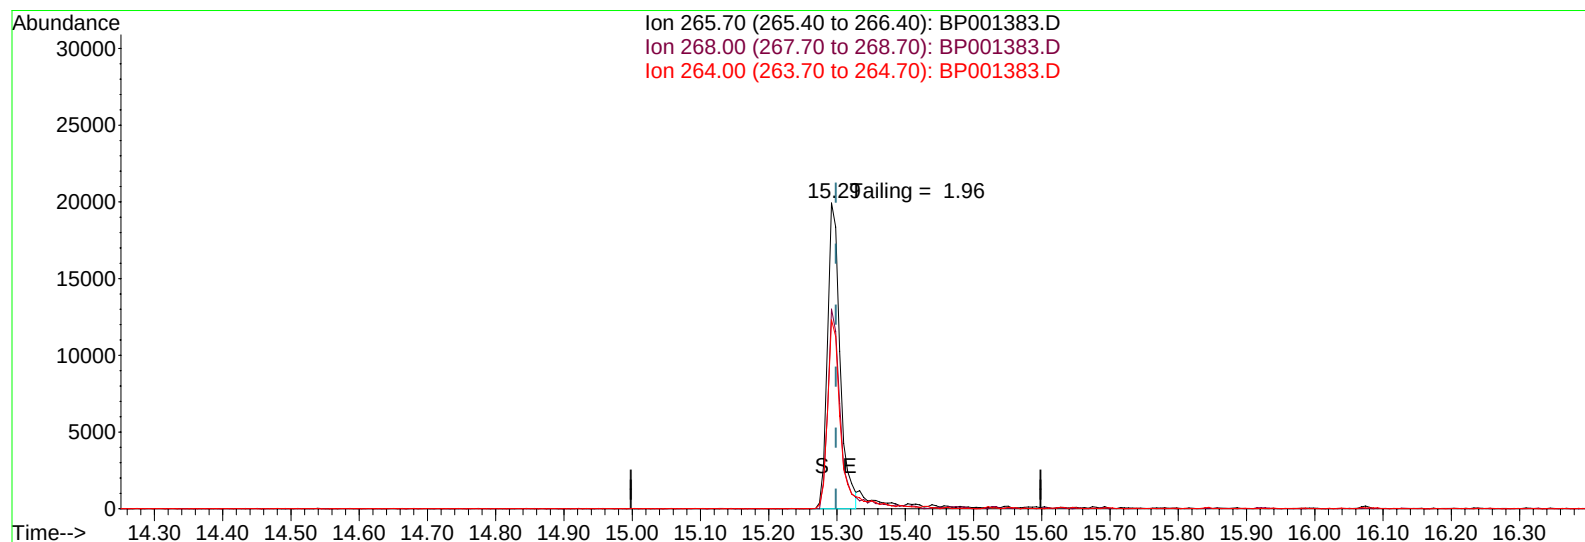

(70) Pentachlorophenol (C)




15.292min (-0.006) 36174.37ng

response 27466

Ion	Exp%	Act%
265.70	100	100
268.00	71.20	65.32
264.00	63.50	67.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP122419\
 Data File : BP001383.D
 Acq On : 24 Dec 2019 13:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 18:00:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP121919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 16:04:49 2019
 Response via : Initial Calibration

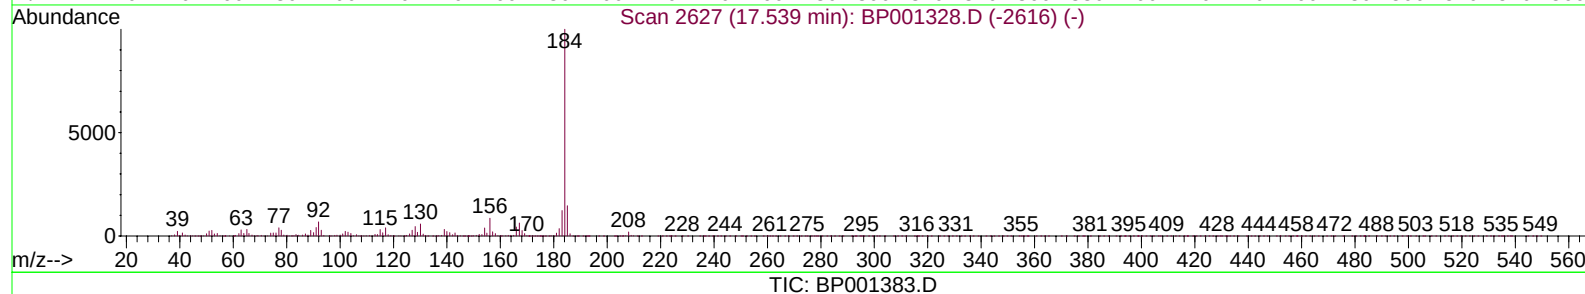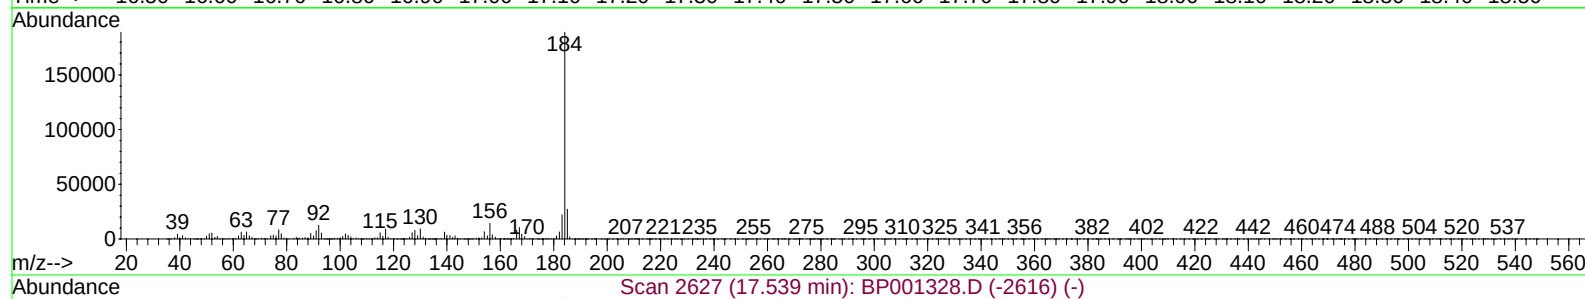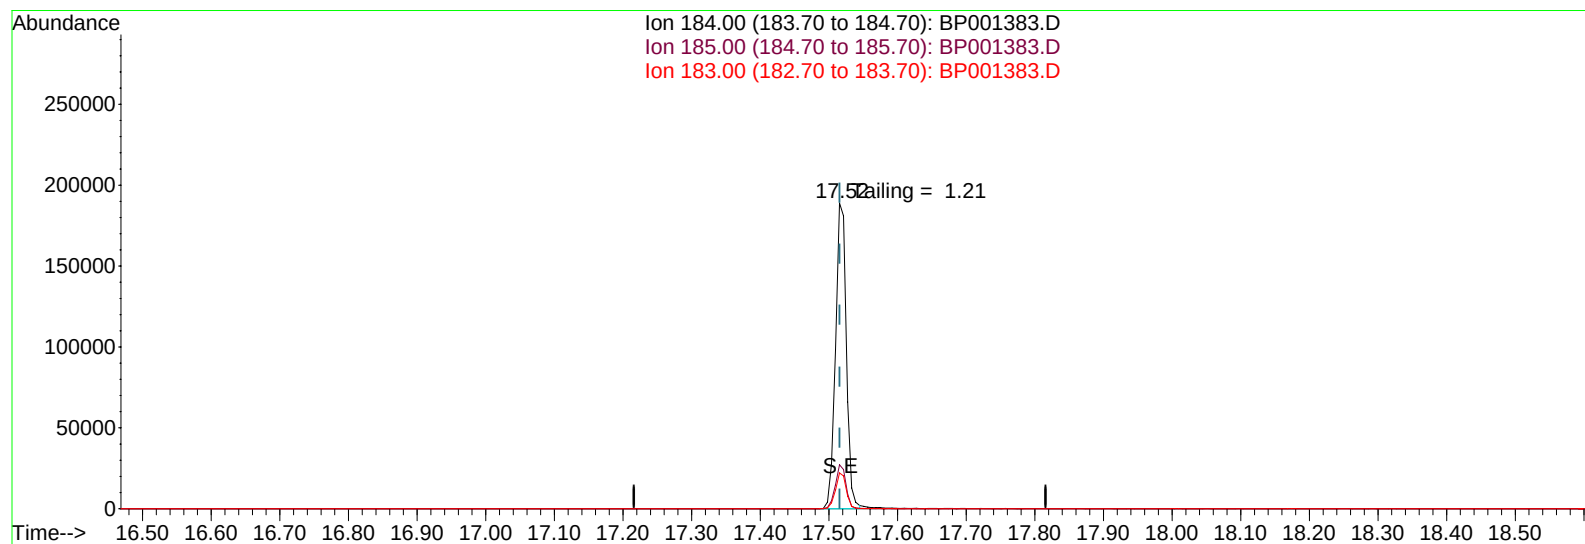

(77) Benzidine

17.515min (-0.000) 82478.26ng

response 208919

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.42
183.00	12.00	11.70
0.00	0.00	0.00